


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL011619\
 Data File : VL033086.D
 Acq On : 16 Jan 2019 8:57
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL010419AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Jan 04 16:09:05 2019
 Last Update : Fri Jan 04 16:09:05 2019

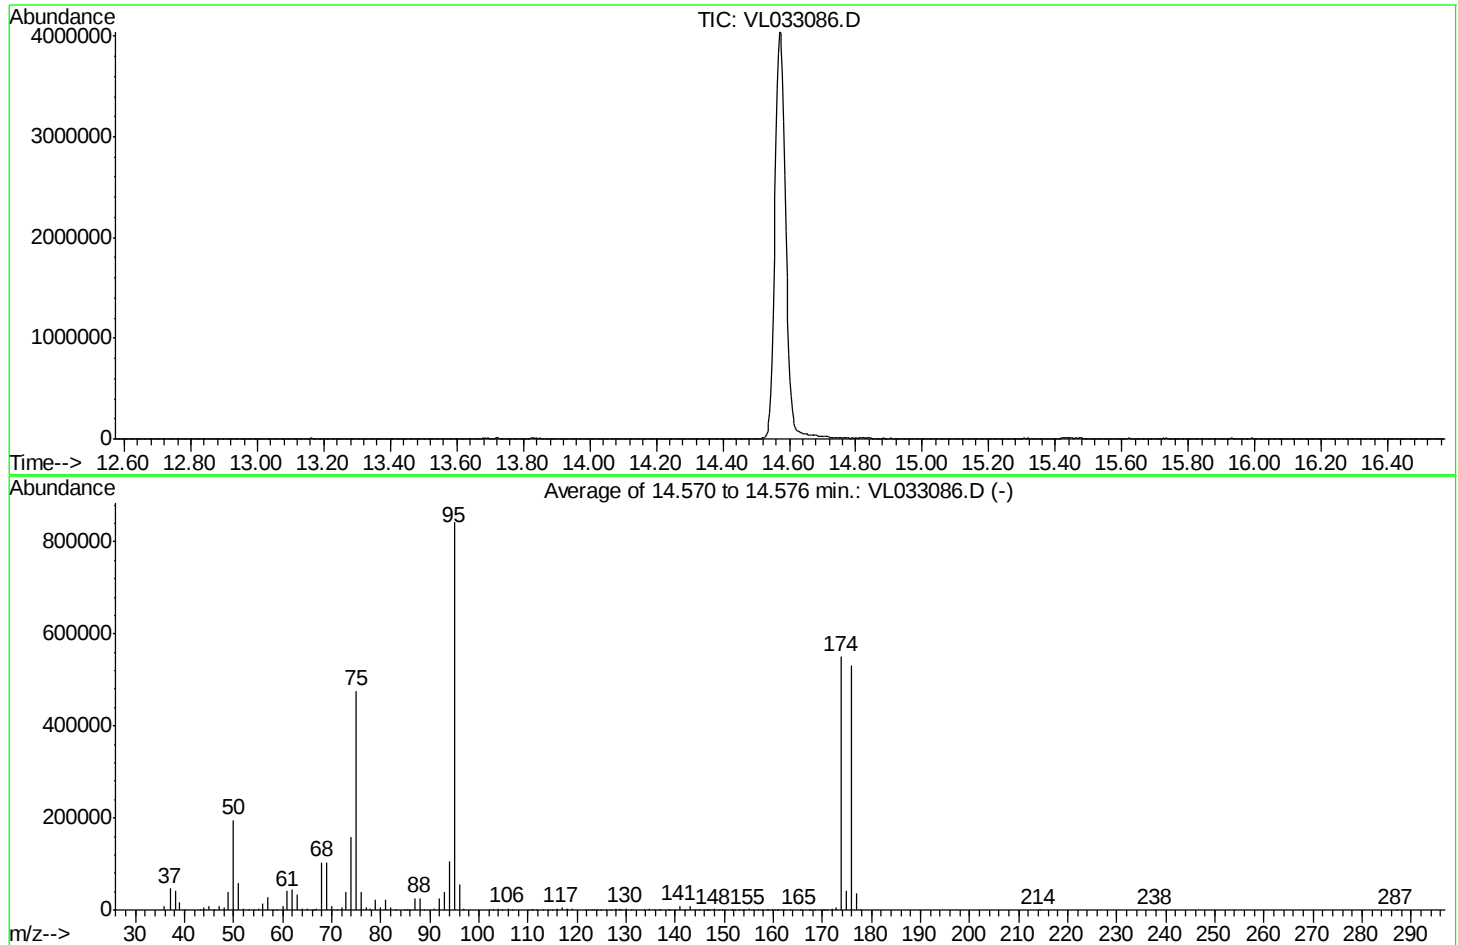

AutoFind: Scans 3618, 3619, 3620; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.2	195349	PASS
75	95	30	66	56.5	475733	PASS
95	95	100	100	100.0	842368	PASS
96	95	5	9	6.6	55925	PASS
173	174	0.00	2	1.1	6270	PASS
174	95	50	120	65.2	549504	PASS
175	174	4	9	7.7	42066	PASS
176	174	93	101	96.6	530986	PASS
177	176	5	9	7.0	37018	PASS