
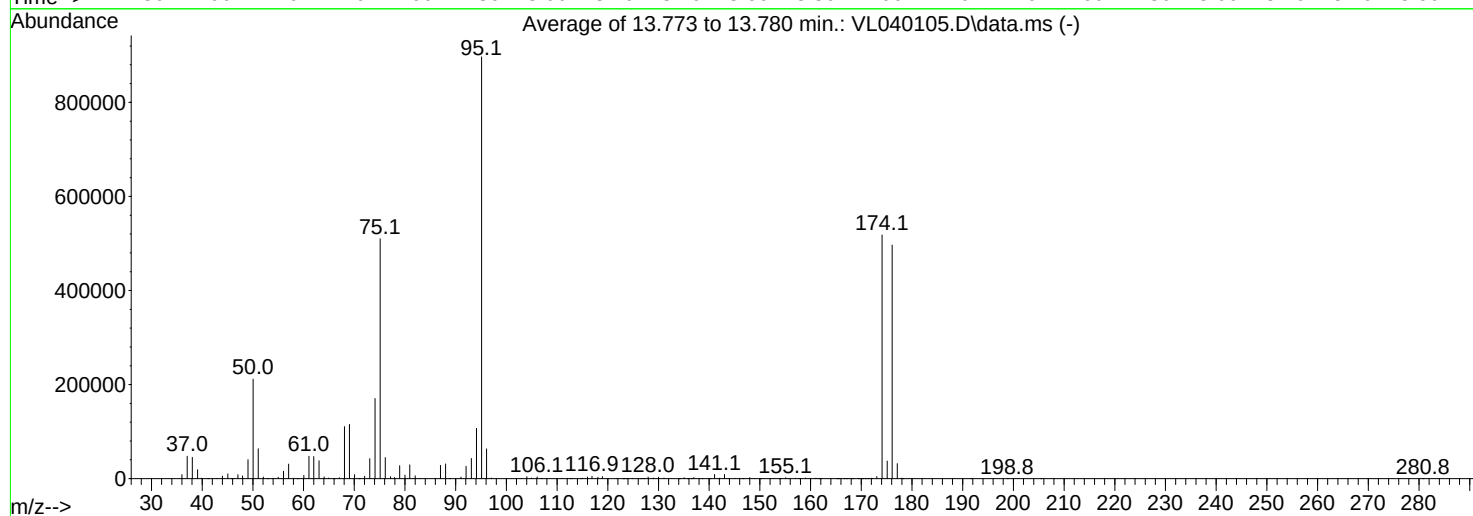


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011923\
 Data File : VL040105.D
 Acq On : 19 Jan 2023 9:25
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011623AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Mon Jan 16 14:40:47 2023

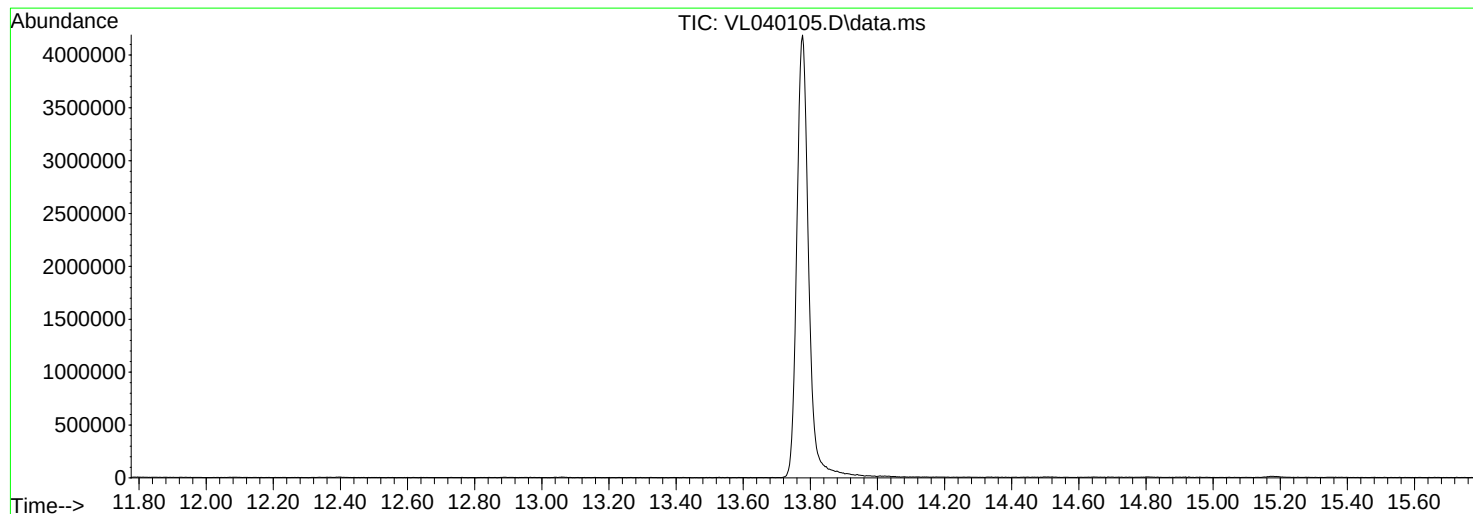

AutoFind: Scans 3474, 3475, 3476; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.6	211712	PASS
75	95	30	66	56.8	509803	PASS
95	95	100	100	100.0	896768	PASS
96	95	5	9	7.0	63147	PASS
173	174	0.00	2	0.9	4445	PASS
174	95	50	120	57.8	518080	PASS
175	174	4	9	7.2	37499	PASS
176	174	93	101	95.9	496640	PASS
177	176	5	9	6.5	32104	PASS

Average of 13.773 to 13.780 min.: VL040105.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	8423	47.05	8478	58.05	1071	69.05	11541
37.05	47592	47.95	5714	58.75	172	70.05	857
38.05	45304	49.05	40587	60.05	7158	70.90	15
39.10	18952	50.05	211712	61.05	47768	71.20	24
39.90	1183	51.05	63637	62.00	46861	72.05	4993
41.10	112	52.05	3560	63.05	38192	73.05	42507
42.90	580	52.90	59	64.05	3758	74.10	170368
44.00	5555	54.00	197	64.95	1348	75.10	509803
45.05	10180	55.00	3190	66.00	64	76.10	44971
45.80	61	56.05	15834	67.05	1939	77.15	4280
46.25	828	57.05	31157	68.05	110533	77.95	2517

Average of 13.773 to 13.780 min.: VL040105.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	27632	93.10	43011	109.90	584	120.00	198
80.00	7581	94.10	106912	110.95	801	121.75	233
80.95	29131	95.10	896768	112.00	845	123.00	189
82.00	6164	96.10	63147	112.60	170	123.20	56
82.95	837	97.05	1515	113.05	792	123.70	141
85.95	1126	102.95	599	114.60	129	123.95	301
87.00	28408	104.05	3938	115.05	910	124.85	298
88.00	31453	104.95	1220	116.00	3563	126.05	390
88.80	177	106.05	3650	116.90	5046	126.50	128
91.05	3382	106.85	328	118.05	3150	127.10	176
92.05	26349	107.10	245	118.95	4460	127.95	3410

Average of 13.773 to 13.780 min.: VL040105.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
129.00	1266	140.20	143	148.95	428	158.10	270
130.00	3181	141.05	8923	149.85	617	159.00	1314
131.10	1249	141.80	198	150.20	78	160.80	209
133.90	63	142.10	1012	152.20	236	161.05	1000
134.10	163	143.00	8871	152.80	567	161.60	58
135.05	1939	143.90	828	153.80	114	162.00	102
135.80	125	145.10	813	154.00	120	165.20	54
136.50	155	146.05	901	155.10	1990	165.50	95
137.00	2302	146.60	106	155.70	233	166.60	78
138.60	74	146.90	522	157.05	1072	167.10	116
139.90	416	148.00	2046	157.80	149	167.60	228

Average of 13.773 to 13.780 min.: VL040105.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
168.30	115	175.10	37499				
169.40	99	176.10	496640				
169.60	243	177.10	32104				
170.20	169	177.90	927				
170.45	416	178.20	187				
170.80	76	191.60	85				
171.40	161	198.80	87				
172.00	1101	205.40	85				
172.20	509	280.80	72				
173.05	4445						
174.10	518080						

Instrument :

MSVOA_L

ClientSampleId :

BFB