


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL012021\
 Data File : VL036242.D
 Acq On : 20 Jan 2021 9:16
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL011321AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Jan 14 16:13:38 2021
 Last Update : Thu Jan 14 16:13:38 2021

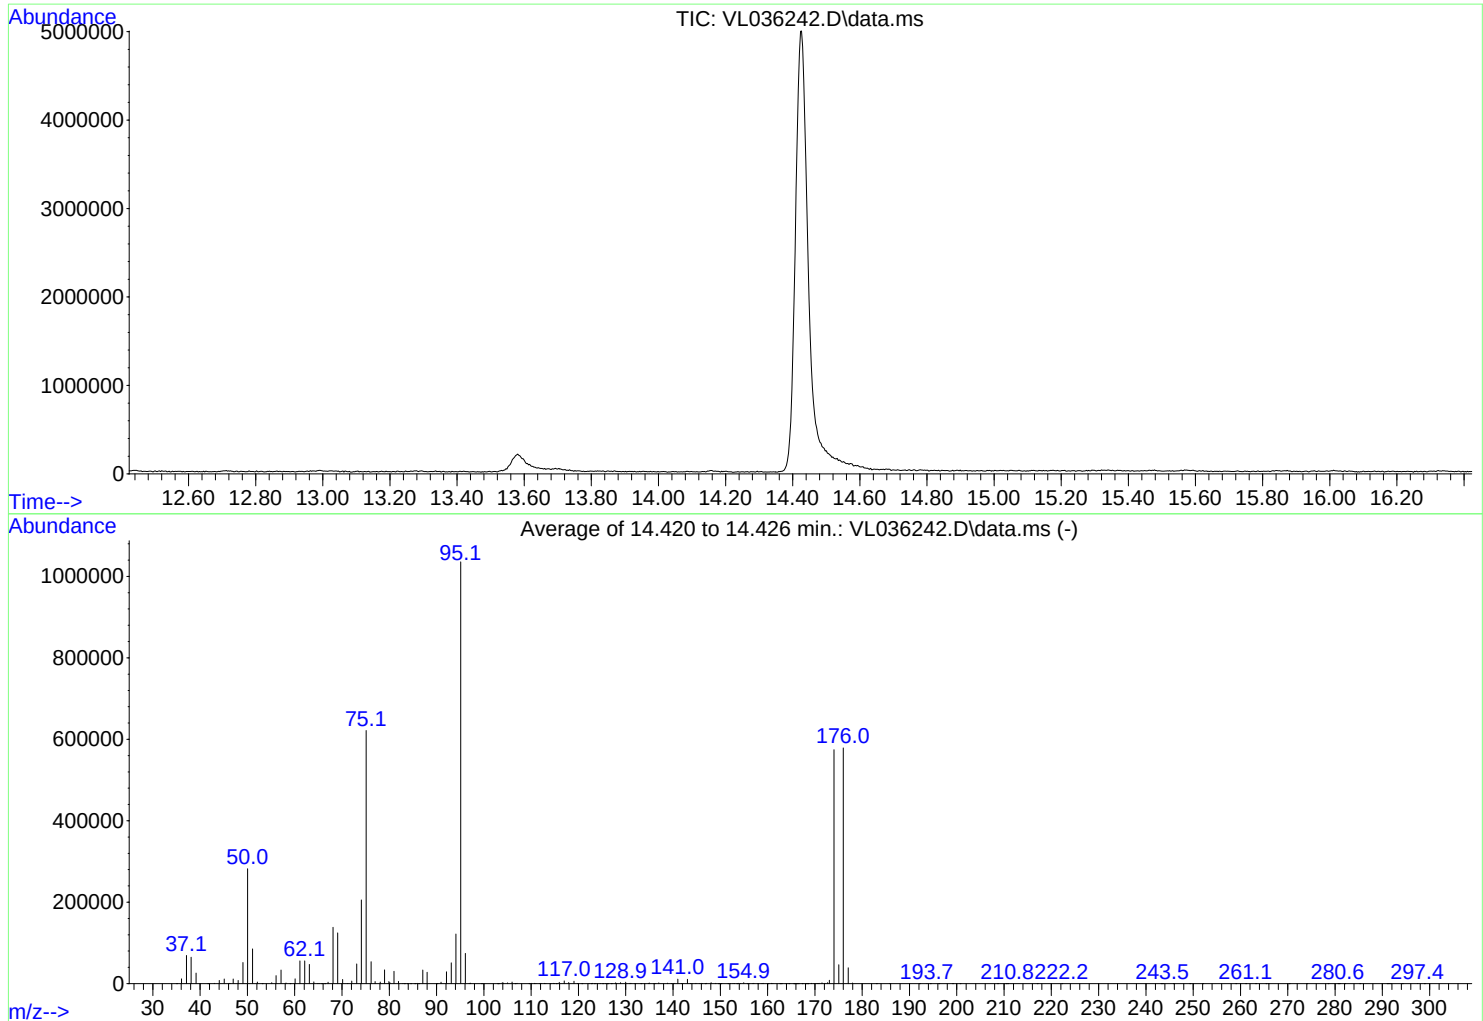

AutoFind: Scans 3618, 3619, 3620; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.2	282128	PASS
75	95	30	66	60.0	621589	PASS
95	95	100	100	100.0	1035776	PASS
96	95	5	9	7.2	74352	PASS
173	174	0.00	2	1.4	8324	PASS
174	95	50	120	55.5	574384	PASS
175	174	4	9	8.1	46416	PASS
176	174	93	101	100.7	578624	PASS
177	176	5	9	6.7	38891	PASS

Average of 14.420 to 14.426 min.: VL036242.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.00	57	46.10	905	57.10	33517	66.35	163
36.05	11661	46.30	588	58.15	1727	67.05	3454
37.10	69110	47.00	11593	59.00	132	68.10	138283
38.10	65037	48.05	7714	60.10	11860	69.10	124504
39.15	25821	49.05	52006	61.10	55704	70.15	10354
40.00	618	50.05	282128	62.10	55963	71.20	312
41.60	77	51.10	85173	63.10	47096	72.05	6174
42.00	310	52.10	3833	64.05	4371	73.10	48305
43.00	765	53.10	92	64.90	316	74.10	205589
44.05	8070	55.15	2196	65.15	309	75.10	621589
45.10	11582	56.05	19521	65.70	164	76.15	53821

Instrument :
MSVOA_L
ClientSampleId :
BFB

Average of 14.420 to 14.426 min.: VL036242.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.00	4976	85.40	52	96.10	74352	107.00	1011
78.10	3777	85.90	1007	96.90	686	109.55	20
79.00	34013	86.20	232	97.20	1225	110.10	860
79.90	5002	87.10	33592	99.50	54	110.75	678
80.10	2948	88.00	27840	102.90	196	111.00	639
81.00	30301	90.10	165	103.10	198	111.80	103
81.95	5503	90.95	3760	103.90	2468	112.05	866
82.90	547	92.10	29173	104.10	1710	112.80	663
83.20	194	93.10	51251	105.00	1915	113.10	324
83.80	72	94.10	121938	105.95	4151	114.00	50
84.50	51	95.10	1.03578e+006	106.60	170	114.65	842

Average of 14.420 to 14.426 min.: VL036242.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
114.90	526	123.40	54	130.00	3654	138.85	1181
115.30	211	124.00	286	130.90	726	139.65	617
115.95	3052	124.60	294	131.10	739	140.20	984
117.00	6700	125.10	83	131.90	213	141.00	10922
117.95	2772	125.70	391	133.20	171	141.80	442
119.05	5846	126.00	58	134.00	615	142.10	344
119.80	384	126.20	104	134.80	798	143.05	10443
120.70	54	126.95	81	135.00	1449	143.70	273
122.25	257	127.85	1821	135.90	118	144.00	407
122.70	207	128.10	927	136.35	310	144.85	989
122.95	792	128.90	2178	137.00	1986	145.70	281

Average of 14.420 to 14.426 min.: VL036242.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
146.00	906	152.70	333	158.80	352	166.00	191
146.20	413	153.00	599	159.05	829	166.20	58
146.80	216	153.50	92	160.10	169	166.50	84
147.05	847	153.85	816	160.85	817	167.30	242
148.05	2465	154.20	273	161.10	321	167.95	390
149.05	728	154.95	2580	162.60	55	168.20	196
149.60	95	155.70	120	162.90	90	168.50	81
149.90	553	156.10	524	163.90	95	168.70	277
150.10	105	156.90	413	164.50	71	169.25	712
151.60	178	157.10	831	165.50	111	169.85	354
152.10	396	157.90	78	165.70	90	170.20	284

Average of 14.420 to 14.426 min.: VL036242.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.50	256	177.95	1698	210.75	149	265.40	71
170.70	346	183.00	60	217.00	54	265.85	177
170.90	773	185.80	205	222.20	82	270.30	74
171.50	2141	192.10	134	243.20	102	274.00	93
172.10	785	193.70	260	243.50	104	278.50	106
172.70	2208	194.40	71	245.80	94	280.60	163
173.05	8324	196.20	88	249.30	95	280.90	79

174.05	574384	199.10	68	252.00	75	282.00	76
175.05	46416	200.70	114	259.00	69	285.20	69
176.00	578624	208.60	60	261.10	183	291.00	74
177.05	38891	210.40	54	263.20	140	291.30	154

Average of 14.420 to 14.426 min.: VL036242.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
291.70	71						
294.20	194						
297.45	315						
298.90	148						

Instrument :
MSVOA_L
ClientSampleId :
BFB