


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL012221\
 Data File : VL036260.D
 Acq On : 22 Jan 2021 9:03
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL011321AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Jan 14 16:13:38 2021
 Last Update : Thu Jan 14 16:13:38 2021

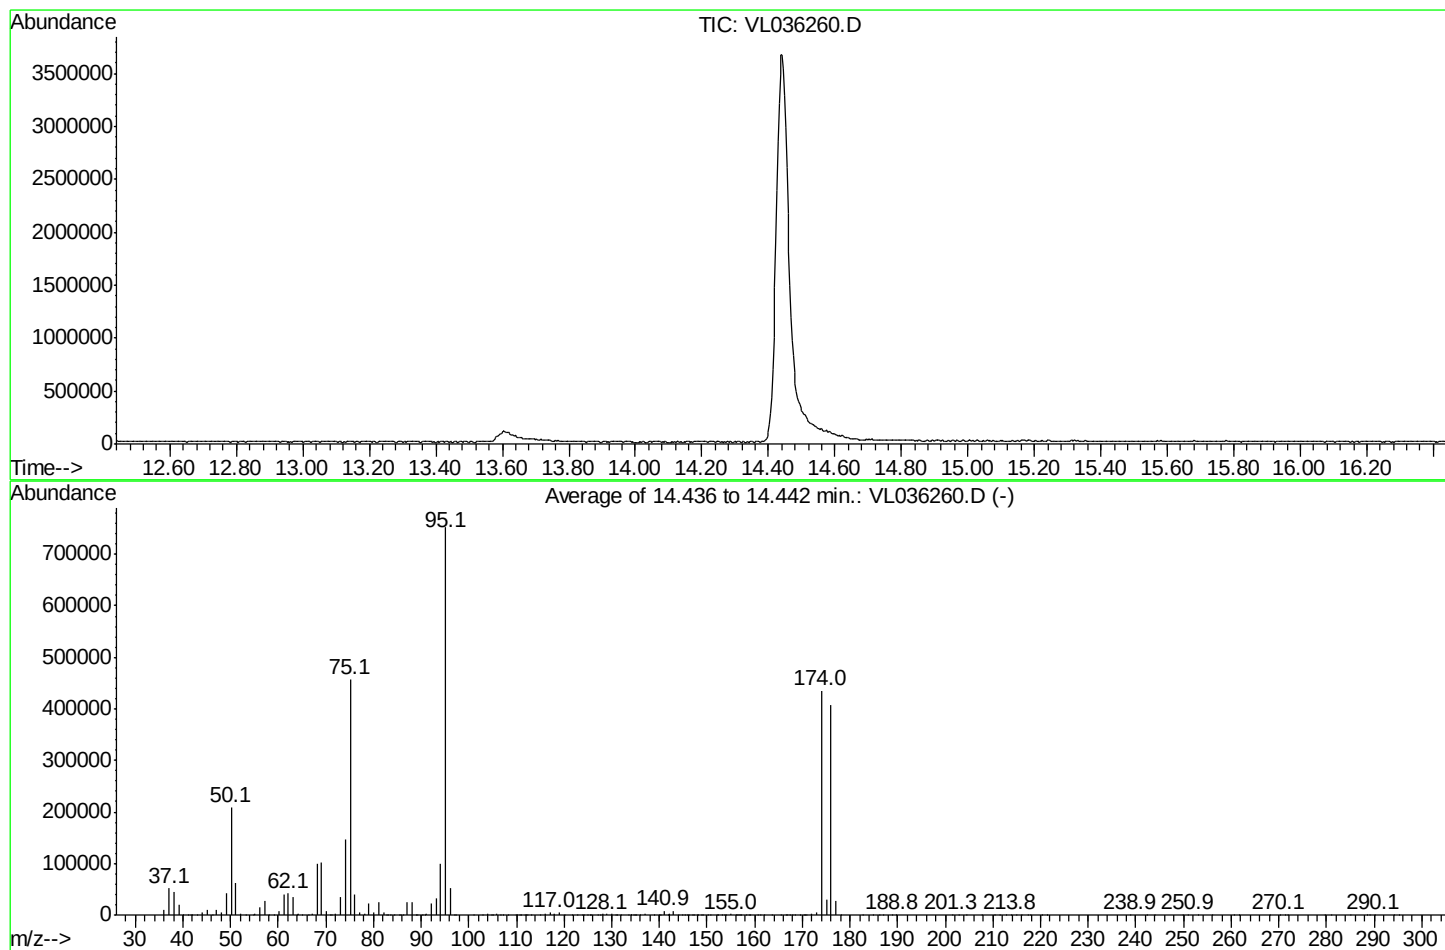

AutoFind: Scans 3623, 3624, 3625; Background Corrected with Scan 3600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.6	207872	PASS
75	95	30	66	60.6	455978	PASS
95	95	100	100	100.0	752234	PASS
96	95	5	9	6.9	51912	PASS
173	174	0.00	2	0.9	4025	PASS
174	95	50	120	58.0	435989	PASS
175	174	4	9	6.6	28784	PASS
176	174	93	101	93.6	407893	PASS
177	176	5	9	6.6	26728	PASS