
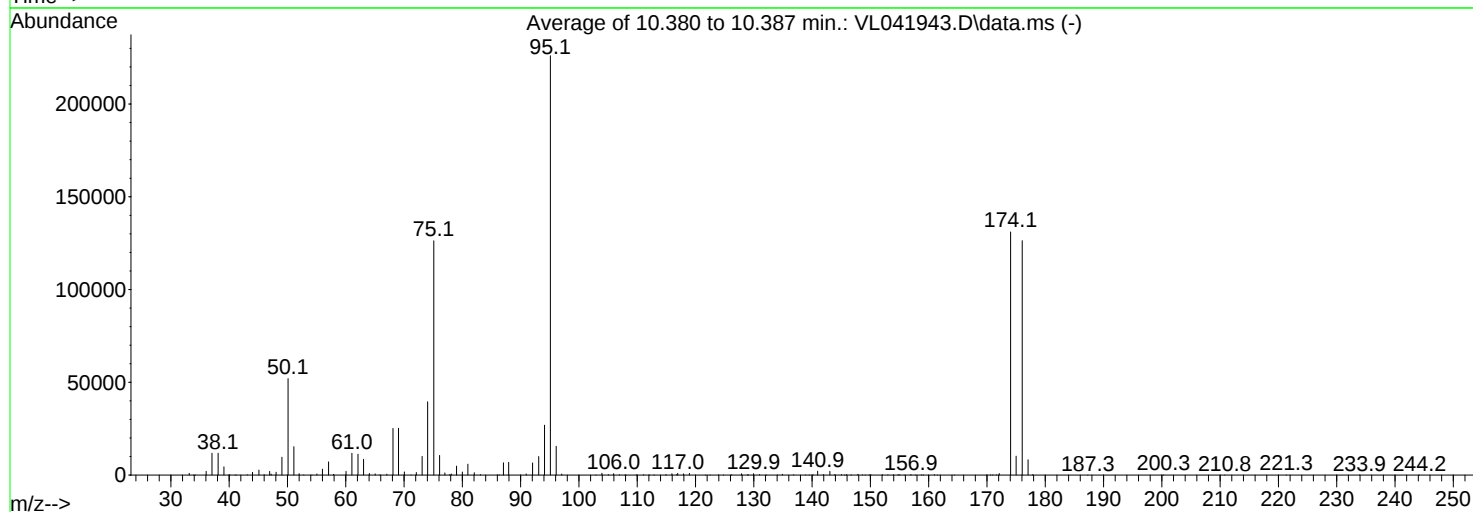


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL012725\
Data File : VL041943.D
Acq On : 27 Jan 2025 09:02
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Jan 14 23:15:42 2025

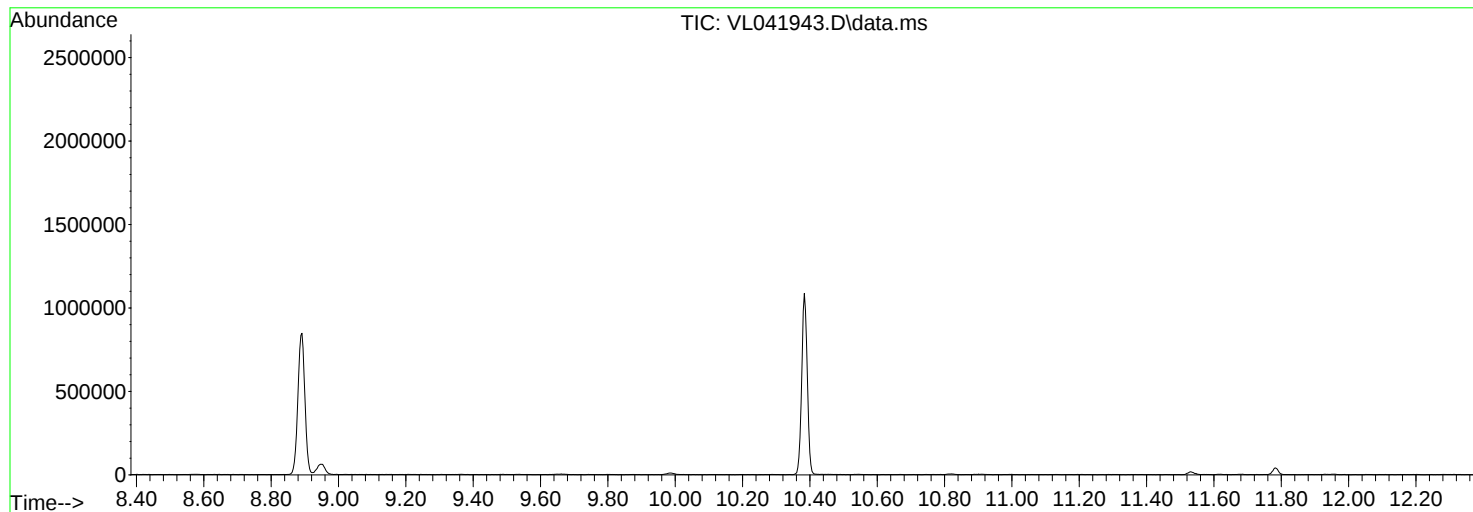

AutoFind: Scans 3180, 3181, 3182; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.0	51995	PASS
75	95	30	66	55.9	126285	PASS
95	95	100	100	100.0	226027	PASS
96	95	5	9	6.9	15556	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	58.0	131061	PASS
175	174	4	9	7.8	10200	PASS
176	174	93	101	96.4	126352	PASS
177	176	5	9	6.5	8251	PASS

Average of 10.380 to 10.387 min.: VL041943.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.15	926	44.00	1478	54.20	18	65.85	116
33.90	24	45.10	2698	55.05	616	67.05	533
34.20	18	46.00	137	56.00	3194	68.10	2517
36.05	2044	46.95	1990	57.05	7133	69.05	2524
37.05	11763	47.20	522	57.90	414	70.05	1707
38.10	11815	48.05	1552	60.05	2014	71.20	21
39.10	4459	49.05	9623	61.05	11740	72.10	1411
39.95	2	50.10	51995	62.10	11259	73.10	10072
41.00	27	51.10	15320	63.05	8514	74.05	39522
41.20	53	52.00	757	64.05	890	75.10	126285
43.10	166	52.80	82	65.05	666	76.10	10576

Average of 10.380 to 10.387 min.: VL041943.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.00	1194	87.95	6853	105.95	750	116.95	940
77.80	171	90.95	649	106.95	205	117.95	687
78.10	601	92.05	6550	107.90	46	118.95	903
79.00	4834	93.10	9983	108.10	17	121.70	39
80.00	1662	94.10	26923	109.85	133	122.50	31
80.95	5879	95.10	226027	111.10	201	123.95	72
82.05	1310	96.10	15556	112.05	127	124.80	54
83.10	263	97.05	574	112.90	137	126.20	212
86.00	65	102.90	42	114.95	366	127.90	735
86.30	127	103.95	1007	115.95	758	128.90	180
87.05	6645	105.05	268	116.80	307	129.05	179

Average of 10.380 to 10.387 min.: VL041943.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
129.95	790	143.05	2056	152.05	151	161.50	19
131.00	289	143.90	270	153.00	123	164.40	21
132.20	42	145.05	277	153.95	170	169.90	42
134.10	32	145.60	78	154.75	263	170.60	106
134.90	436	145.90	237	155.05	277	171.00	100
136.85	175	146.70	174	155.80	19	171.60	142
138.90	80	147.85	432	156.95	339	172.10	834
139.50	49	148.65	116	157.70	40	174.05	131061
140.15	155	149.10	67	158.80	149	175.00	10200
140.95	2102	149.80	170	159.10	68	176.05	126352
141.95	219	150.10	76	161.00	213	177.05	8251

Average of 10.380 to 10.387 min.: VL041943.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
177.85	237						
187.30	21						
200.30	68						
210.80	30						
221.35	34						
233.90	29						
244.20	20						