

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL020122\
 Data File : VL038320.D
 Acq On : 1 Feb 2022 13:44
 Operator : SY/AP
 Sample : N1341-02DL 10X
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 SVP-2DL

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 02/07/2022
 Supervised By : Mahesh Dadoda 02/07/2022

Quant Time: Feb 02 06:25:18 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL012422A

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument:

QLast Update : Mon Jan 24 14:12:48 2022

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.64	49	941925	10.00	ppbv	-0.04
33) 1,4-Difluorobenzene	7.14	114	2580170	10.00	ppbv	-0.04
55) Chlorobenzene-d5	12.04	117	2267684	10.00	ppbv	-0.05




System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.37	95	1795067	10.43	ppbv	-0.05
Spiked Amount	10.000	Range	65 - 135	Recovery	=	104.30%

Target Compounds

						Qvalue
9) Propene	3.01	41	746777m	12.234	ppbv	
13) Ethanol	3.60	45	12449m	1.900	ppbv	
15) Acetone	3.84	43	85865m	1.034	ppbv	
17) tert-Butyl alcohol	4.29	59	15193m	0.167	ppbv	
19) Isopropyl Alcohol	3.96	45	6048m	0.116	ppbv	
26) Hexane	5.65	57	59307	0.548	ppbv	# 45
30) Cyclohexane	7.09	84	13794m	0.147	ppbv	
32) 1,1,1-Trichloroethane	6.47	97	5347m	0.030	ppbv	
34) 2-Butanone	5.24	43	18489m	0.219	ppbv	
36) Benzene	6.85	78	24558m	0.108	ppbv	
38) Trichloroethene	7.80	130	2798m	0.033	ppbv	
52) Tetrachloroethene	11.19	164	5157m	0.066	ppbv	
53) Toluene	9.76	91	42709	0.169	ppbv	96
58) Ethyl Benzene	12.66	91	33749	0.101	ppbv	94
59) m/p-Xylene	12.92	91	57968m	0.204	ppbv	
60) o-Xylene	13.65	91	30651	0.116	ppbv	100
62) Isopropylbenzene	14.62	105	39030m	0.111	ppbv	
63) 1,1,2,2-Tetrachloroethane	13.63	83	22055m	0.113	ppbv	
64) n-propylbenzene	15.52	120	10561m	0.125	ppbv	
65) tert-Butylbenzene	16.70	119	43279m	0.149	ppbv	
67) sec-Butylbenzene	17.25	105	60532	0.150	ppbv	97
69) p-Isopropyltoluene	17.61	119	69080m	0.223	ppbv	
70) n-Butylbenzene	18.51	91	49950	0.165	ppbv	97
71) 2-Chlorotoluene	15.41	91	33579m	0.129	ppbv	
72) 4-Ethyltoluene	15.79	105	36452m	0.132	ppbv	
73) 1,3,5-Trimethylbenzene	15.95	105	33502m	0.135	ppbv	
74) 1,2,4-Trimethylbenzene	16.72	105	42035	0.160	ppbv	96
75) 1,3-Dichlorobenzene	16.94	146	20902m	0.149	ppbv	
76) 1,4-Dichlorobenzene	17.09	146	18413	0.135	ppbv	82
77) 1,2-Dichlorobenzene	17.77	146	18924m	0.145	ppbv	
78) Hexachloro-1,3-Butadiene	23.33	225	16612m	0.183	ppbv	
79) Naphthalene	22.16	128	17241m	0.141	ppbv	
81) 1,2,4-Trichlorobenzene	21.89	180	9545m	0.132	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

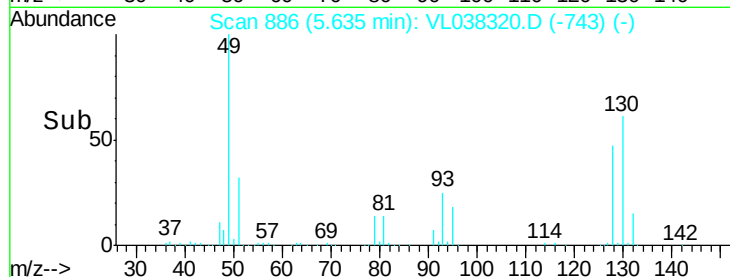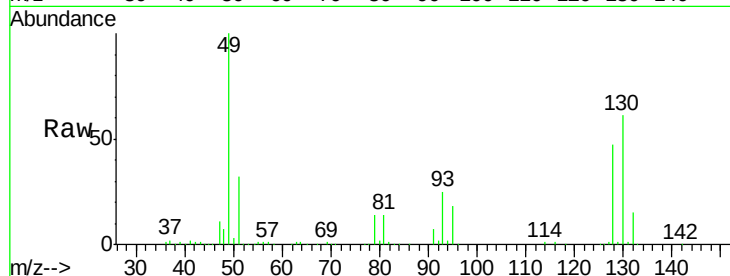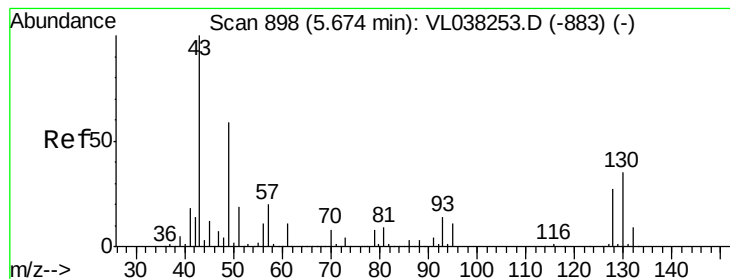

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.64 Instrument :

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

Acq: 1 Feb 2022 13:44 SVP-2DL

Tgt Ion:

Ion Ratio

49 100

128 48.





130 62.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022

Supervised By :Mahesh Dadoda 02/07/2022

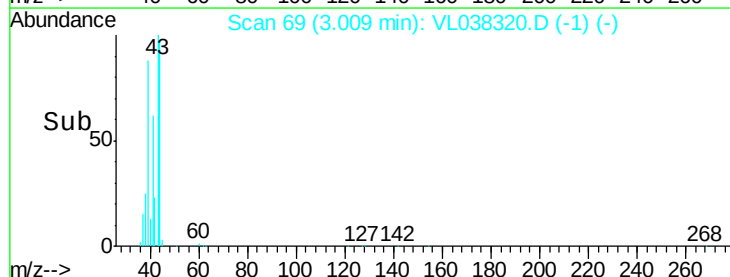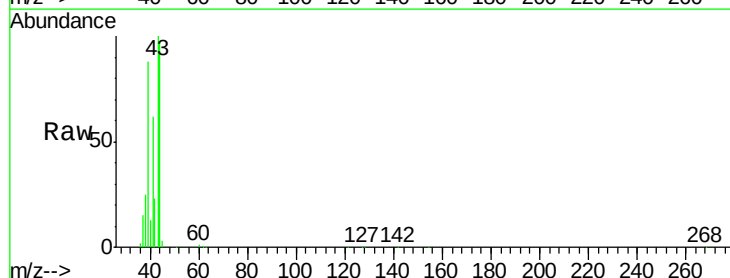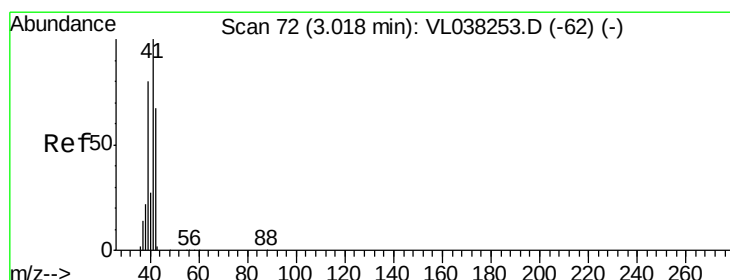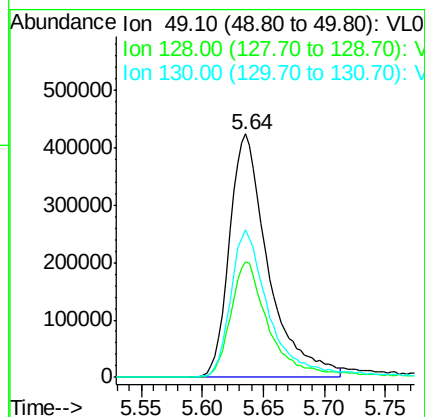

#9

Propene

Concen: 12.234 ppbv m

RT: 3.01 min Scan# 69

Delta R.T. -0.01 min

Lab File: VL038320.D


Acq: 1 Feb 2022 13:44


Tgt Ion: 41 Resp: 746777

Ion Ratio Lower Upper

41 100

42 17.7 54.9 82.3#

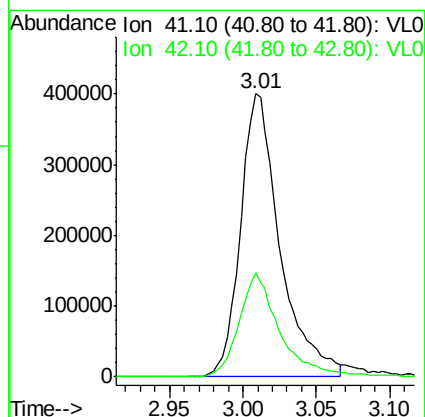




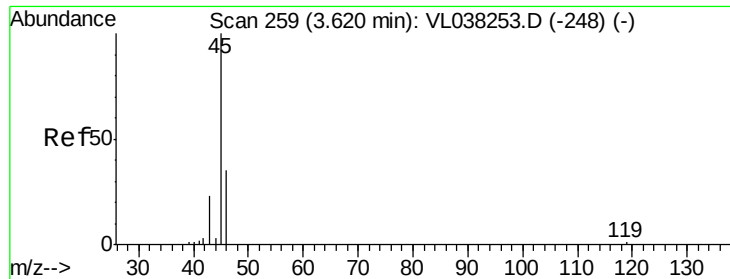


#13
Ethanol
Concen: 1.900 ppbv m
RT: 3.60
Instrument: MSVOA_L
Delta R.T.:
Lab File: ClientSampleId:
Acq: 1 Feb 2022 13:44

Tgt Ion:
Ion Ratio
45 100
46 0.




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/07/2022
Supervised By :Mahesh Dadoda 02/07/2022

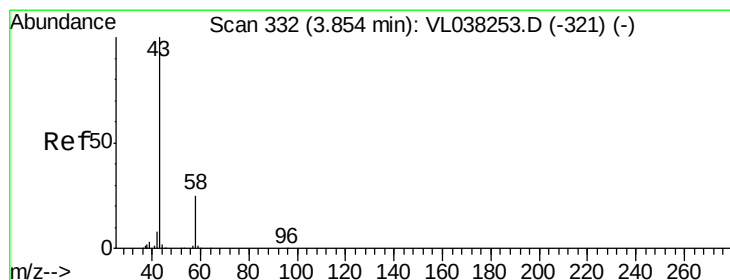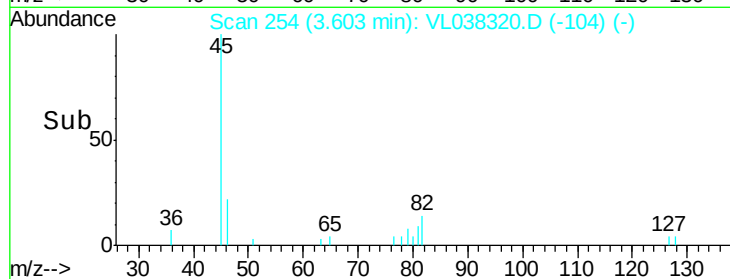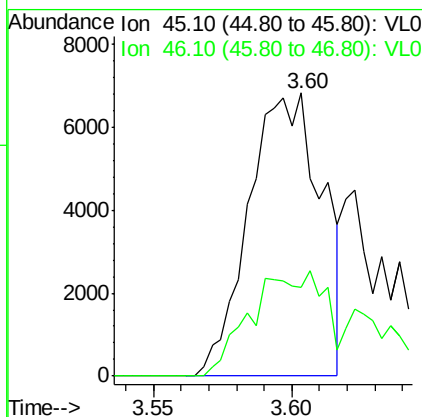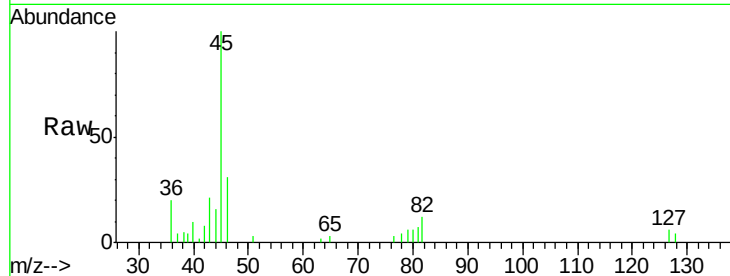

#15
Acetone
Concen: 1.034 ppbv m
RT: 3.84 min Scan# 329
Delta R.T. -0.01 min
Lab File: VL038320.D
Acq: 1 Feb 2022 13:44

Tgt Ion: 43 Resp: 85865
Ion Ratio Lower Upper
43 100
58 40.4 21.5 32.3#

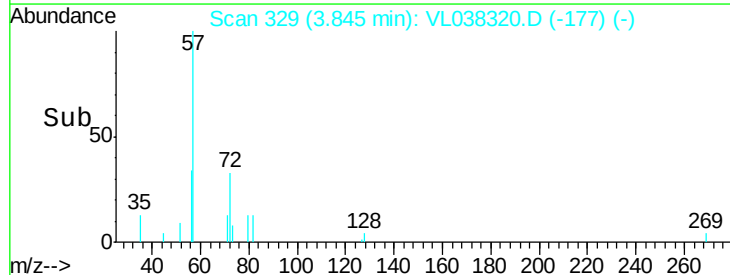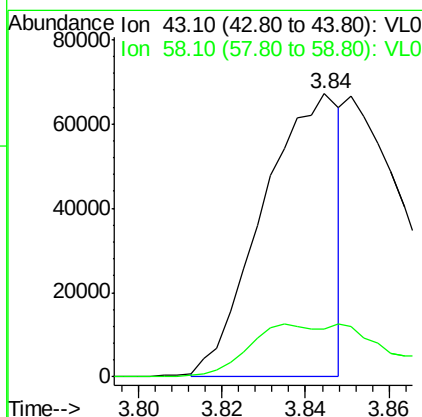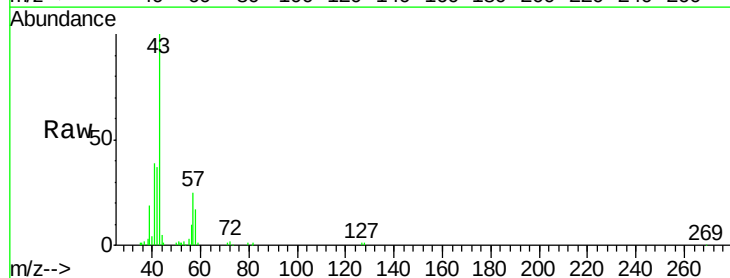

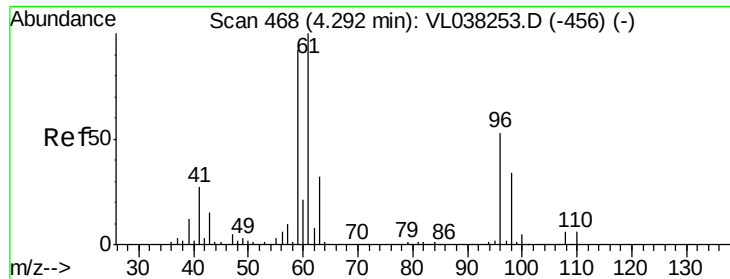

#17

tert-Butyl alcohol

Concen: 0.167 ppbv m

RT: 4.29 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 1 Feb 2022 13:44 SVP-2DL

Tgt Ion:

Ion Ratio

59 100





57 0.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022

Supervised By :Mahesh Dadoda 02/07/2022

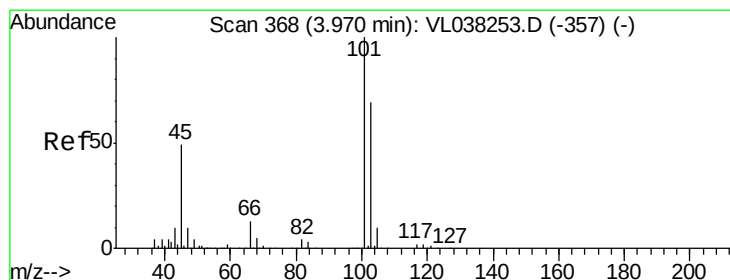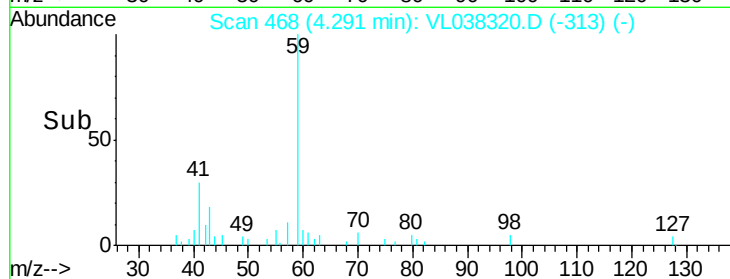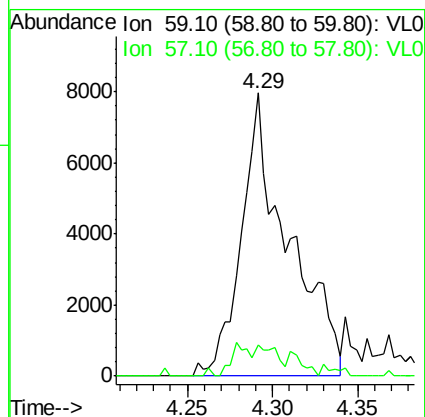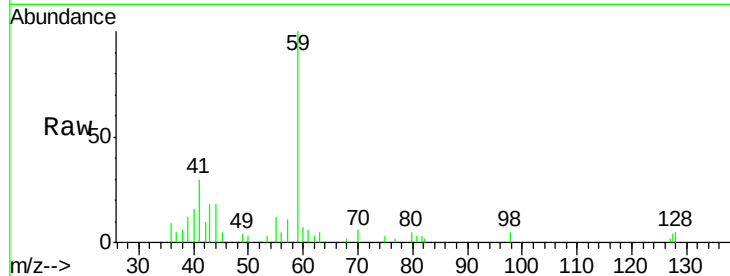

#19

Isopropyl Alcohol

Concen: 0.116 ppbv m

RT: 3.96 min Scan# 365

Delta R.T. -0.01 min

Lab File: VL038320.D




Acq: 1 Feb 2022 13:44


Tgt Ion: 45 Resp: 6048

Ion Ratio Lower Upper

45 100

58 0.0 2.3 3.5#

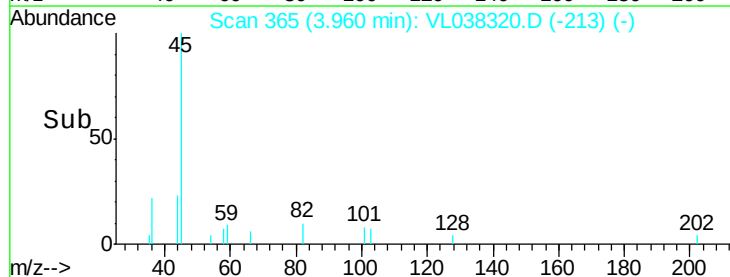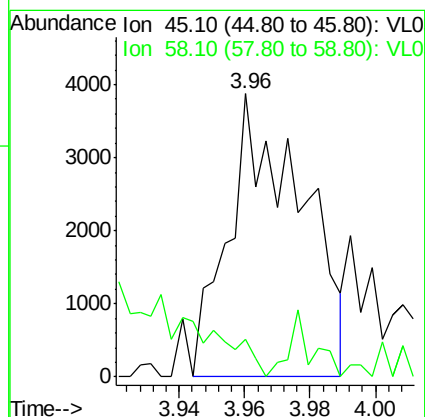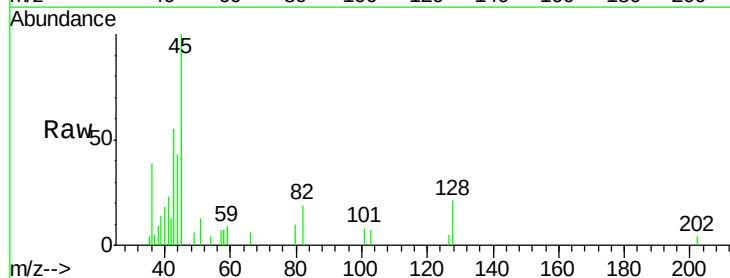




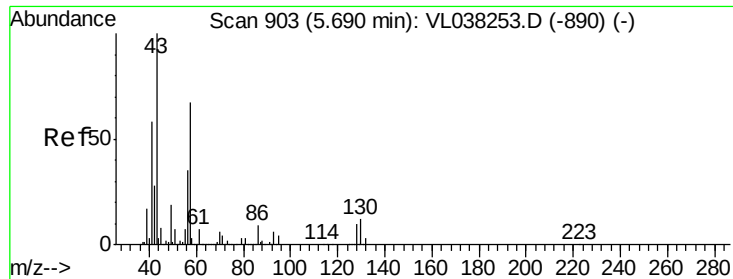


#26
Hexane
Concen: 0.548 ppbv
RT: 5.65
Delta R.T. MSVOA_L
Lab File: ClientSampleId :
Acq: 1 Feb 2022 13:44

Tgt Ion:
Ion Ratio
57 100
41 109.
43 89.
56 58.0 43.3 64.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/07/2022
Supervised By :Mahesh Dadoda 02/07/2022

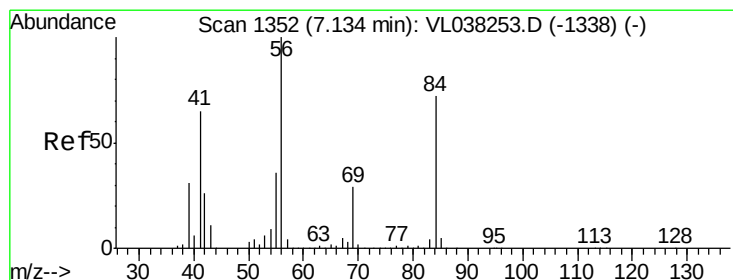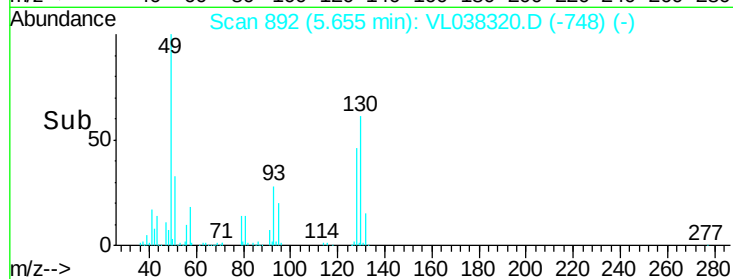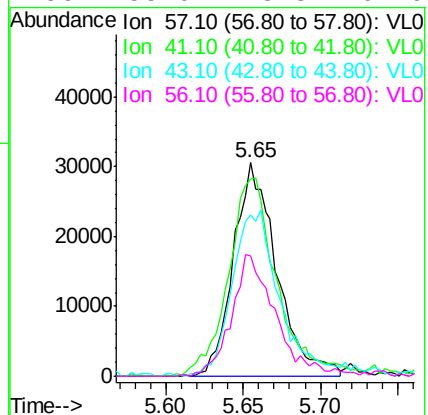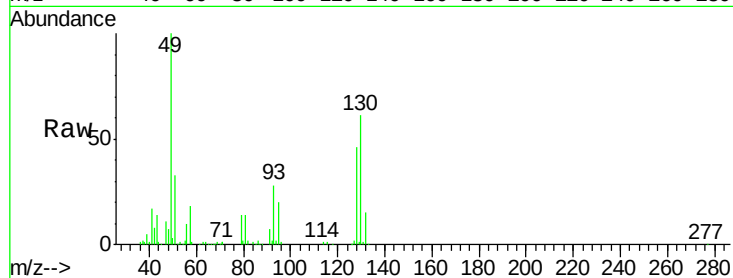

#30
Cyclohexane
Concen: 0.147 ppbv m
RT: 7.09 min Scan# 1339
Delta R.T. -0.04 min
Lab File: VL038320.D
Acq: 1 Feb 2022 13:44

Tgt Ion: 84 Resp: 13794
Ion Ratio Lower Upper
84 100
56 0.0 112.7 169.1#
41 0.0 71.1 106.7#

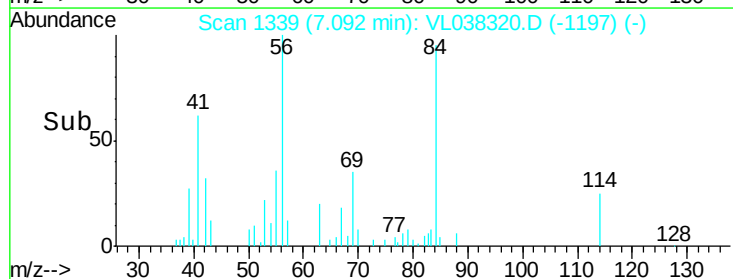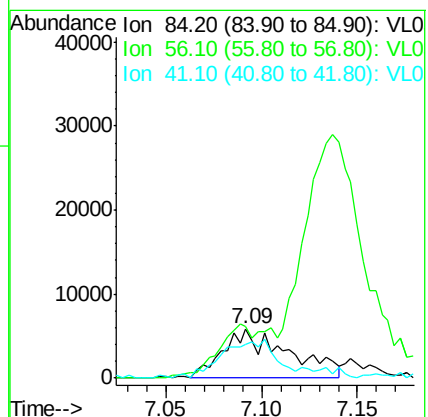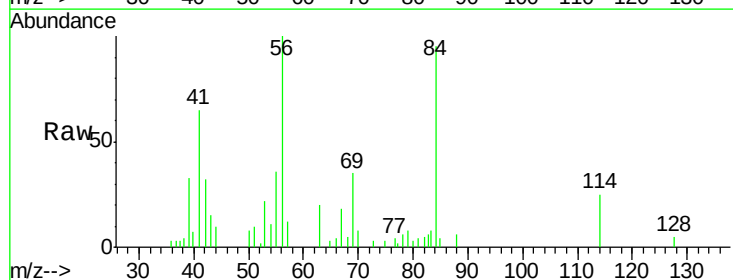

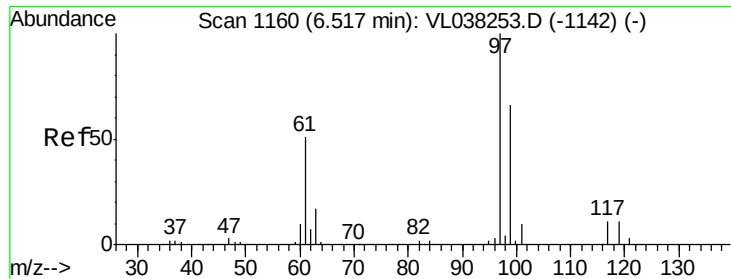

#32

1,1,1-Trichloroethane

Concen: 0.030 ppbv m

RT: 6.47 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 1 Feb 2022 13:44 SVP-2DL

Tgt Ion:

Ion Ratio

97 100

99 0.





61 58.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022

Supervised By :Mahesh Dadoda 02/07/2022

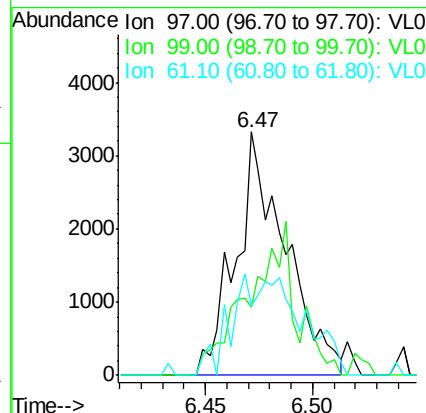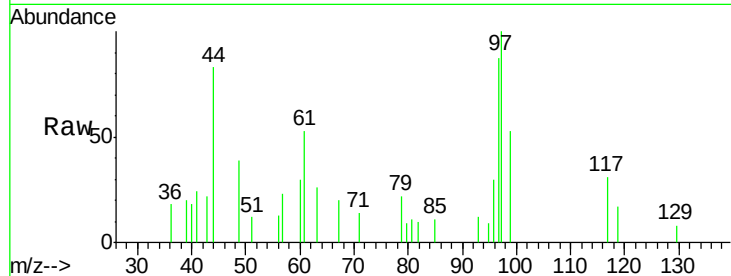

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.14 min Scan# 1353

Delta R.T. -0.04 min

Lab File: VL038320.D

Acq: 1 Feb 2022 13:44




Tgt Ion:114 Resp: 2580170


Ion Ratio Lower Upper

114 100

63 26.5 22.0 33.0

88 18.8 15.0 22.6

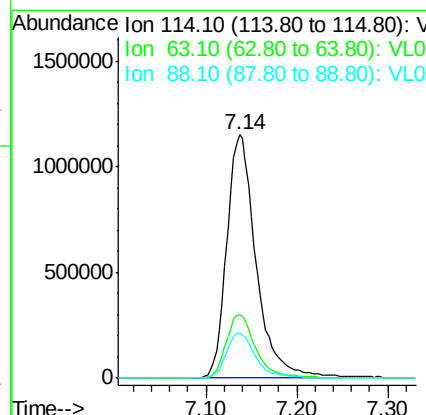

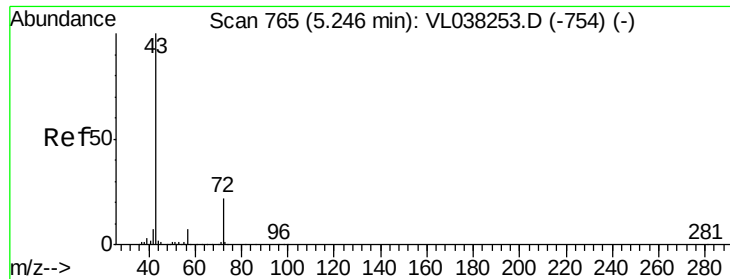

#34

2-Butanone

Concen: 0.219 ppbv m

RT: 5.24 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 1 Feb 2022 13:44 SVP-2DL

Tgt Ion:

Ion Ratio

43 100





72 0.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022

Supervised By :Mahesh Dadoda 02/07/2022

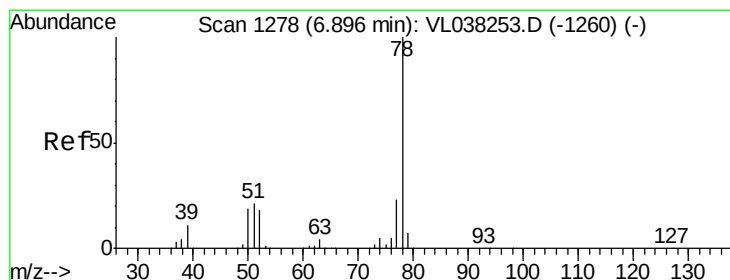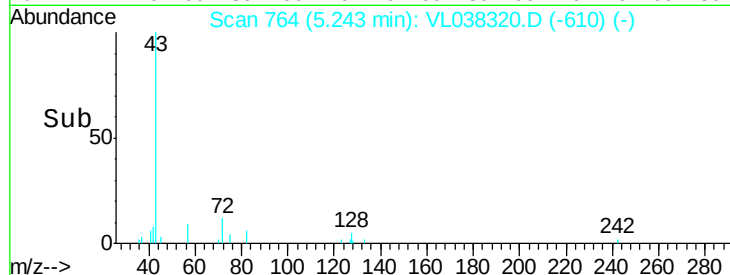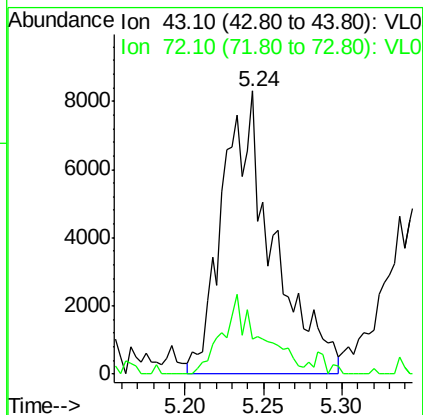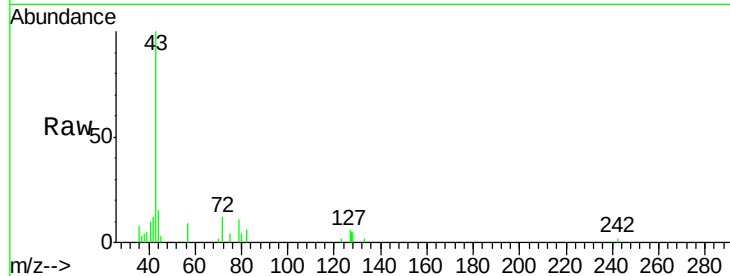

#36

Benzene

Concen: 0.108 ppbv m

RT: 6.85 min Scan# 1264

Delta R.T. -0.05 min

Lab File: VL038320.D

Acq: 1 Feb 2022 13:44




Tgt Ion: 78 Resp: 24558


Ion Ratio Lower Upper

78 100

77 27.6 18.2 27.2#

50 18.8 15.1 22.7

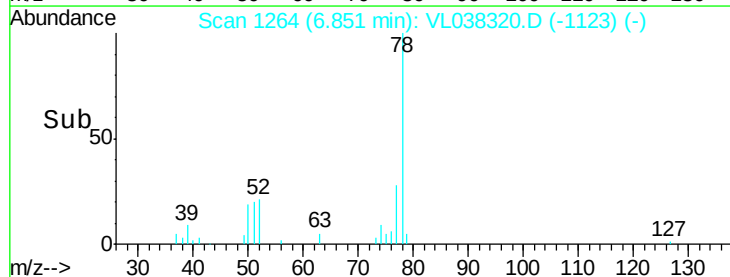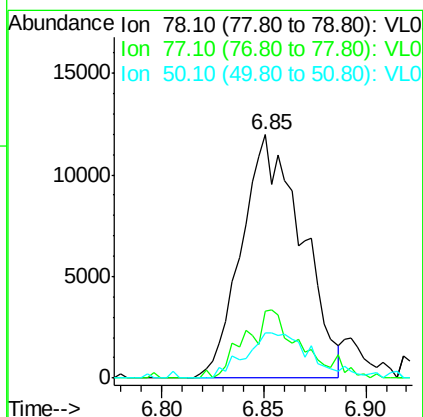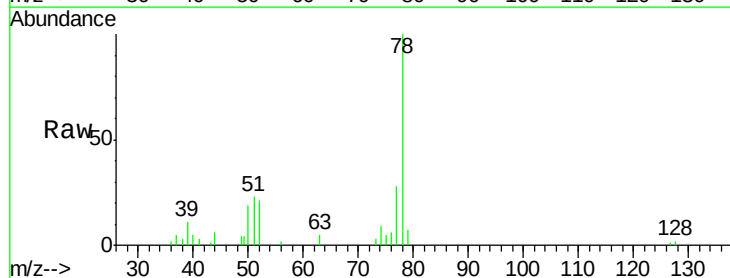




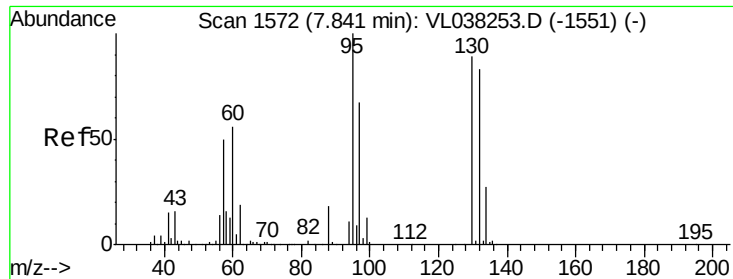


#38
 Trichloroethene
 Concen: 0.033 ppbv m
 RT: 7.80 min
 Instrument: MSVOA_L
 Delta R.T.:
 Lab File: ClientSampleId:
 SVP-2DL
 Acq: 1 Feb 2022 13:44

Tgt Ion:1
 Ion Ratio
 130 100
 95 92.
 132 81.
 97 31.5 59.6 89.4#




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 02/07/2022
 Supervised By :Mahesh Dadoda 02/07/2022

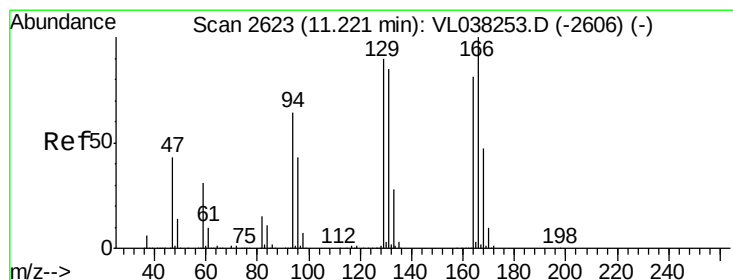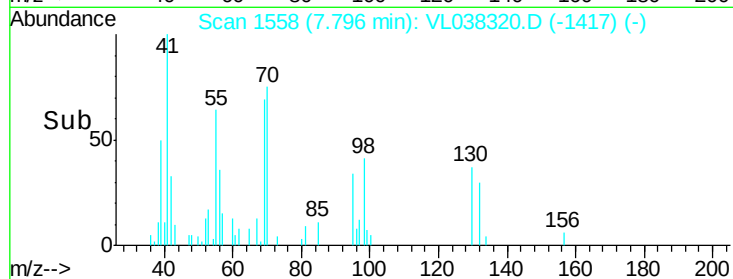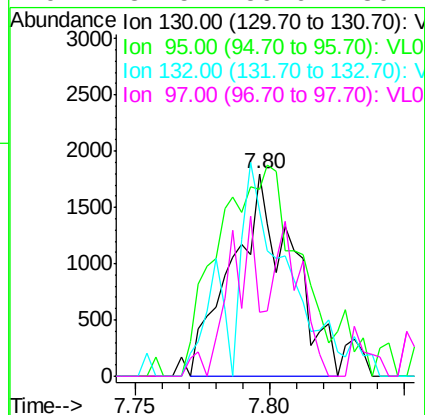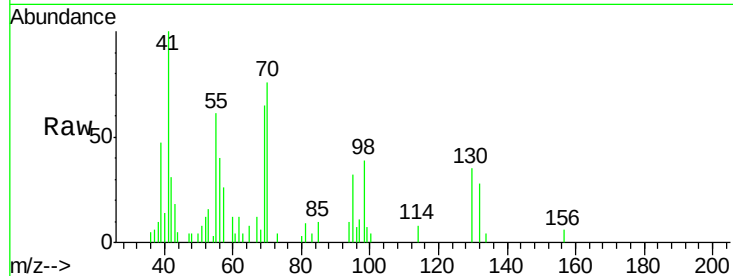

#52
 Tetrachloroethene
 Concen: 0.066 ppbv m
 RT: 11.19 min Scan# 2612
 Delta R.T. -0.04 min
 Lab File: VL038320.D
 Acq: 1 Feb 2022 13:44

Tgt Ion:164 Resp: 5157
 Ion Ratio Lower Upper
 164 100
 166 106.2 98.8 148.2
 129 89.7 89.2 133.8
 131 101.8 83.6 125.4

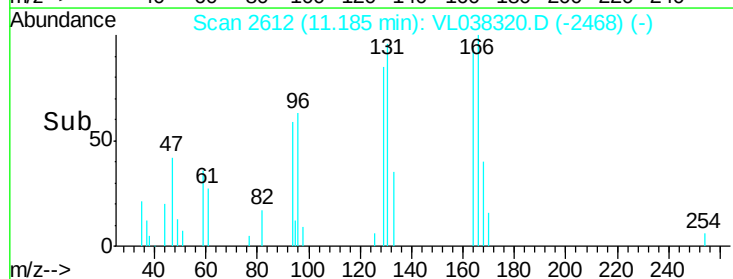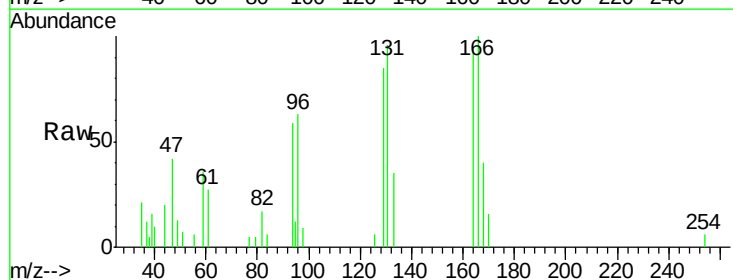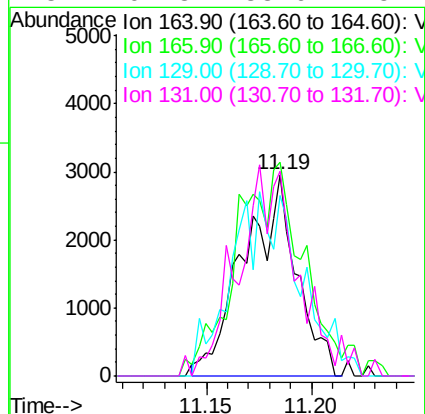







#53
Toluene
Concen: 0.169 ppbv
RT: 9.76
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId:
Acq: 1 Feb 2022 13:44

Tgt Ion:
Ion Ratio
91 100
92 62.




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/07/2022
Supervised By :Mahesh Dadoda 02/07/2022

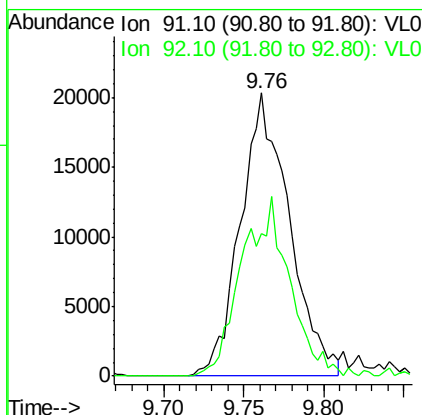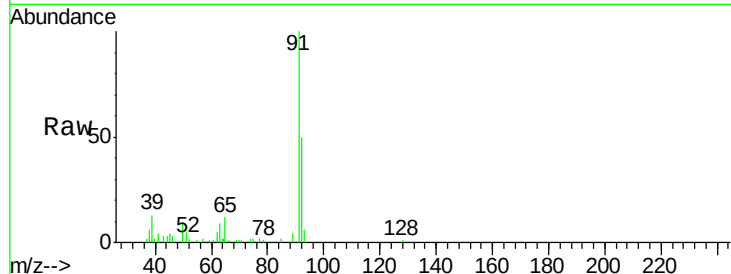

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.04 min Scan# 2878
Delta R.T. -0.05 min
Lab File: VL038320.D
Acq: 1 Feb 2022 13:44

Tgt Ion:117 Resp: 2267684
Ion Ratio Lower Upper
117 100
82 69.4 54.4 81.6
119 33.1 45.9 68.9#

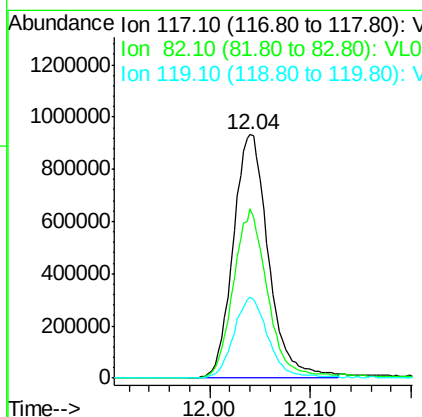




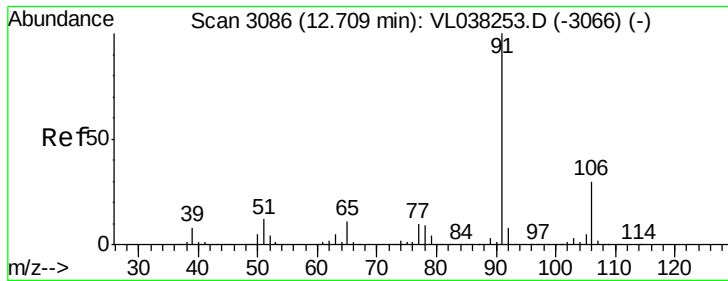


#58
Ethyl Benzene
Concen: 0.101 ppbv
RT: 12.66
Delta R.T. MSVOA_L
Lab File: ClientSampleId :
Acq: 1 Feb 2022 13:44

Tgt Ion:
Ion Ratio
91 100
106 26.




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/07/2022
Supervised By :Mahesh Dadoda 02/07/2022

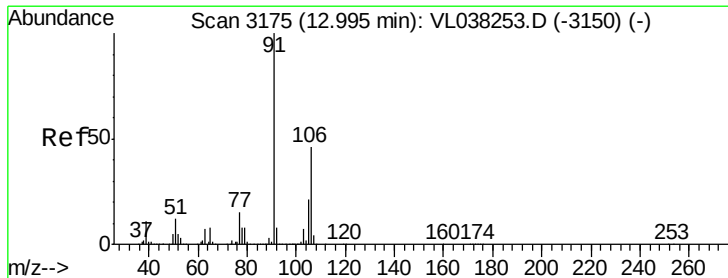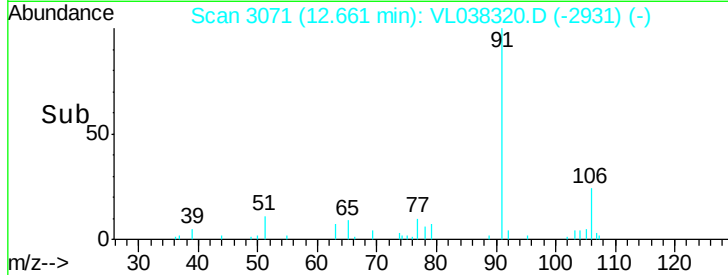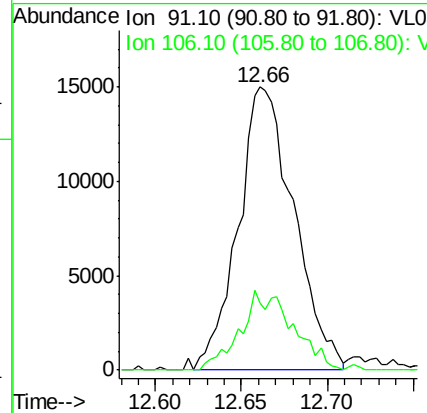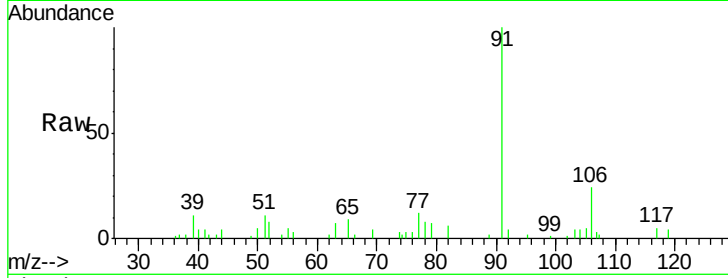

#59
m/p-Xylene
Concen: 0.204 ppbv m
RT: 12.92 min Scan# 3152
Delta R.T. -0.07 min
Lab File: VL038320.D
Acq: 1 Feb 2022 13:44

Tgt Ion: 91 Resp: 57968
Ion Ratio Lower Upper
91 100
106 0.0 34.8 52.2#

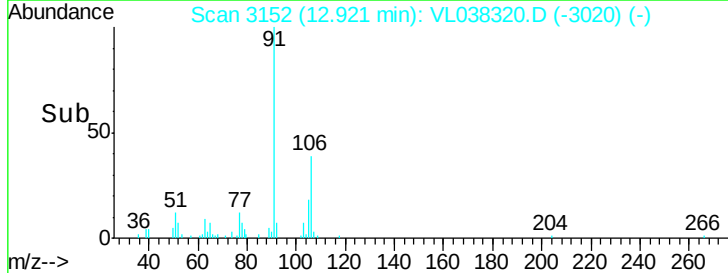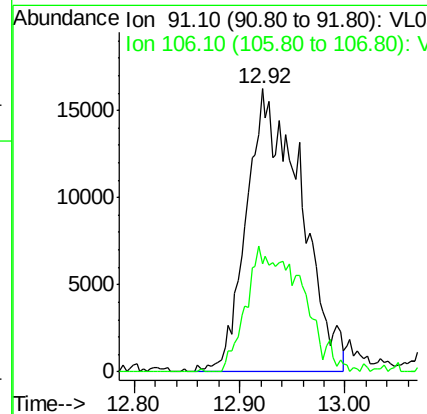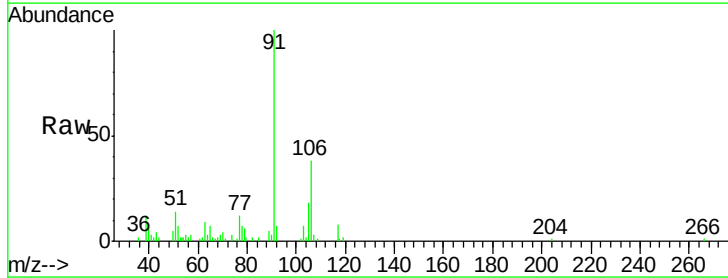




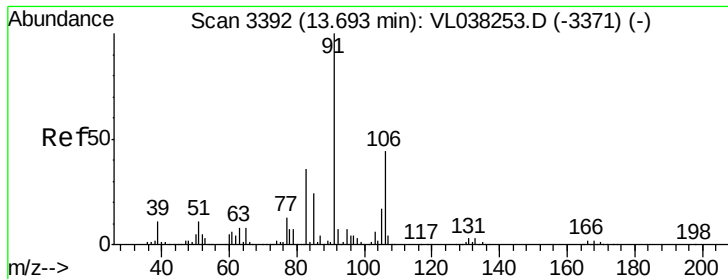


#60
o-Xylene
Concen: 0.116 ppbv
RT: 13.65
Delta R.T. MSVOA_L
Lab File: ClientSampleId :
Acq: 1 Feb 2022 13:44

Tgt Ion:
Ion Ratio
91 100
106 44.




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/07/2022
Supervised By :Mahesh Dadoda 02/07/2022

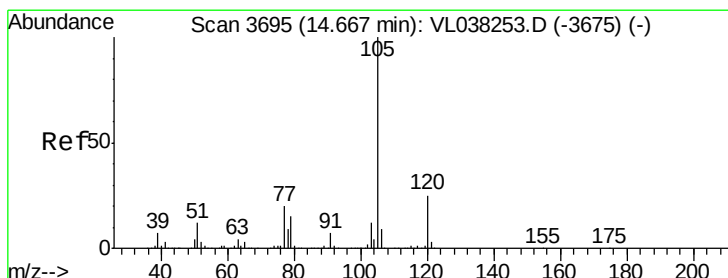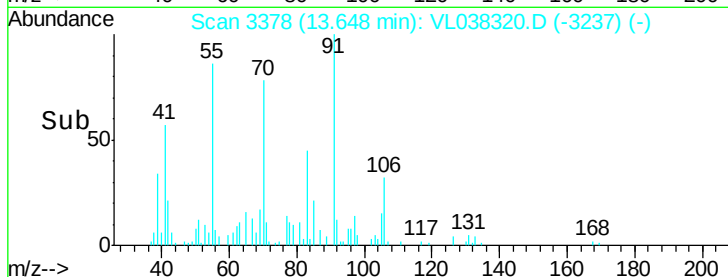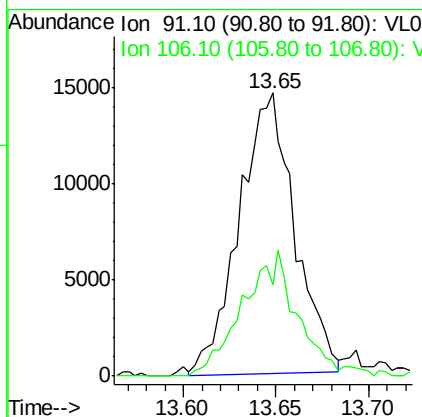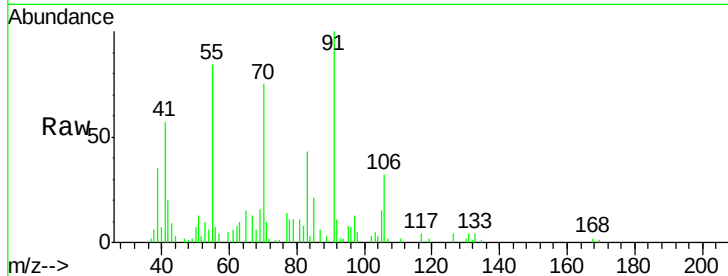

#62
Isopropylbenzene
Concen: 0.111 ppbv m
RT: 14.62 min Scan# 3680
Delta R.T. -0.05 min
Lab File: VL038320.D
Acq: 1 Feb 2022 13:44

Tgt Ion:105 Resp: 39030
Ion Ratio Lower Upper
105 100
120 23.1 20.5 30.7

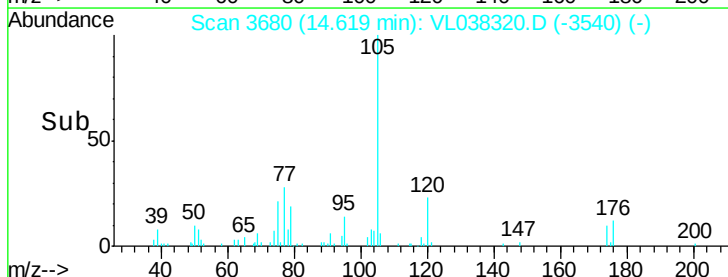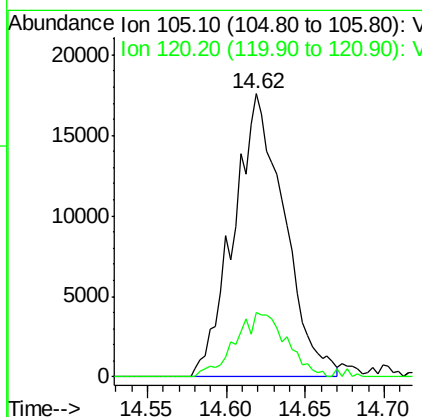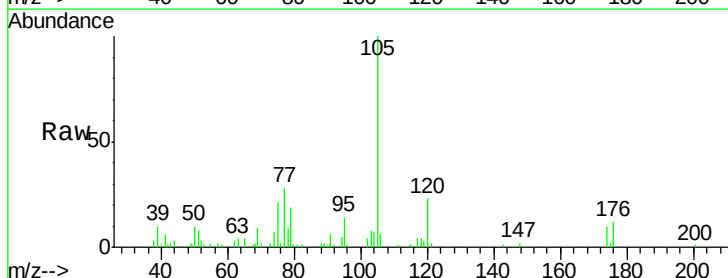

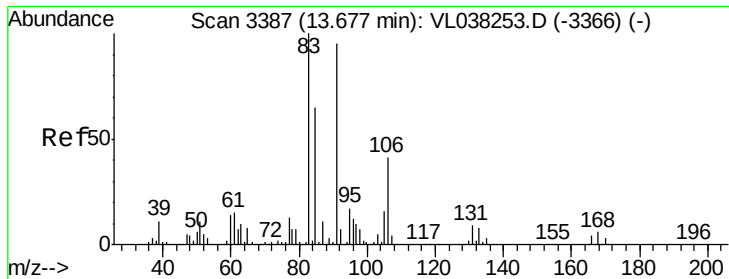

#63

1,1,2,2-Tetrachloroethane

Concen: 0.113 ppbv m

RT: 13.63

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

Acq: 1 Feb 2022 13:44

Tgt Ion:

Ion Ratio

83 100

131 0.





85 0.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022

Supervised By :Mahesh Dadoda 02/07/2022

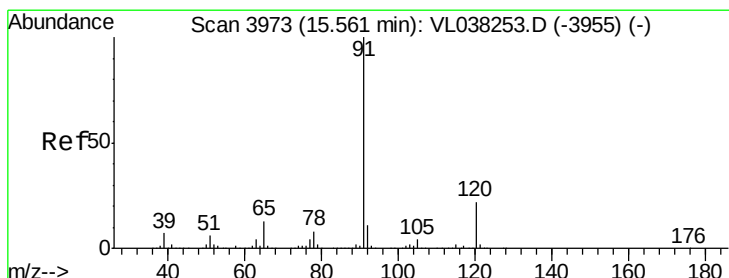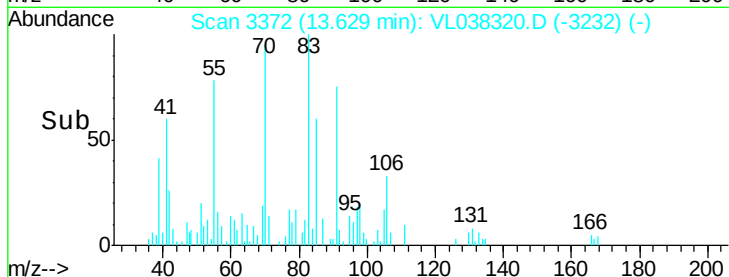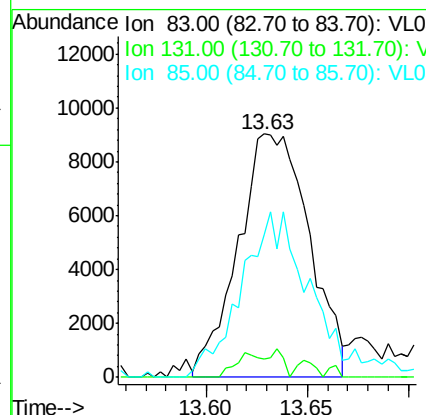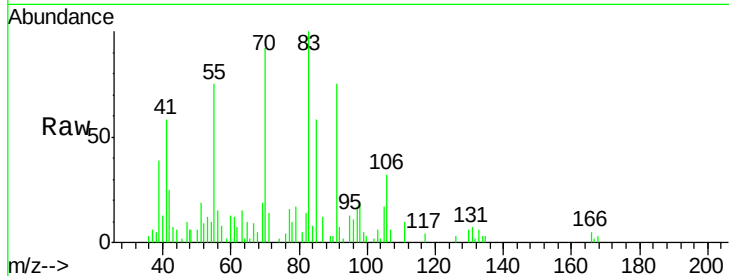

#64

n-propylbenzene

Concen: 0.125 ppbv m

RT: 15.52 min Scan# 3959

Delta R.T. -0.05 min

Lab File: VL038320.D




Acq: 1 Feb 2022 13:44


Tgt Ion:120 Resp: 10561

Ion Ratio Lower Upper

120 100

91 37.2 390.8 586.2#

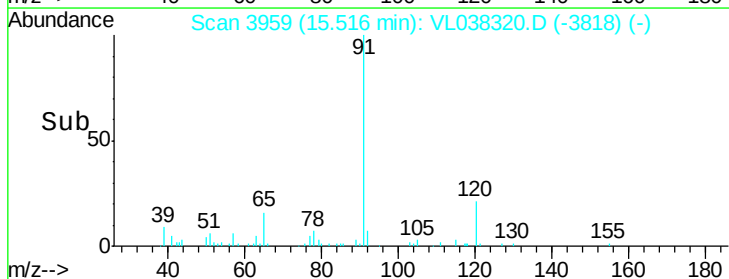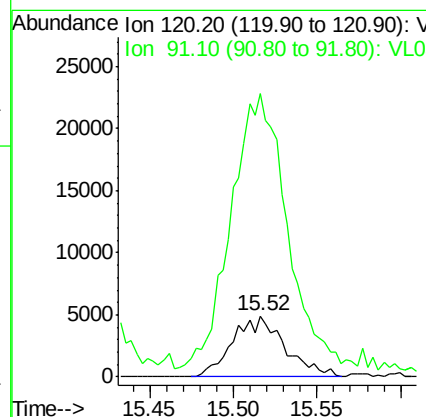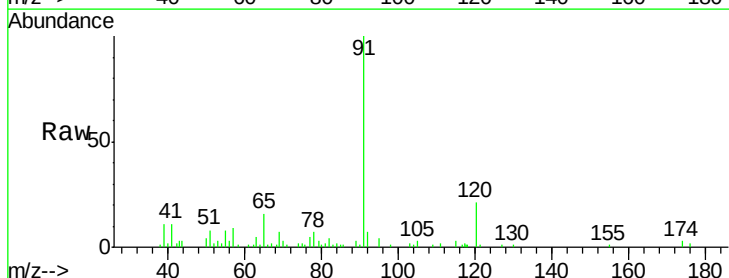

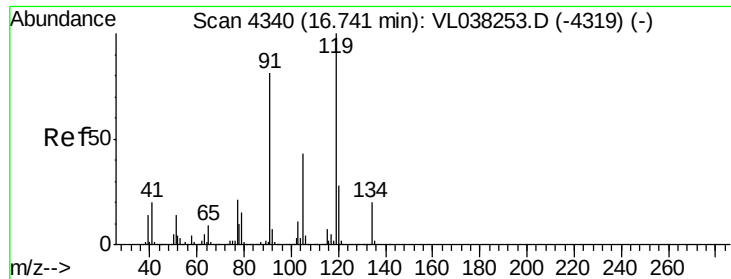

#65

tert-Butylbenzene

Concen: 0.149 ppbv m

RT: 16.70

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

Acq: 1 Feb 2022 13:44

Tgt Ion:1

Ion Rati

119 100

91 94.





134 21.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022

Supervised By :Mahesh Dadoda 02/07/2022

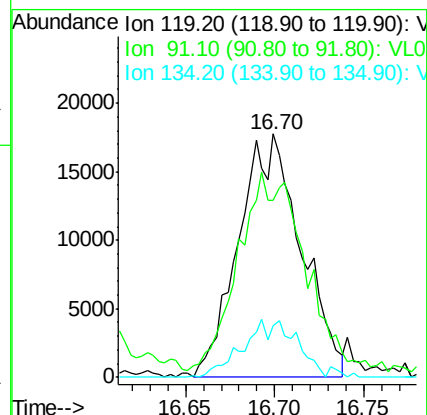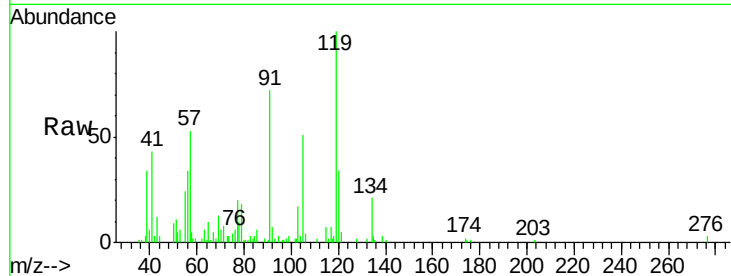

#67

sec-Butylbenzene

Concen: 0.150 ppbv

RT: 17.25 min Scan# 4497

Delta R.T. -0.05 min

Lab File: VL038320.D




Acq: 1 Feb 2022 13:44


Tgt Ion:105 Resp: 60532

Ion Ratio Lower Upper

105 100

134 19.4 14.3 21.5

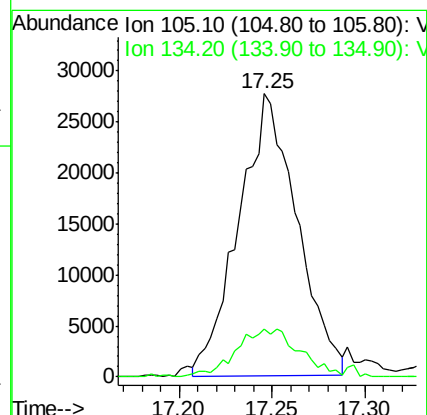




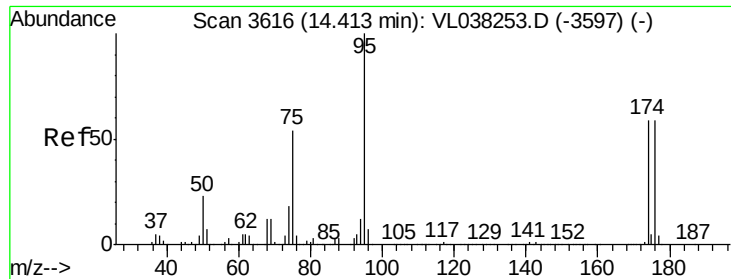


#68
 1-Bromo-4-Fluorobenzene
 Concen: 10.429 ppbv
 RT: 14.37
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId :
 Acq: 1 Feb 2022 13:44

Tgt Ion:
 Ion Ratio
 95 100
 174 60.
 175 4.




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 02/07/2022
 Supervised By :Mahesh Dadoda 02/07/2022

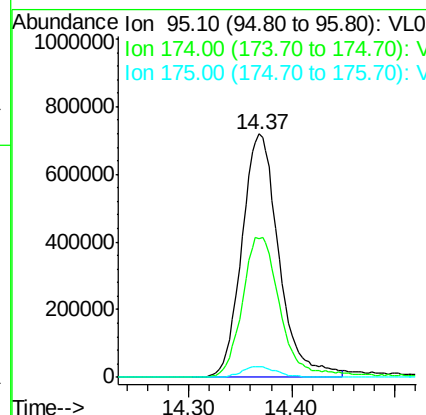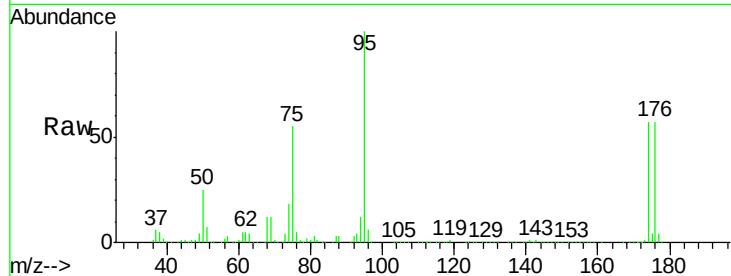

#69
 p-Isopropyltoluene
 Concen: 0.223 ppbv m
 RT: 17.61 min Scan# 4610
 Delta R.T. -0.04 min
 Lab File: VL038320.D
 Acq: 1 Feb 2022 13:44

Tgt Ion:119 Resp: 69080
 Ion Ratio Lower Upper
 119 100
 134 0.0 20.2 30.2#
 91 30.9 23.2 34.8

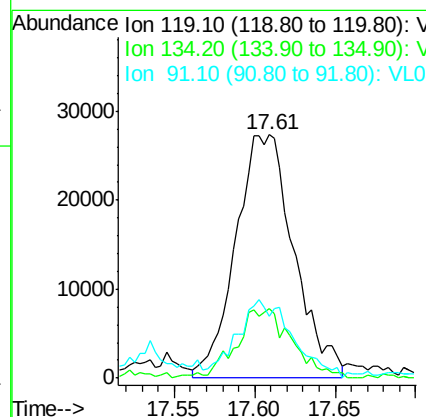

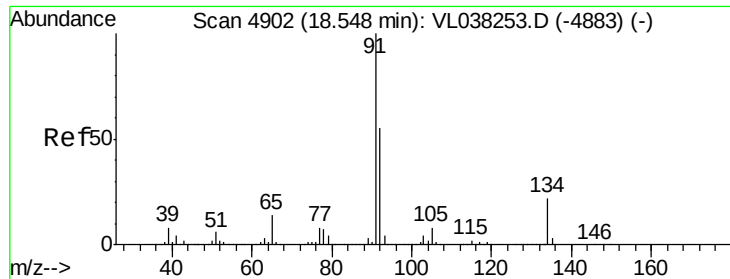

#70

n-Butylbenzene

Concen: 0.165 ppbv

RT: 18.51

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 1 Feb 2022 13:44

Tgt Ion:

Ion Ratio

91 100

92 55.





134 23.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022

Supervised By :Mahesh Dadoda 02/07/2022

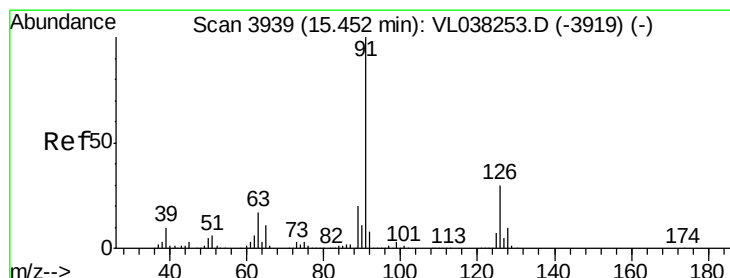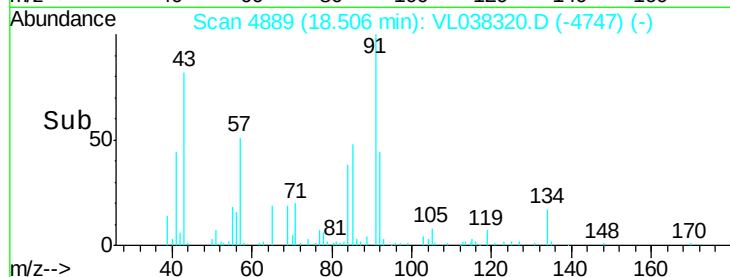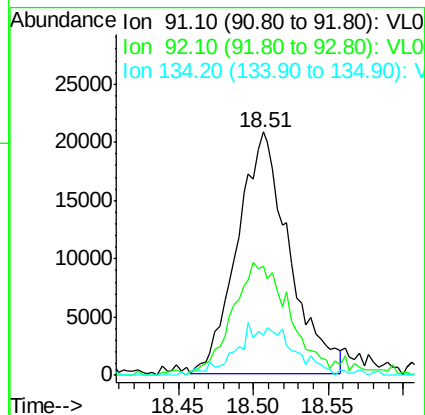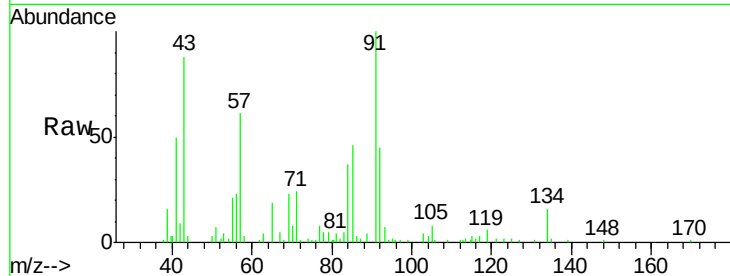

#71

2-Chlorotoluene

Concen: 0.129 ppbv m

RT: 15.41 min Scan# 3925

Delta R.T. -0.05 min

Lab File: VL038320.D




Acq: 1 Feb 2022 13:44


Tgt Ion: 91 Resp: 33579

Ion Ratio Lower Upper

91 100

126 30.0 12.1 48.5

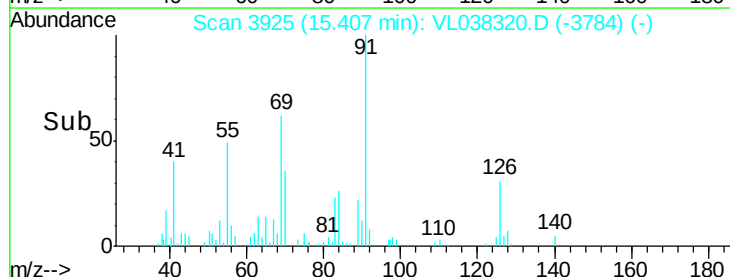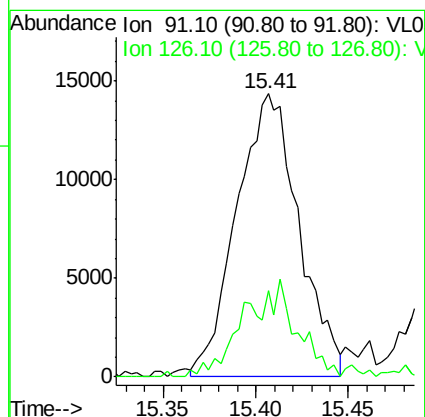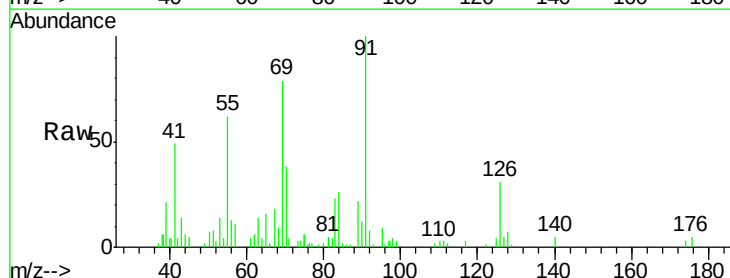







#72
 4-Ethyltoluene
 Concen: 0.132 ppbv m
 RT: 15.79
 Instrument: MSVOA_L
 Delta R.T.:
 Lab File: ClientSampleId:
 SVP-2DL
 Acq: 1 Feb 2022 13:44

Tgt Ion: 105.10 (104.80 to 105.80): V
 Ion Ratio: 100
 105 100
 120 30.
 91 14.
 77 17.0 11.7 17.5




Manual Integrations
 APPROVED


Reviewed By : Semsettin Yesilyurt 02/07/2022
 Supervised By : Mahesh Dadoda 02/07/2022

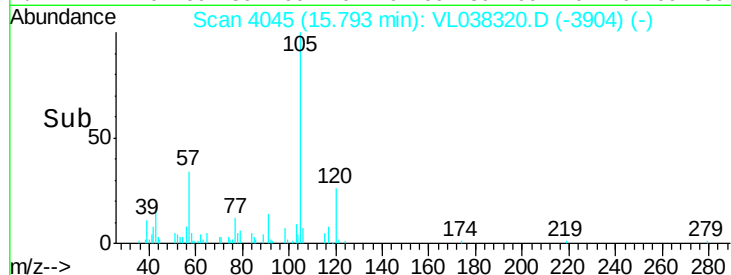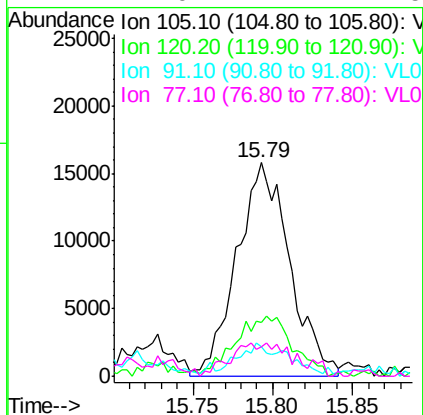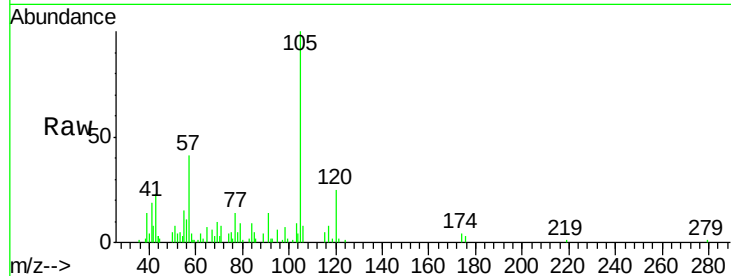

#73
 1,3,5-Trimethylbenzene
 Concen: 0.135 ppbv m
 RT: 15.95 min Scan# 4093
 Delta R.T. -0.05 min
 Lab File: VL038320.D
 Acq: 1 Feb 2022 13:44

Tgt Ion: 105 Resp: 33502
 Ion Ratio Lower Upper
 105 100
 120 41.1 36.6 55.0

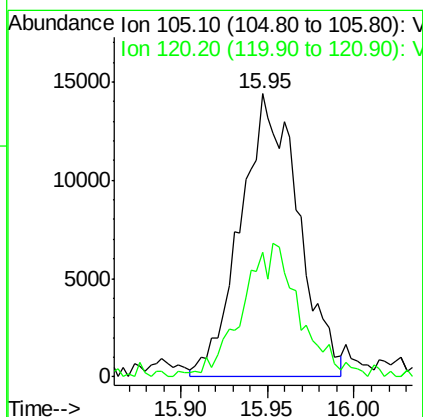




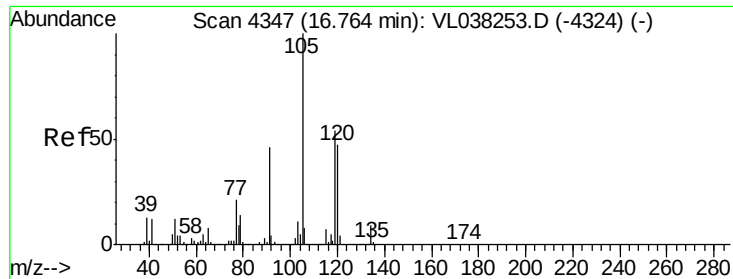


#74
1,2,4-Trimethylbenzene
Concen: 0.160 ppbv
RT: 16.72
Delta R.T. MSVOA_L
Lab File: ClientSampleId :
Acq: 1 Feb 2022 13:44

Tgt Ion: 105
Ion Ratio: 100
105 100
120 43.1
91 47.1
77 18.9 16.9 25.3




Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 02/07/2022
Supervised By : Mahesh Dadoda 02/07/2022

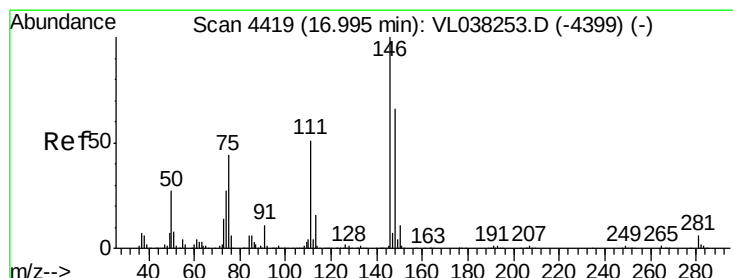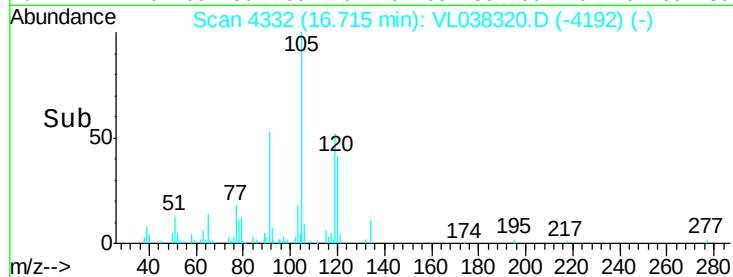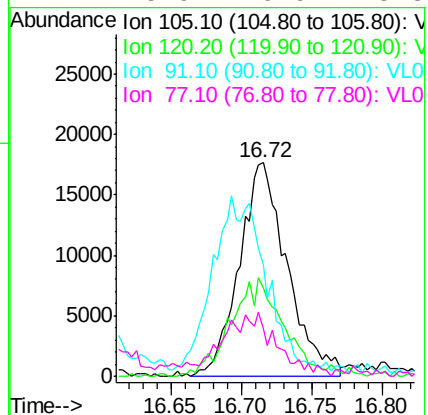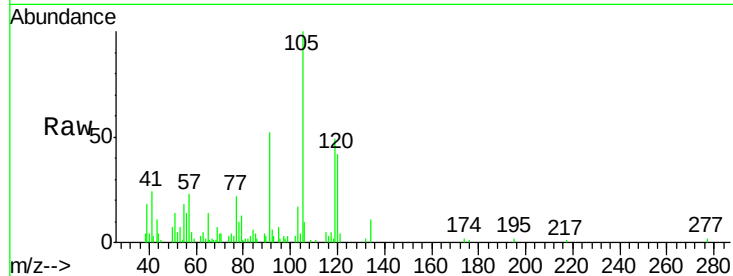

#75
1,3-Dichlorobenzene
Concen: 0.149 ppbv m
RT: 16.94 min Scan# 4403
Delta R.T. -0.05 min
Lab File: VL038320.D
Acq: 1 Feb 2022 13:44

Tgt Ion: 146 Resp: 20902
Ion Ratio Lower Upper
146 100
111 66.8 24.1 72.4
148 69.4 32.1 96.5

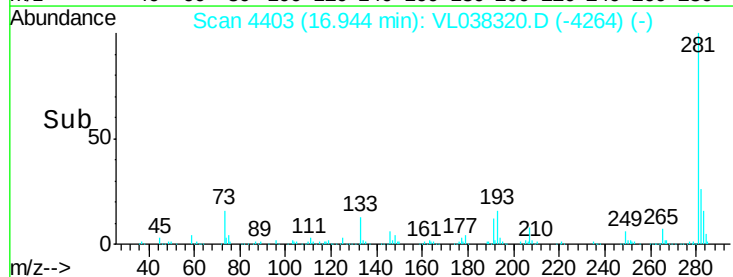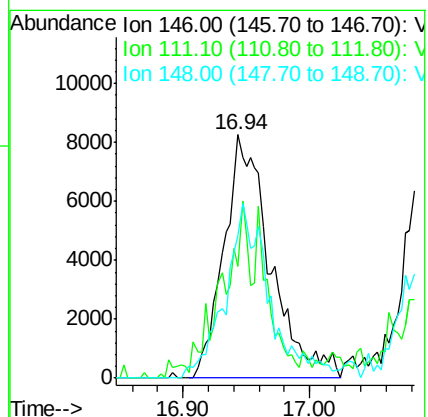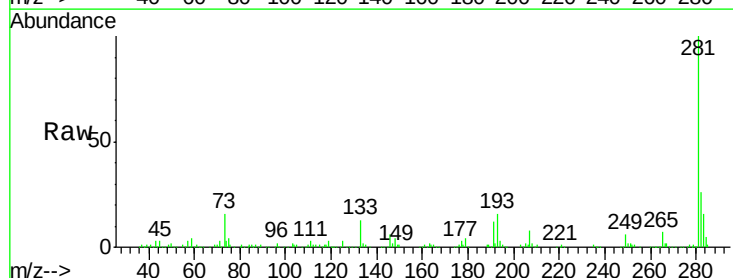




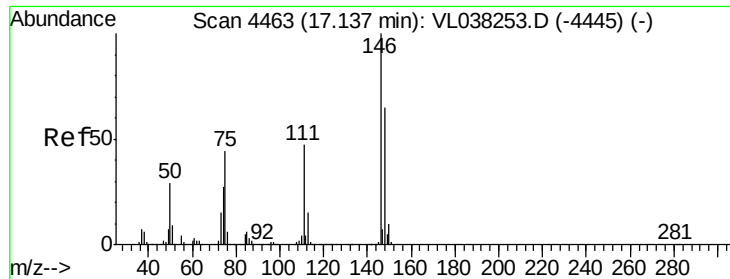


#76
 1,4-Dichlorobenzene
 Concen: 0.135 ppbv
 RT: 17.09
 Instrument: MSVOA_L
 Delta R.T.:
 Lab File: ClientSampleId:
 SVP-2DL
 Acq: 1 Feb 2022 13:44

Tgt Ion:1
 Ion Rati
 146 100
 111 65.
 148 72.




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 02/07/2022
 Supervised By :Mahesh Dadoda 02/07/2022

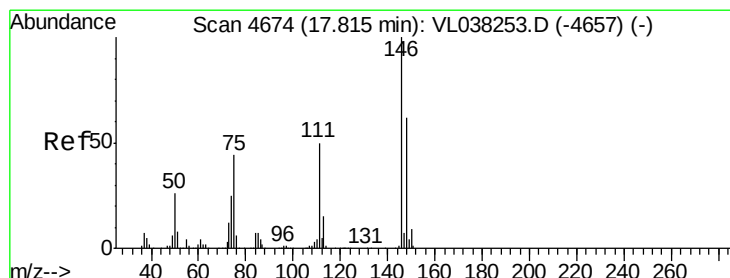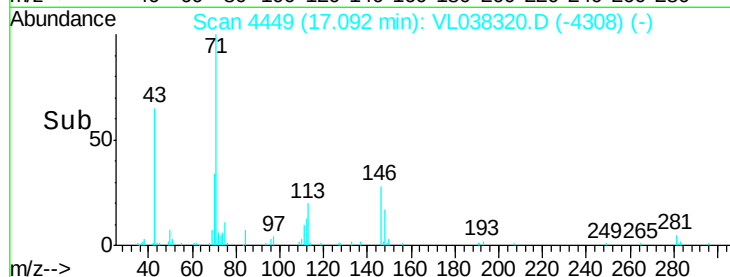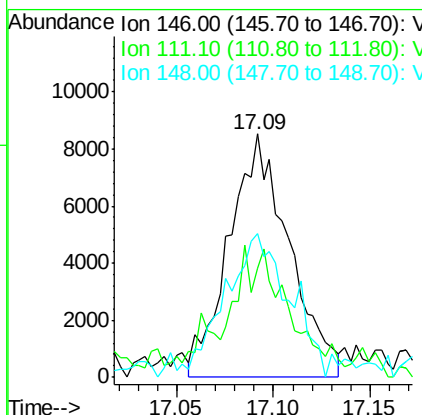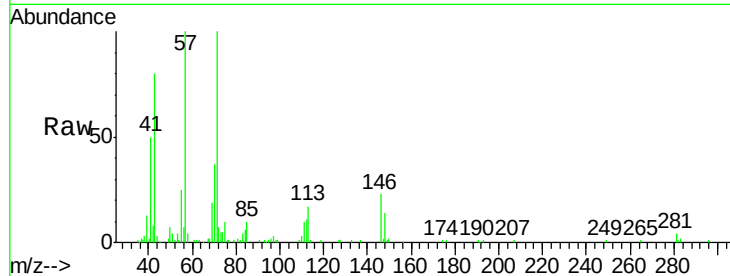

#77
 1,2-Dichlorobenzene
 Concen: 0.145 ppbv m
 RT: 17.77 min Scan# 4661
 Delta R.T. -0.04 min
 Lab File: VL038320.D
 Acq: 1 Feb 2022 13:44

Tgt Ion:146 Resp: 18924
 Ion Ratio Lower Upper
 146 100
 111 56.2 25.2 75.6
 148 67.4 32.6 97.8

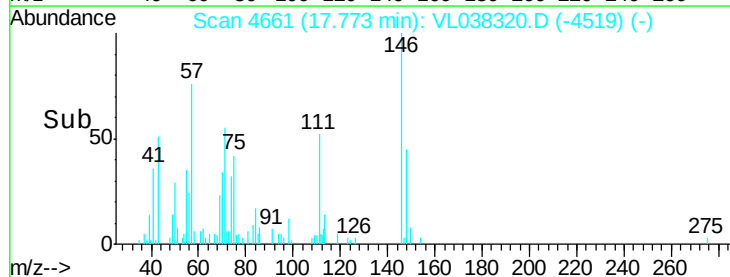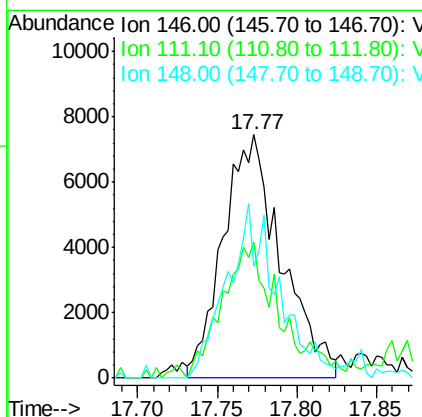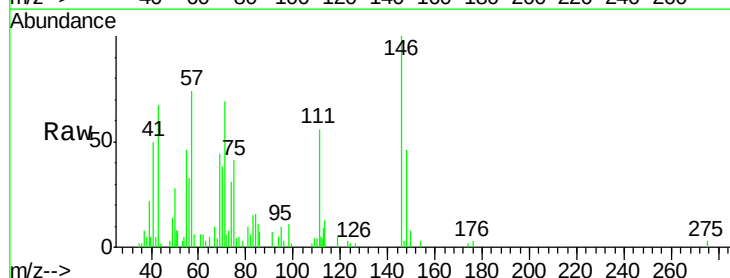




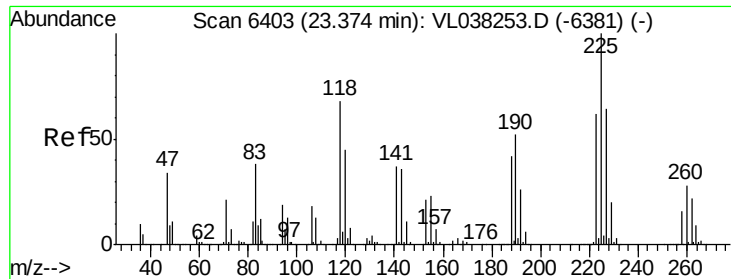


#78
Hexachloro-1,3-Butadiene
Concen: 0.183 ppbv m
RT: 23.33
Instrument: MSVOA_L
Delta R.T.:
Lab File: ClientSampleId :
Acq: 1 Feb 2022 13:44

Tgt Ion: 225
Ion Ratio: 100
223 0.
227 0.




Manual Integrations
APPROVED




Reviewed By : Semsettin Yesilyurt 02/07/2022
Supervised By : Mahesh Dadoda 02/07/2022

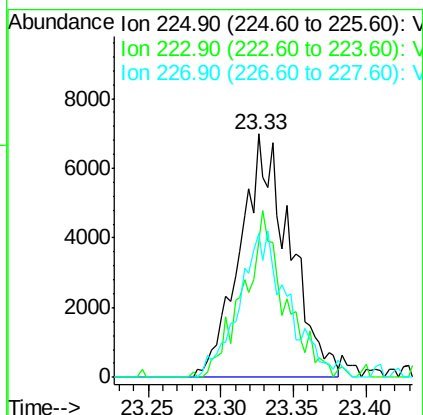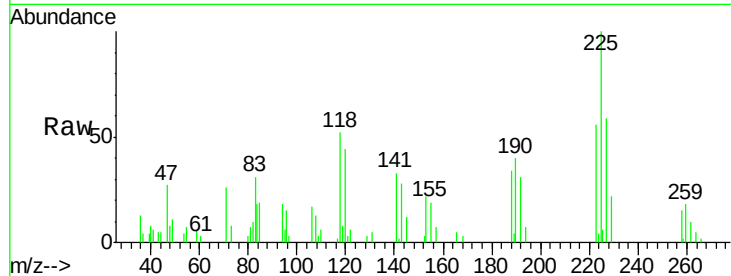

#79
Naphthalene
Concen: 0.141 ppbv m
RT: 22.16 min Scan# 6024
Delta R.T. -0.04 min
Lab File: VL038320.D
Acq: 1 Feb 2022 13:44

Tgt Ion: 128 Resp: 17241
Ion Ratio Lower Upper
128 100
127 14.8 9.7 14.5#
129 14.6 8.1 12.1#

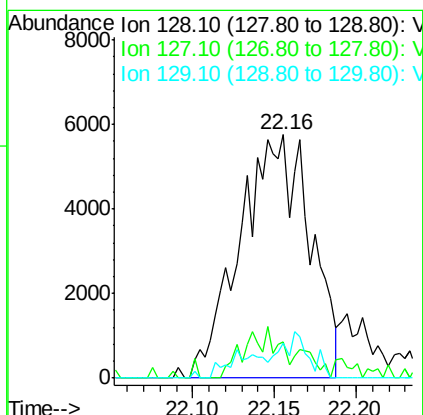

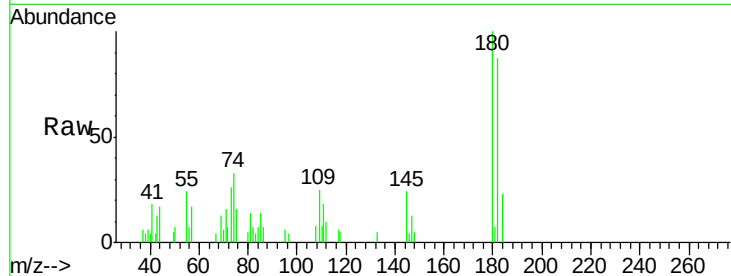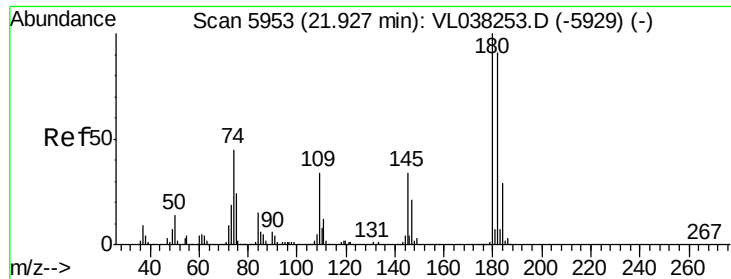

#81
 1,2,4-Trichlorobenzene
 Concen: 0.132 ppbv m
 RT: 21.89
 Delta R.T: MSVOA_L
 Lab File: ClientSampleId :
 SVP-2DL
 Acq: 1 Feb 2022 13.44

Tgt Ion:1
 Ion Rati
 180 100
 182 0.
 184 0.

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022
 Supervised By :Mahesh Dadoda 02/07/2022

