

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL020122\
 Data File : VL038325.D
 Acq On : 1 Feb 2022 17:34
 Operator : SY/AP
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010EC

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 02/07/2022
 Supervised By : Mahesh Dadoda 02/07/2022

Quant Time: Feb 02 06:49:56 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL012422A

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument:

QLast Update : Mon Jan 24 14:12:48 2022

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.64	49	854320	10.00	ppbv	-0.04
33) 1,4-Difluorobenzene	7.14	114	2530542	10.00	ppbv	-0.04
55) Chlorobenzene-d5	12.04	117	2332460m	10.00	ppbv	-0.04

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.37	95	1820091	10.28	ppbv	-0.04
Spiked Amount	10.000	Range	65 - 135	Recovery	=	102.80%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	3.03	85	1613653	8.873	ppbv	98
3) Chlorodifluoromethane	2.97	51	1458922	8.578	ppbv	99
4) Chloromethane	3.13	50	481734	8.233	ppbv	96
5) Vinyl Chloride	3.24	62	488466	8.364	ppbv	98
6) Bromomethane	3.46	94	181987	5.764	ppbv	97
7) Chloroethane	3.54	64	170434	8.641	ppbv	98
8) Dichlorotetrafluoroethane	3.17	85	1146922	8.150	ppbv	93
9) Propene	3.00	41	488791	8.829	ppbv	100
10) Heptane	8.09	43	1183423	8.308	ppbv	98
11) Trichlorofluoromethane	3.93	101	1127387	7.957	ppbv	99
12) 1,1,2-Trichlorotrifluoroet	4.46	101	859432	8.025	ppbv	96
13) Ethanol	3.58	45	56336m	9.479	ppbv	
14) Bromoethene	3.72	108	354647	8.474	ppbv	98
15) Acetone	3.83	43	689309	9.153	ppbv	99
16) 1,3-Butadiene	3.31	39	499681	9.246	ppbv	93
17) tert-Butyl alcohol	4.26	59	650126	7.865	ppbv	97
18) 1,1-Dichloroethene	4.27	96	389534	8.364	ppbv	99
19) Isopropyl Alcohol	3.94	45	371391	7.883	ppbv #	97
20) Methylene Chloride	4.32	84	311261	7.106	ppbv	97
21) Allyl Chloride	4.39	41	522322	7.839	ppbv	96
22) trans-1,2-Dichloroethene	4.86	96	387092	8.044	ppbv	97
23) Vinyl Acetate	5.04	43	944238	8.623	ppbv	99
24) 1,1-Dichloroethane	4.98	63	810864	8.312	ppbv	99
25) Ethyl Acetate	5.65	43	1758118	8.338	ppbv	99
26) Hexane	5.66	57	876133	8.933	ppbv	92
27) Carbon Disulfide	4.53	76	903077	7.871	ppbv	100
28) Methyl tert-Butyl Ether	5.01	73	864398	8.496	ppbv	99
29) Chloroform	5.72	83	1337155	8.353	ppbv	97
30) Cyclohexane	7.10	84	787689	9.224	ppbv	94
31) cis-1,2-Dichloroethene	5.52	61	843192	9.856	ppbv	97
32) 1,1,1-Trichloroethane	6.48	97	1343407	8.402	ppbv	97
34) 2-Butanone	5.21	43	626175	7.567	ppbv	99
35) Carbon Tetrachloride	6.98	117	1338101	7.533	ppbv	97
36) Benzene	6.85	78	1881468	8.406	ppbv	98
37) 1,2-Dichloroethane	6.27	62	969380	7.561	ppbv #	96
38) Trichloroethene	7.80	130	678989	8.143	ppbv	98
39) 1,2-Dichloropropane	7.57	63	731429	8.060	ppbv	98
40) 1,4-Dioxane	7.80	88	172333	7.890	ppbv #	1
41) Tetrahydrofuran	6.02	42	429565	7.722	ppbv	98
42) Bromodichloromethane	7.75	83	1468325	7.719	ppbv	99
43) Methyl Methacrylate	7.98	69	697960	8.816	ppbv	96

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL020122\
 Data File : VL038325.D
 Acq On : 1 Feb 2022 17:34
 Operator : SY/AP
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010EC

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 02/07/2022
 Supervised By : Mahesh Dadoda 02/07/2022

Quant Time: Feb 02 06:49:56 2022

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL012422A


Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument:

QLast Update : Mon Jan 24 14:12:48 2022

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 2,2,4-Trimethylpentane	7.83	57	3137965	7.955	ppbv	99
45) t-1,3-Dichloropropene	9.24	75	233337	3.627	ppbv	96
46) cis-1,3-Dichloropropene	8.66	75	407591	4.749	ppbv	96
47) 1,1,2-Trichloroethane	9.44	97	757711	8.497	ppbv	96
48) Dibromochloromethane	10.26	129	1251533	8.337	ppbv	100
49) Bromoform	13.00	173	964511	8.912	ppbv	99
50) 4-Methyl-2-Pentanone	8.70	43	1284861	8.703	ppbv	99
51) 2-Hexanone	10.09	43	627254	9.647	ppbv #	91
52) Tetrachloroethene	11.18	164	616688	7.994	ppbv	99
53) Toluene	9.76	91	2127662	8.588	ppbv	97
54) 1,2-Dibromoethane	10.57	107	1023830	8.076	ppbv	98
56) 1,1,1,2-Tetrachloroethane	12.08	131	826000	8.091	ppbv #	52
57) Chlorobenzene	12.10	112	1505729	8.067	ppbv	95
58) Ethyl Benzene	12.67	91	2788751	8.135	ppbv	97
59) m/p-Xylene	12.96	91	4492321m	15.360	ppbv	
60) o-Xylene	13.65	91	2132073	7.838	ppbv	97
61) Styrene	13.48	104	1094156	8.619	ppbv	97
62) Isopropylbenzene	14.62	105	3043906	8.394	ppbv	99
63) 1,1,2,2-Tetrachloroethane	13.63	83	1533025	7.617	ppbv	99
64) n-propylbenzene	15.52	120	772242	8.853	ppbv	90
65) tert-Butylbenzene	16.70	119	2568010	8.598	ppbv	96
66) Benzyl Chloride	16.94	91	33713m	2.485	ppbv	
67) sec-Butylbenzene	17.25	105	3564585	8.580	ppbv	99
69) p-Isopropyltoluene	17.61	119	2798662	8.802	ppbv	99
70) n-Butylbenzene	18.50	91	2703664	8.682	ppbv	99
71) 2-Chlorotoluene	15.41	91	2208085	8.221	ppbv	99
72) 4-Ethyltoluene	15.80	105	2410178	8.473	ppbv	99
73) 1,3,5-Trimethylbenzene	15.95	105	2124137	8.304	ppbv	100
74) 1,2,4-Trimethylbenzene	16.72	105	2147585	7.969	ppbv	97
75) 1,3-Dichlorobenzene	16.95	146	1209179	8.361	ppbv	99
76) 1,4-Dichlorobenzene	17.09	146	1150908	8.220	ppbv	98
77) 1,2-Dichlorobenzene	17.77	146	1156567	8.611	ppbv	100
78) Hexachloro-1,3-Butadiene	23.33	225	661043	7.078	ppbv	99
79) Naphthalene	22.15	128	1028211	8.160	ppbv	98
80) Naphthalene,2-methyl-	24.94	142	132788	9.691	ppbv #	83
81) 1,2,4-Trichlorobenzene	21.87	180	592544m	7.995	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.64 Instrument: MSVOA_L

Delta R.T.

Lab File: ClientSampleId:

Acq: 1 Feb 2022 17:34 VSTDCCC010EC

Tgt Ion:

Ion Ratio

49 100

128 54.





130 65.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022

Supervised By :Mahesh Dadoda 02/07/2022

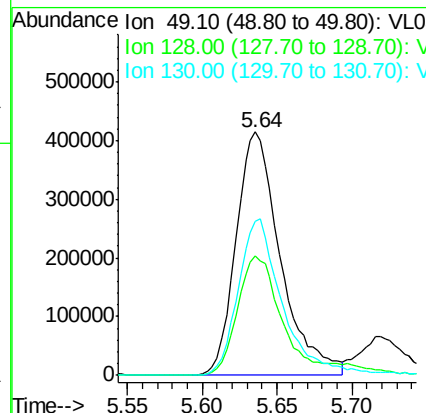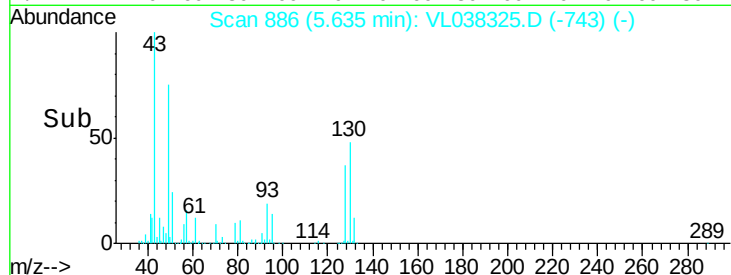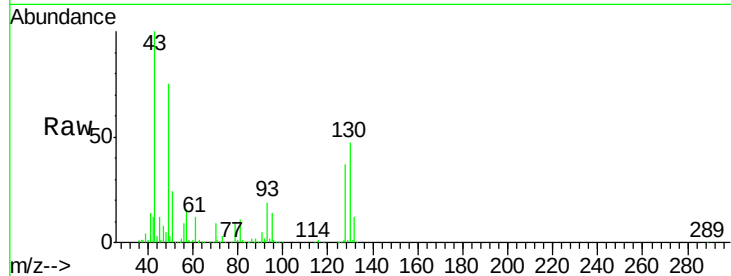

#2

Dichlorodifluoromethane

Concen: 8.873 ppbv

RT: 3.03 min Scan# 77

Delta R.T. -0.03 min

Lab File: VL038325.D




Acq: 1 Feb 2022 17:34


Tgt Ion: 85 Resp: 1613653

Ion Ratio Lower Upper

85 100

87 32.9 27.0 40.6

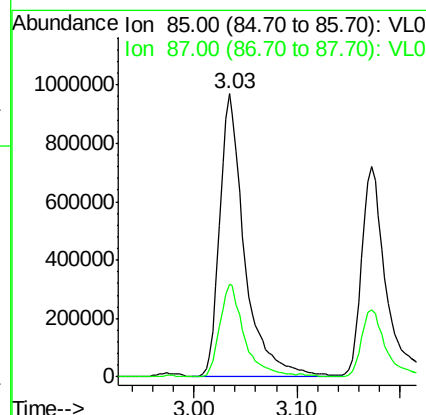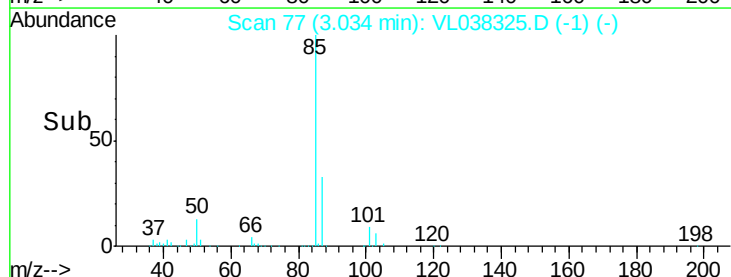

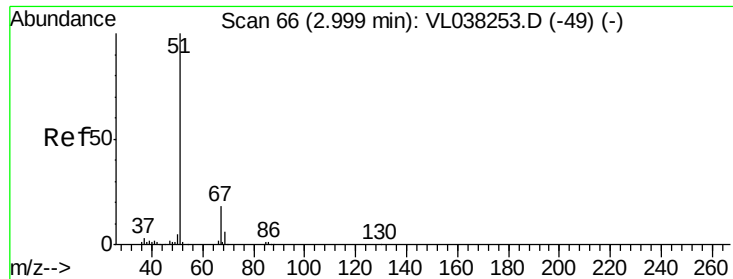

#3

Chlorodifluoromethane

Concen: 8.578 ppbv

RT: 2.97 Instrument :

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

Acq: 1 Feb 2022 17:34 VSTDCCC010EC

Tgt Ion:

Ion Ratio

51 100


67 17.

Manual Integrations

APPROVED




Reviewed By :Semsettin Yesilyurt 02/07/2022

Supervised By :Mahesh Dadoda 02/07/2022

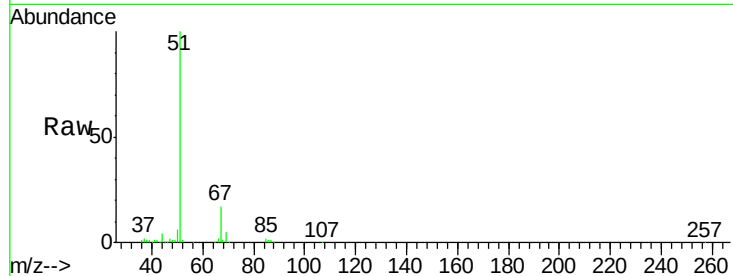

Abundance Ion 51.00 (50.70 to 51.70): VL0

Ion 67.00 (66.70 to 67.70): VL0

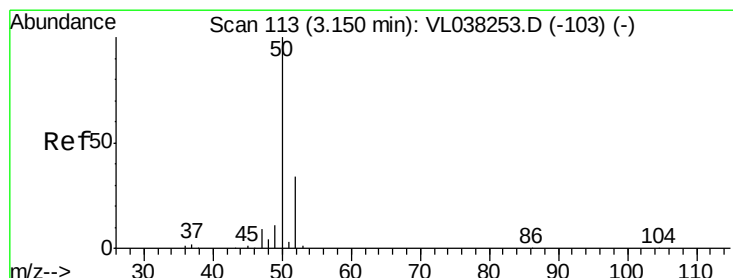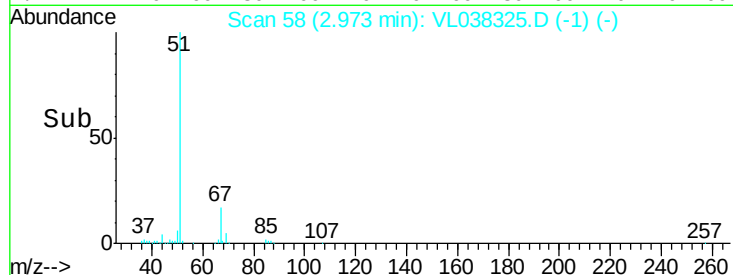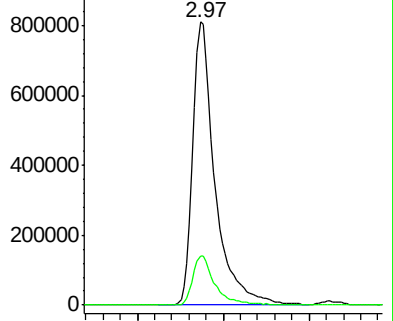

#4

Chloromethane

Concen: 8.233 ppbv

RT: 3.13 min Scan# 106

Delta R.T. -0.02 min

Lab File: VL038325.D


Acq: 1 Feb 2022 17:34

Tgt Ion: 50 Resp: 481734

Ion Ratio Lower Upper



50 100


52 31.4 27.1 40.7

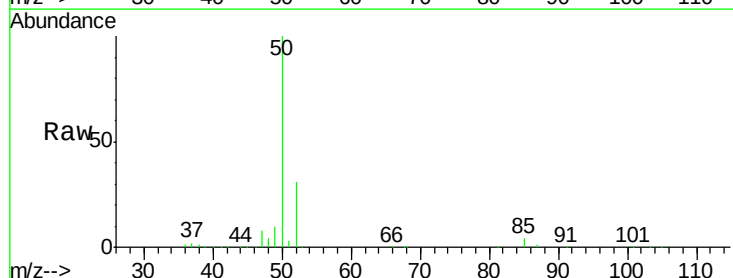

Abundance Ion 50.10 (49.80 to 50.80): VL0

Ion 52.10 (51.80 to 52.80): VL0

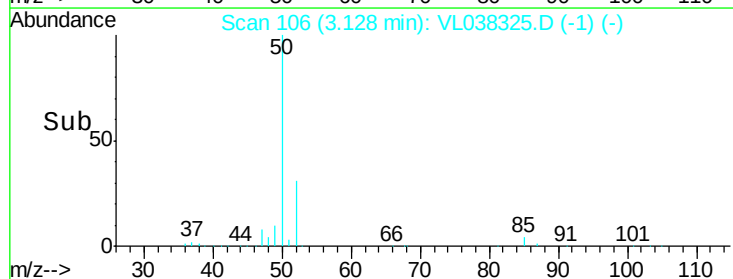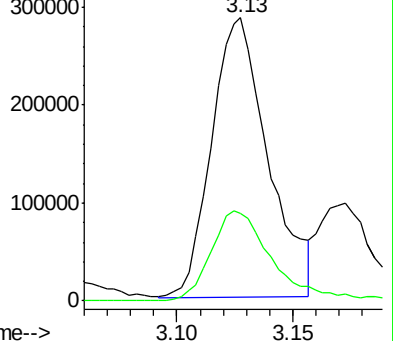

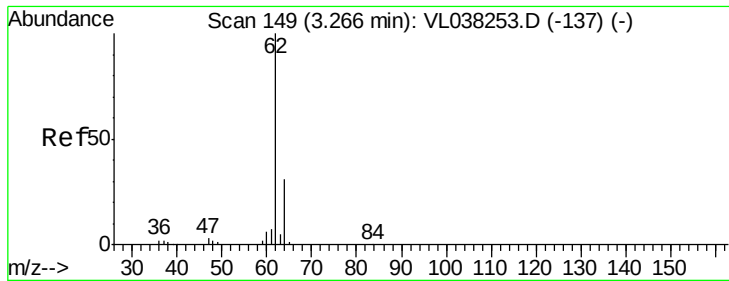

#5

Vinyl Chloride

Concen: 8.364 ppbv

RT: 3.24

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

Acq: 1 Feb 2022 17:34

Tgt Ion:

Ion Ratio

62 100





64 29.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022

Supervised By :Mahesh Dadoda 02/07/2022

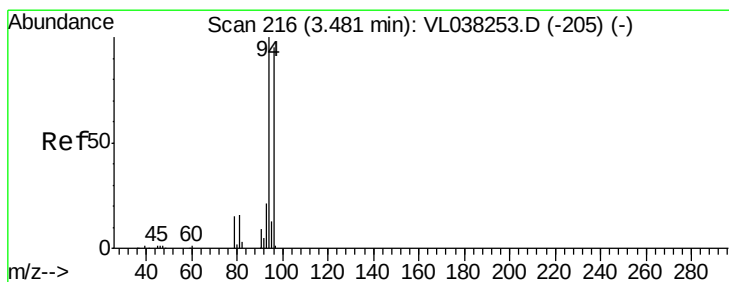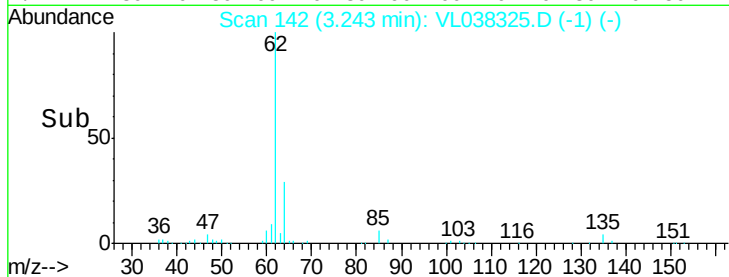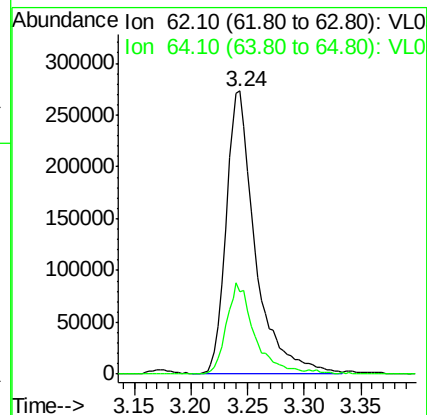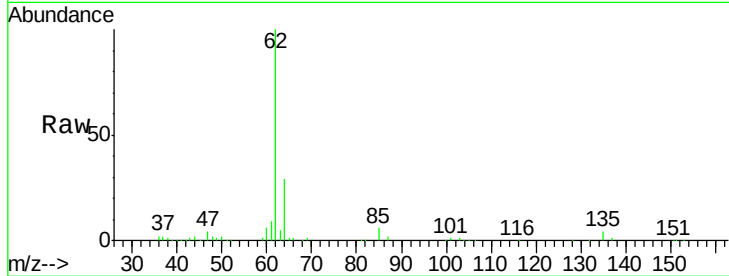

#6

Bromomethane

Concen: 5.764 ppbv

RT: 3.46 min Scan# 209

Delta R.T. -0.02 min

Lab File: VL038325.D




Acq: 1 Feb 2022 17:34


Tgt Ion: 94 Resp: 181987

Ion Ratio Lower Upper

94 100

96 92.4 76.0 114.0

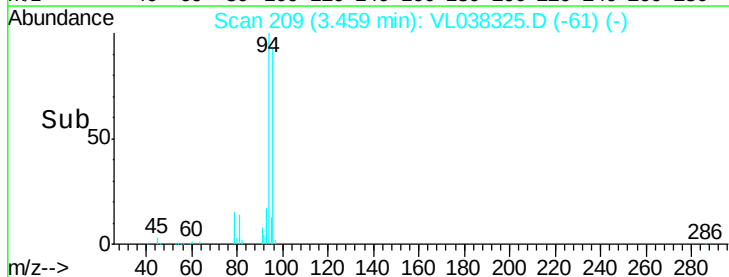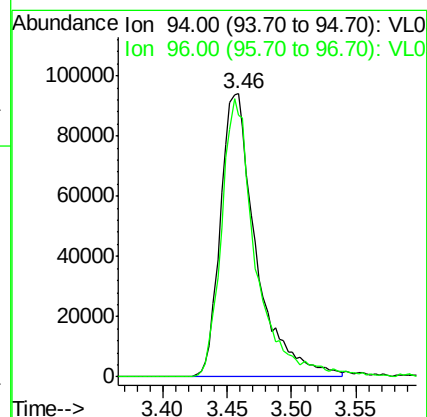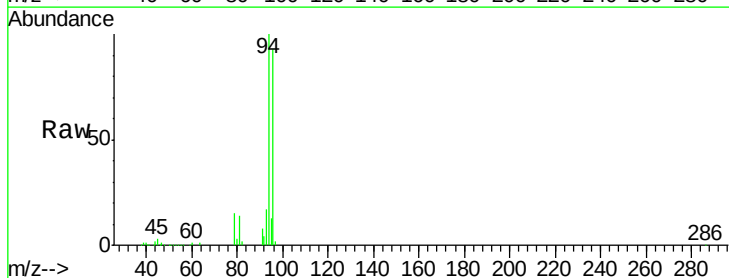



#7

Chloroethane

Concen: 8.641 ppbv

RT: 3.54 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 1 Feb 2022 17:34 VSTDCCC010EC

Tgt Ion:

Ion Ratio

64 100





66 33.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022

Supervised By :Mahesh Dadoda 02/07/2022

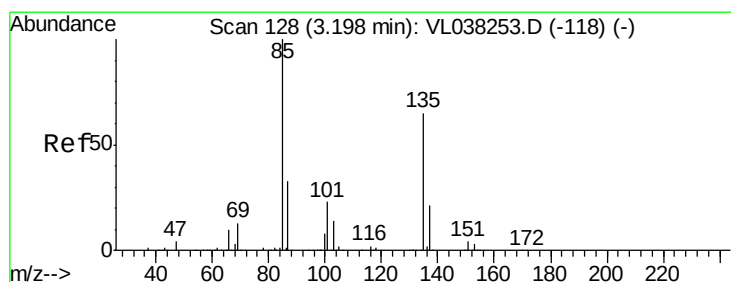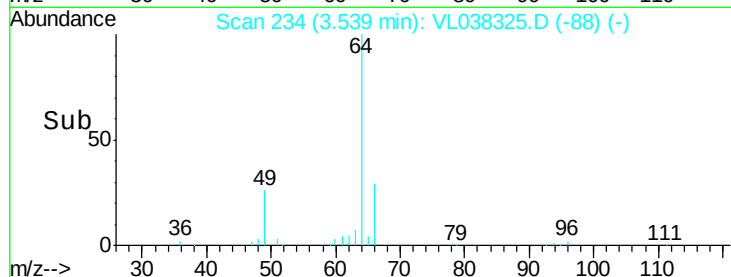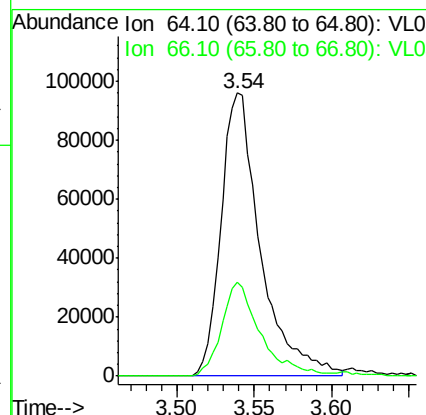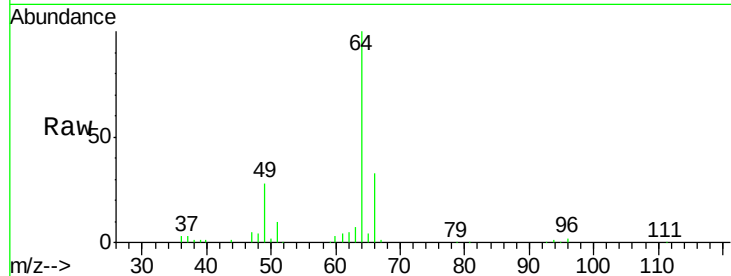

#8

Dichlorotetrafluoroethane

Concen: 8.150 ppbv

RT: 3.17 min Scan# 120

Delta R.T. -0.03 min

Lab File: VL038325.D




Acq: 1 Feb 2022 17:34


Tgt Ion: 85 Resp: 1146922

Ion Ratio Lower Upper

85 100

135 72.4 53.7 80.5

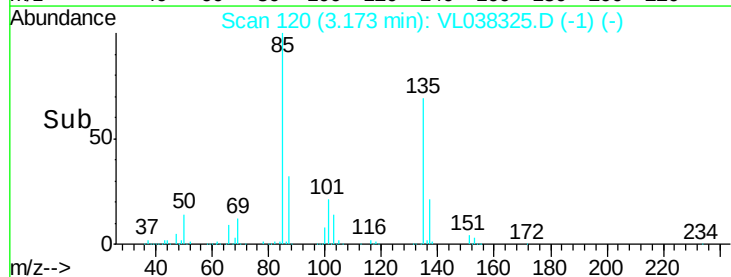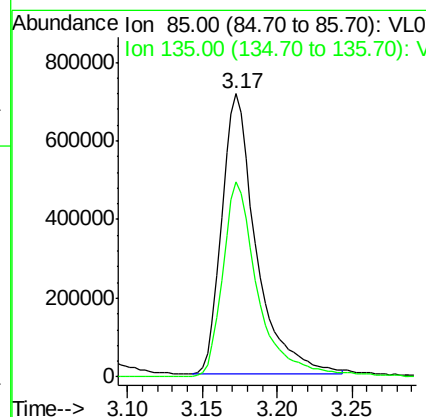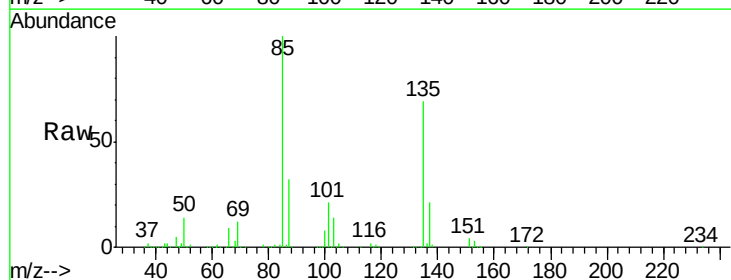







#9
 Propene
 Concen: 8.829 ppbv
 RT: 3.00
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId :
 VSTDCCC010EC
 Acq: 1 Feb 2022 17:34

Tgt Ion:
 Ion Ratio
 41 100
 42 68.




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 02/07/2022
 Supervised By :Mahesh Dadoda 02/07/2022

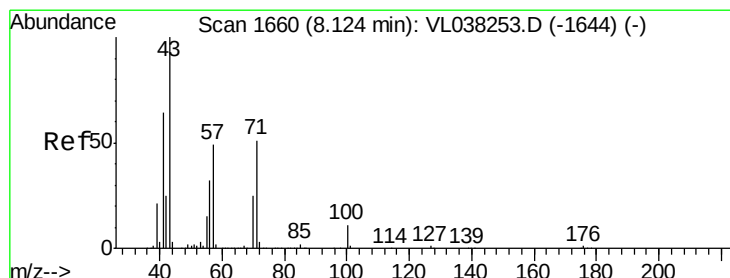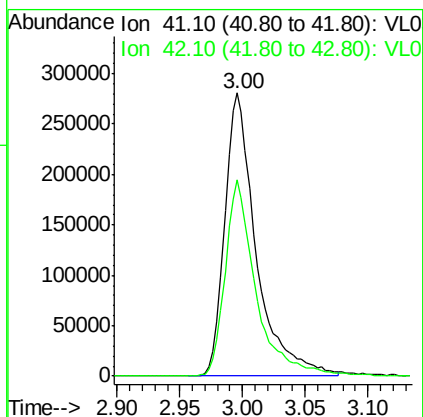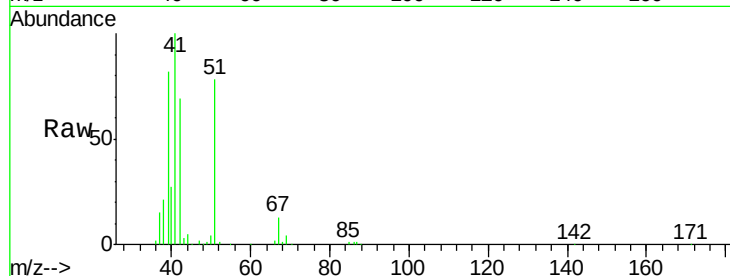

#10
 Heptane
 Concen: 8.308 ppbv
 RT: 8.09 min Scan# 1648
 Delta R.T. -0.04 min
 Lab File: VL038325.D
 Acq: 1 Feb 2022 17:34

Tgt Ion: 43 Resp: 1183423
 Ion Ratio Lower Upper
 43 100
 57 50.6 39.5 59.3

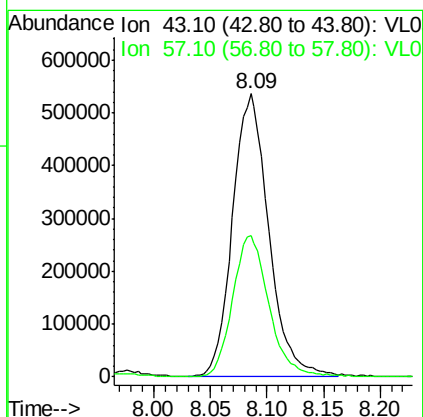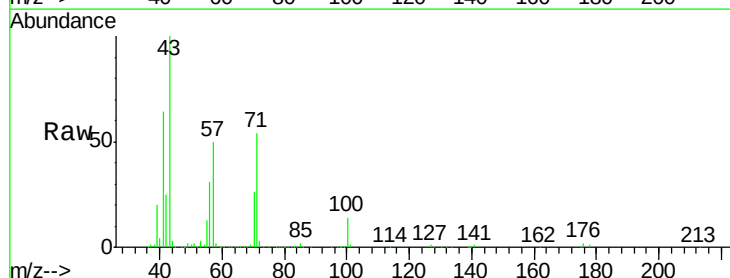




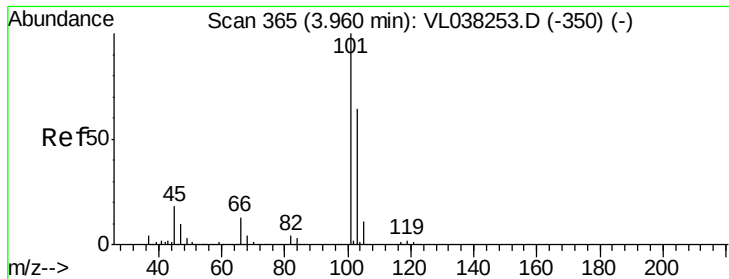


#11
 Trichlorofluoromethane
 Concen: 7.957 ppbv
 RT: 3.93
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId :
 VSTDCCC010EC
 Acq: 1 Feb 2022 17:34

Tgt Ion:1
 Ion Ratio
 101 100
 103 65.




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 02/07/2022
 Supervised By :Mahesh Dadoda 02/07/2022

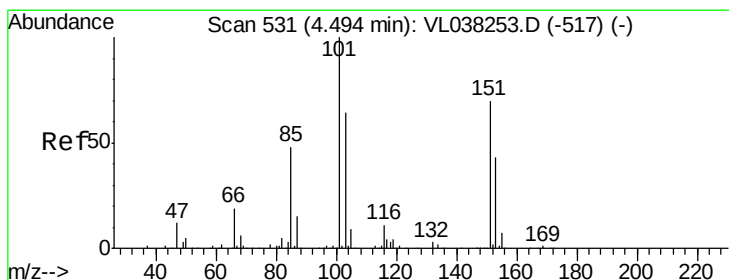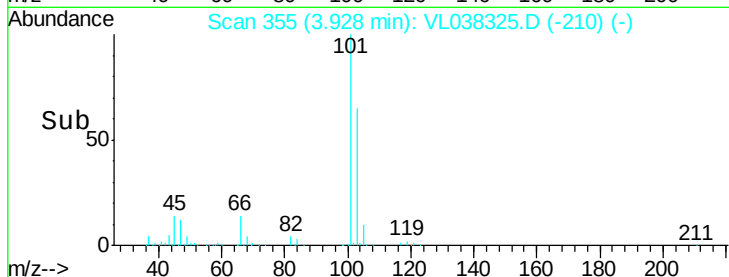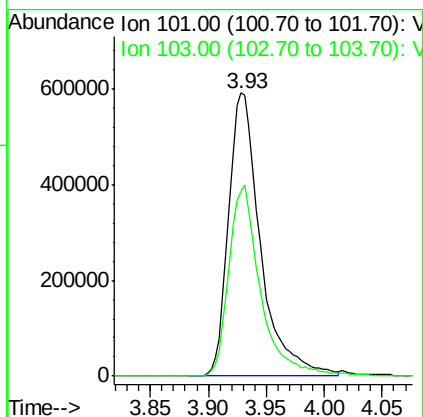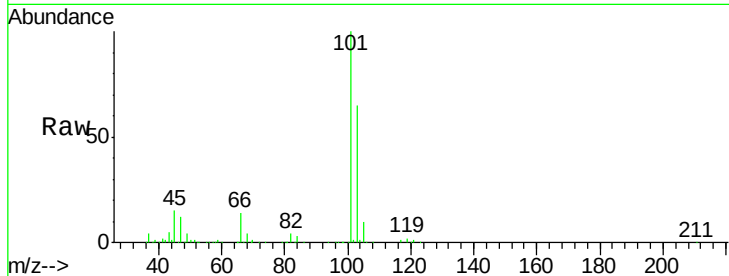

#12
 1,1,2-Trichlorotrifluoroethane
 Concen: 8.025 ppbv
 RT: 4.46 min Scan# 520
 Delta R.T. -0.04 min
 Lab File: VL038325.D
 Acq: 1 Feb 2022 17:34

Tgt Ion:101 Resp: 859432
 Ion Ratio Lower Upper
 101 100
 151 72.5 55.3 82.9

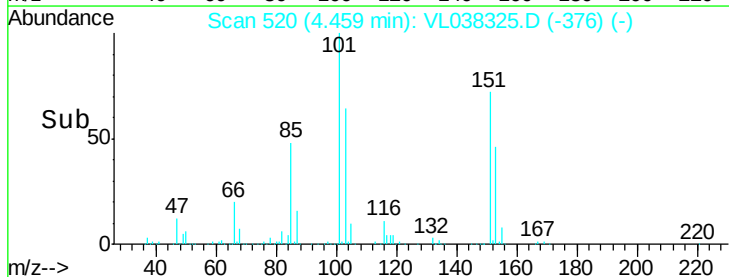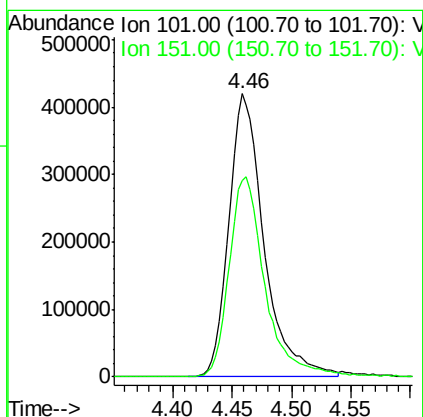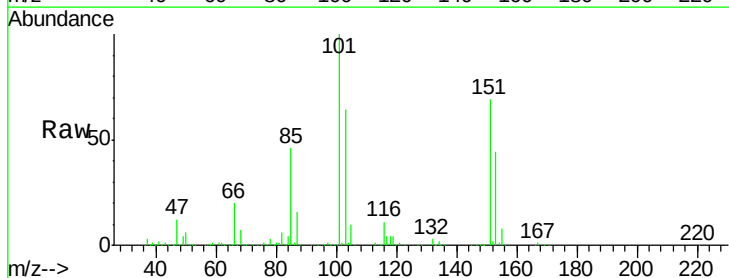







#13
Ethanol
Concen: 9.479 ppbv m
RT: 3.58
Delta R.T. MSVOA_L
Lab File: ClientSampleId :
Acq: 1 Feb 2022 17:34

Tgt Ion:
Ion Ratio
45 100
46 43.




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/07/2022
Supervised By :Mahesh Dadoda 02/07/2022

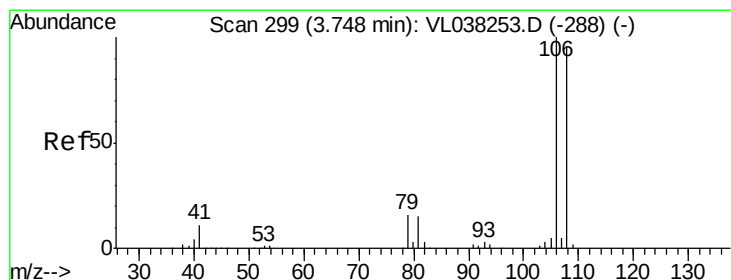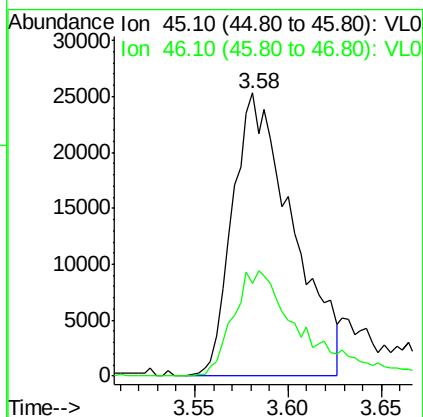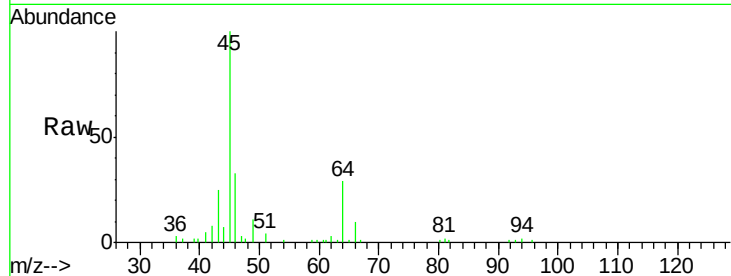

#14
Bromoethene
Concen: 8.474 ppbv
RT: 3.72 min Scan# 291
Delta R.T. -0.03 min
Lab File: VL038325.D
Acq: 1 Feb 2022 17:34

Tgt Ion:108 Resp: 354647
Ion Ratio Lower Upper
108 100
106 110.3 86.4 129.6
79 17.0 14.1 21.1

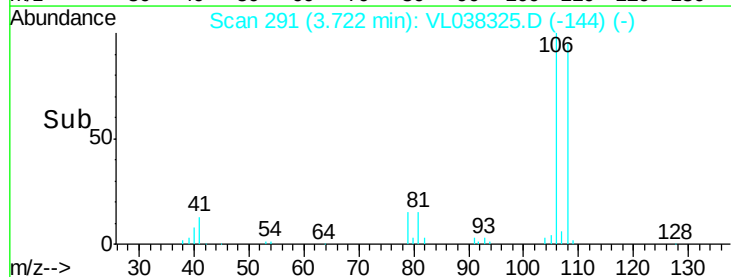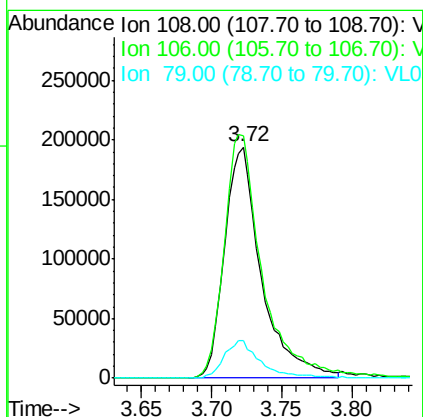



#15

Acetone

Concen: 9.153 ppbv

RT: 3.83

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

Acq: 1 Feb 2022 17:34 VSTDC010EC

Tgt Ion:

Ion Ratio

43 100





58 27.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022

Supervised By :Mahesh Dadoda 02/07/2022

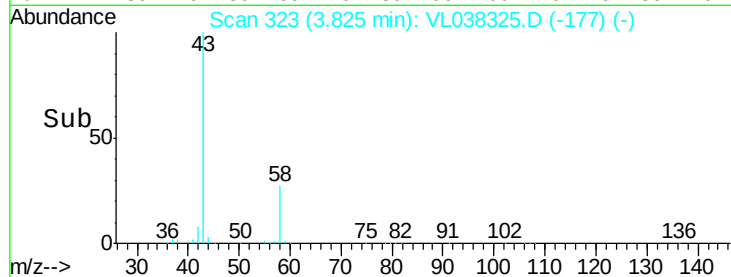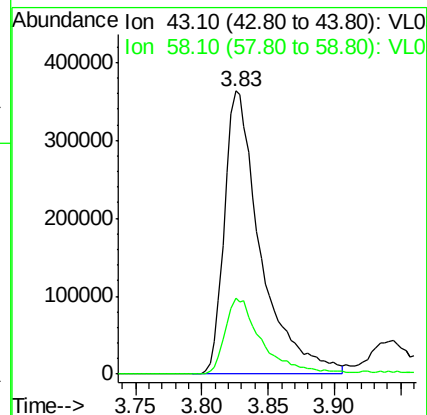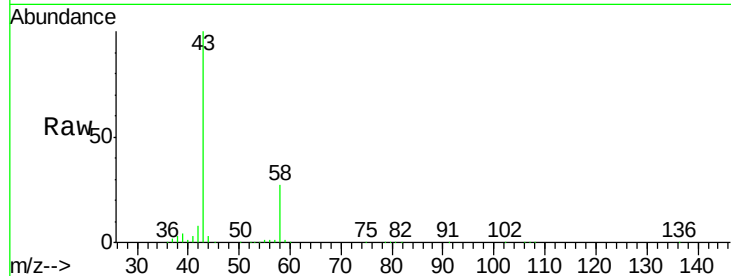

#16

1,3-Butadiene

Concen: 9.246 ppbv

RT: 3.31 min Scan# 163

Delta R.T. -0.03 min

Lab File: VL038325.D




Acq: 1 Feb 2022 17:34


Tgt Ion: 39 Resp: 499681

Ion Ratio Lower Upper

39 100

54 71.8 62.6 94.0

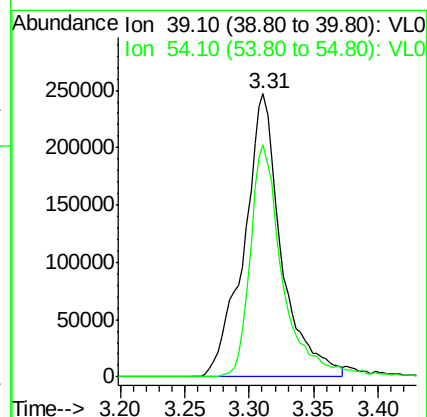

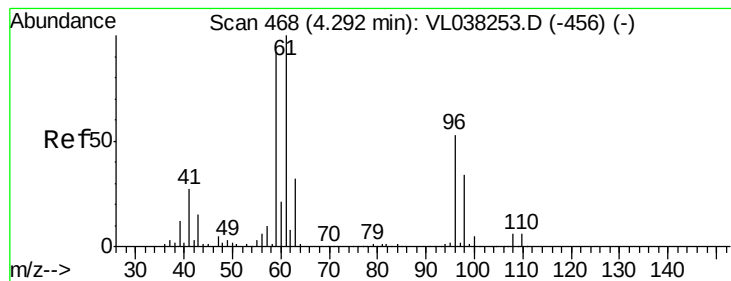

#17

tert-Butyl alcohol

Concen: 7.865 ppbv

RT: 4.26 Instrument :

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

Acq: 1 Feb 2022 17:34 VSTDCC010EC

Tgt Ion:

Ion Ratio

59 100





57 10.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022

Supervised By :Mahesh Dadoda 02/07/2022

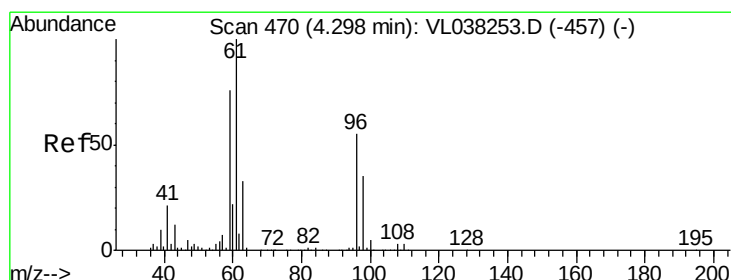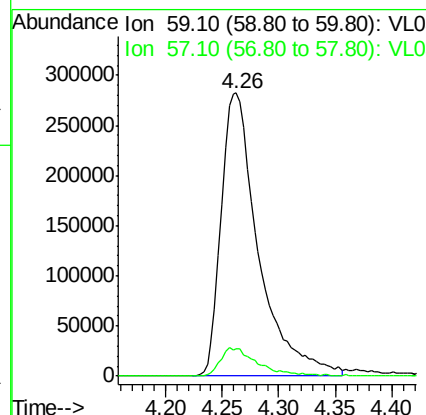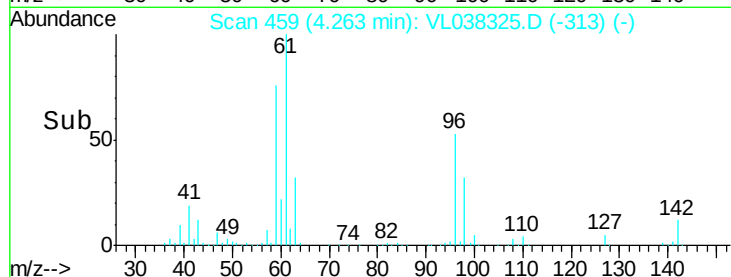

#18

1,1-Dichloroethene

Concen: 8.364 ppbv

RT: 4.27 min Scan# 460

Delta R.T. -0.03 min

Lab File: VL038325.D

Acq: 1 Feb 2022 17:34




Tgt Ion: 96 Resp: 389534


Ion Ratio Lower Upper

96 100

61 182.4 146.5 219.7

98 62.3 51.9 77.9

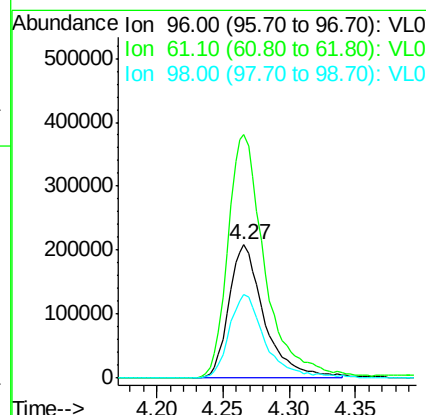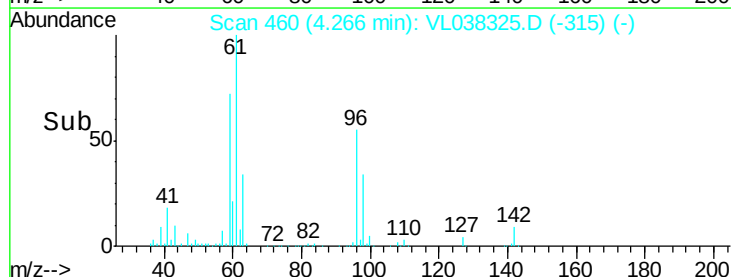




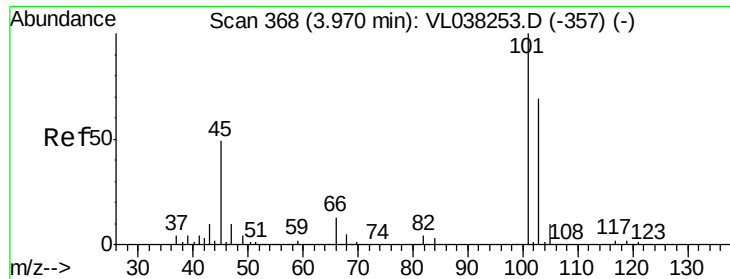


#19
Isopropyl Alcohol
Concen: 7.883 ppbv
RT: 3.94
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId :
VSTDCCC010EC
Acq: 1 Feb 2022 17:34

Tgt Ion:
Ion Ratio
45 100
58 1.




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/07/2022
Supervised By :Mahesh Dadoda 02/07/2022

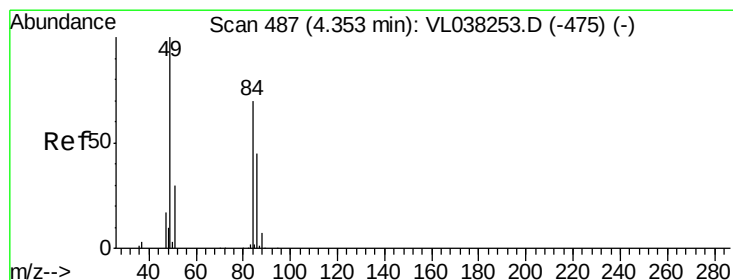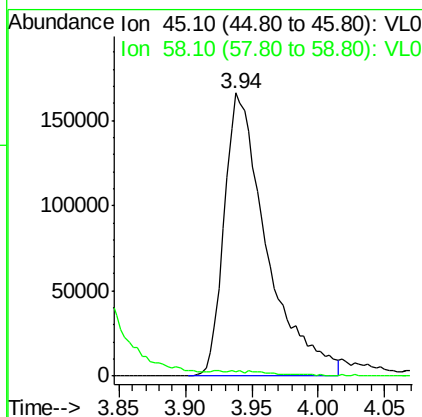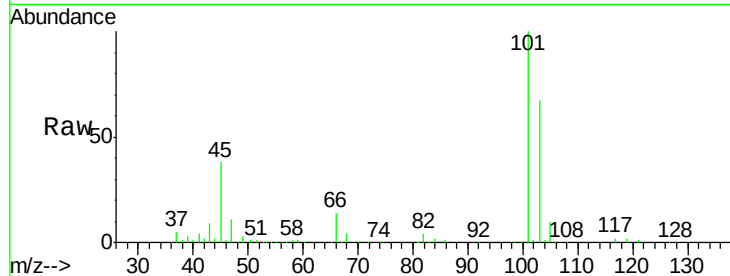

#20
Methylene Chloride
Concen: 7.106 ppbv
RT: 4.32 min Scan# 477
Delta R.T. -0.03 min
Lab File: VL038325.D
Acq: 1 Feb 2022 17:34

Tgt Ion: 84 Resp: 311261
Ion Ratio Lower Upper
84 100
49 149.3 115.0 172.6
51 44.6 35.0 52.6
86 65.1 51.4 77.0

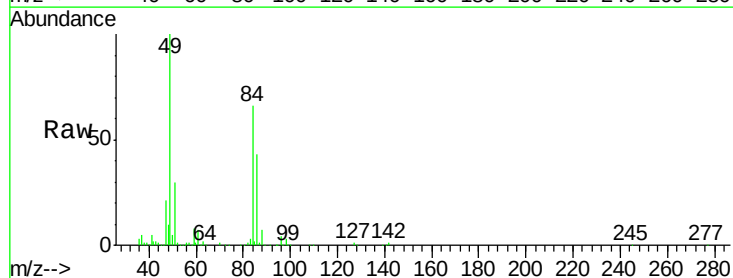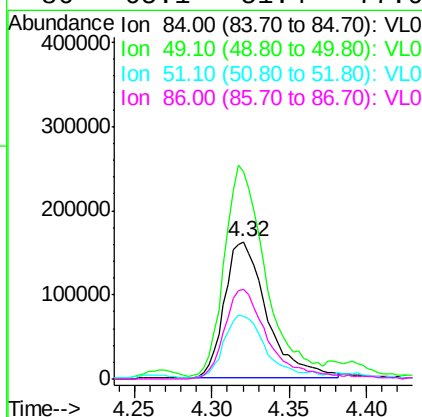







#21
 Allyl Chloride
 Concen: 7.839 ppbv
 RT: 4.39
 Instrument: MSVOA_1
 Delta R.T.:
 Lab File: ClientSampleId:
 VSTDCCC010EC
 Acq: 1 Feb 2022 17:34

Tgt Ion:
 Ion Ratio
 41 100
 76 29.
 39 74.




Manual Integrations
 APPROVED







Reviewed By :Semsettin Yesilyurt 02/07/2022
 Supervised By :Mahesh Dadoda 02/07/2022

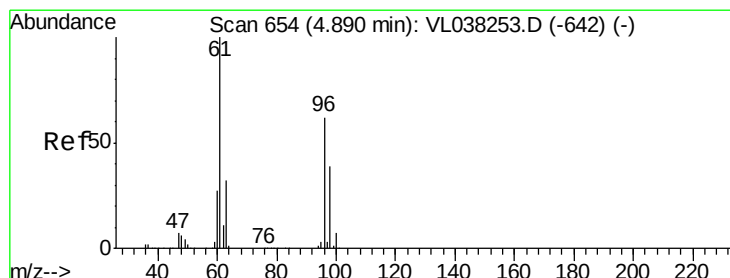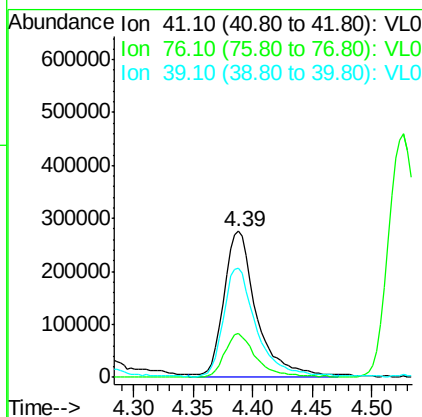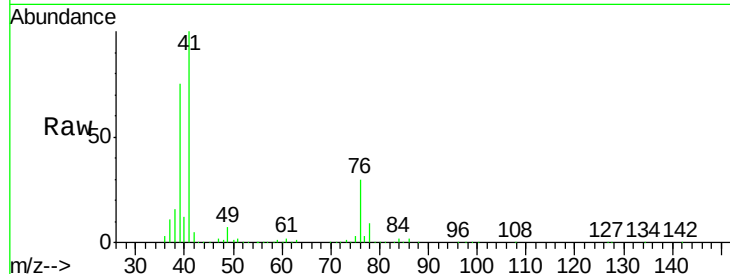

#22
 trans-1,2-Dichloroethene
 Concen: 8.044 ppbv
 RT: 4.86 min Scan# 645
 Delta R.T. -0.03 min
 Lab File: VL038325.D
 Acq: 1 Feb 2022 17:34

Tgt Ion: 96 Resp: 387092
 Ion Ratio Lower Upper
 96 100
 61 155.3 128.8 193.2
 98 62.2 49.8 74.8

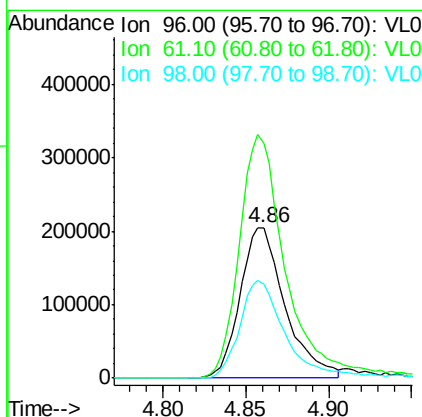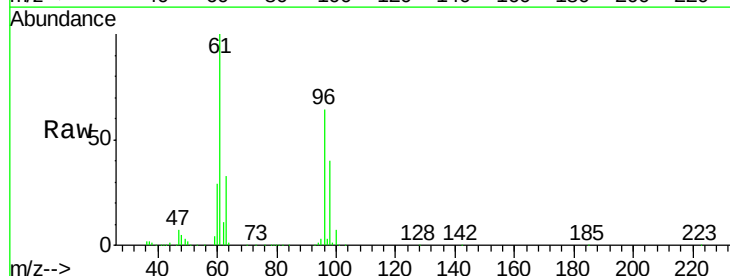

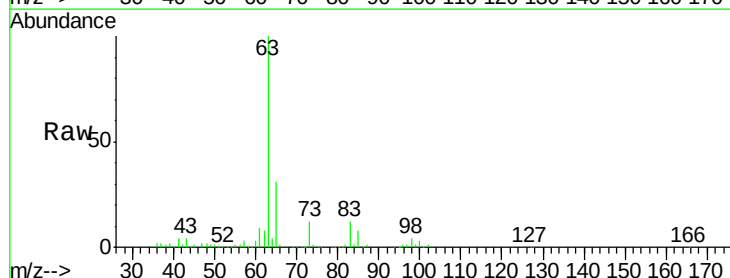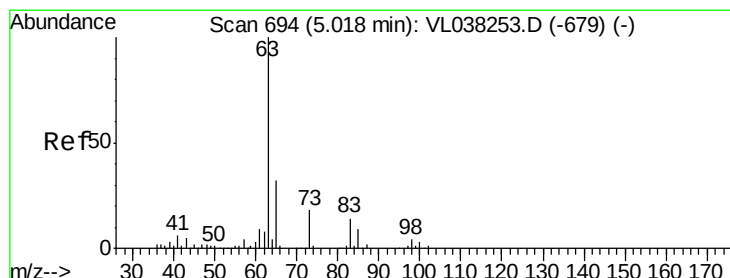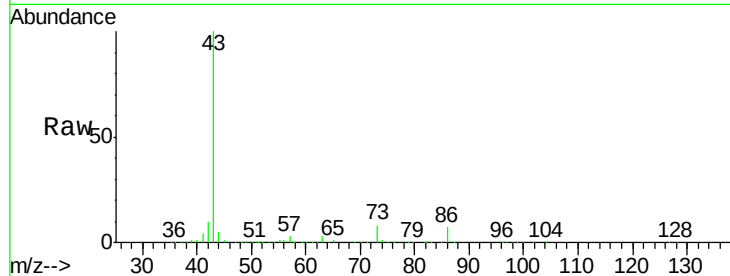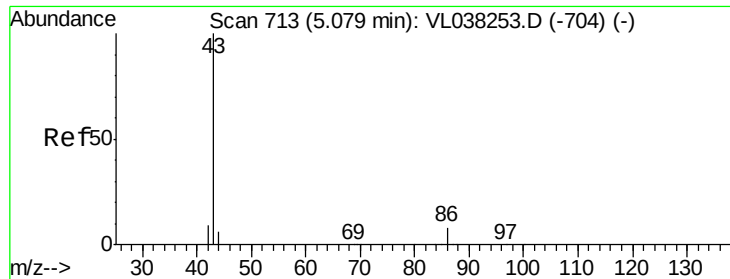

#23

Vinyl Acetate

Concen: 8.623 ppbv

RT: 5.04 Instrument: MSVOA_1

Delta R.T. ClientSampleId:

Lab File: VSTDCCC010EC

Acq: 1 Feb 2022 17:34

Tgt Ion:

Ion Ratio

43 100

86 7.

42 9.


44 4.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022

Supervised By :Mahesh Dadoda 02/07/2022

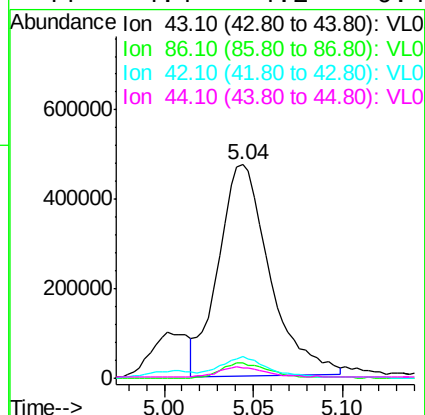

#24

1,1-Dichloroethane

Concen: 8.312 ppbv

RT: 4.98 min Scan# 683

Delta R.T. -0.04 min

Lab File: VL038325.D

Acq: 1 Feb 2022 17:34


Tgt Ion: 63 Resp: 810864


Ion Ratio Lower Upper

63 100

98 4.1 2.3 6.8

100 2.6 1.3 3.9

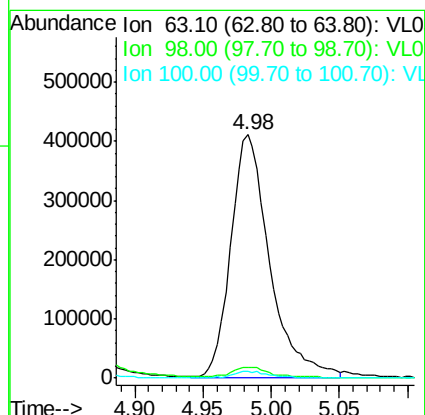







#25
Ethyl Acetate
Concen: 8.338 ppbv
RT: 5.65
Instrument: MSVOA_L
Delta R.T.:
Lab File: ClientSampleId :
Acq: 1 Feb 2022 17:34
VSTDCCC010EC

Tgt Ion:
Ion Ratio
43 100
45 9.
61 9.
70 6.8 5.4 8.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 02/07/2022
Supervised By :Mahesh Dadoda 02/07/2022

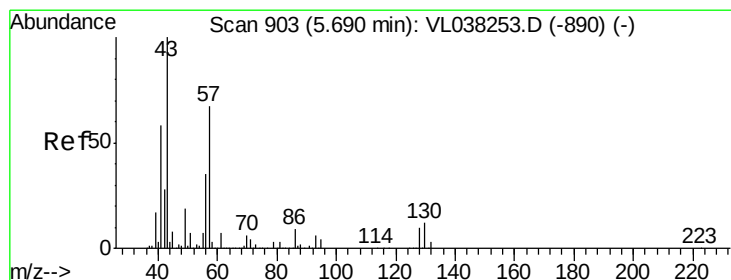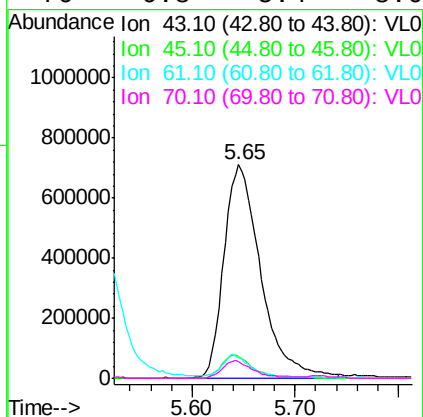

#26
Hexane
Concen: 8.933 ppbv
RT: 5.66 min Scan# 893
Delta R.T. -0.03 min
Lab File: VL038325.D
Acq: 1 Feb 2022 17:34

Tgt Ion: 57 Resp: 876133
Ion Ratio Lower Upper
57 100
41 87.9 72.8 109.2
43 203.7 177.0 265.6
56 52.1 43.3 64.9

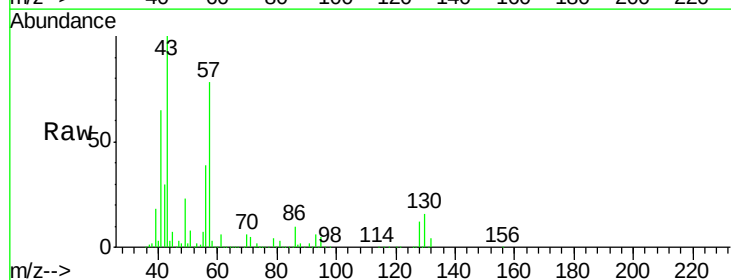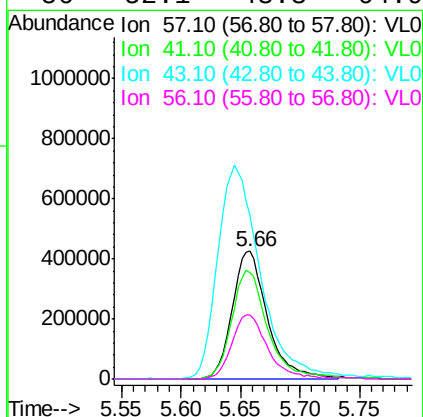



#27

Carbon Disulfide

Concen: 7.871 ppbv

RT: 4.53

Delta R.T. MSVOA_L

Lab File: ClientSampleId :

Acq: 1 Feb 2022 17:34 VSTDCCC010EC

Tgt Ion:

Ion Ratio

76 100

44 18.





78 9.

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022

Supervised By :Mahesh Dadoda 02/07/2022

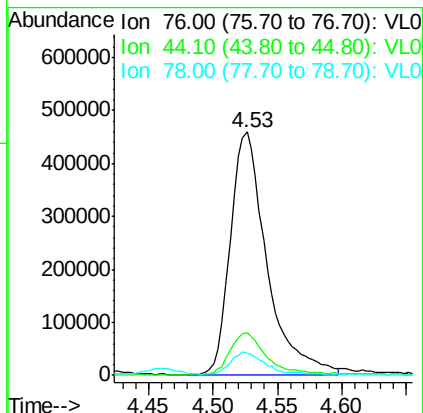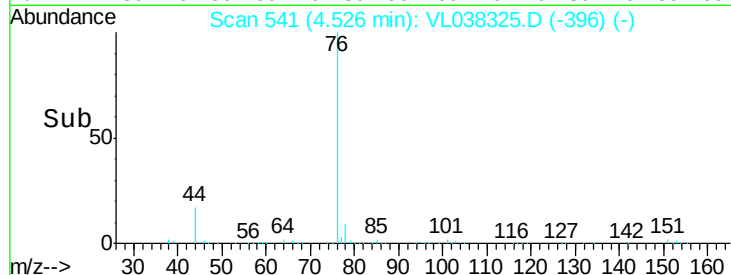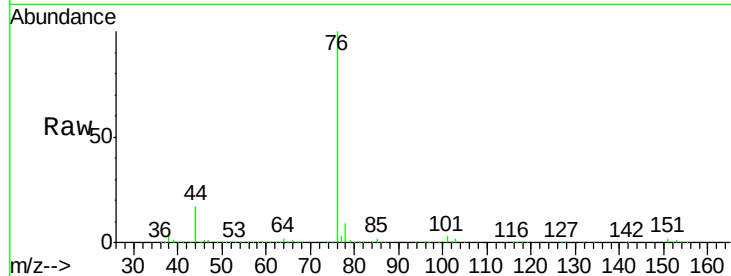

#28

Methyl tert-Butyl Ether

Concen: 8.496 ppbv

RT: 5.01 min Scan# 690

Delta R.T. -0.03 min

Lab File: VL038325.D




Acq: 1 Feb 2022 17:34


Tgt Ion: 73 Resp: 864398

Ion Ratio Lower Upper

73 100

57 23.3 18.2 27.4

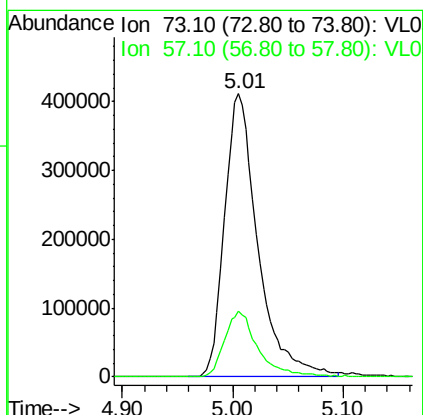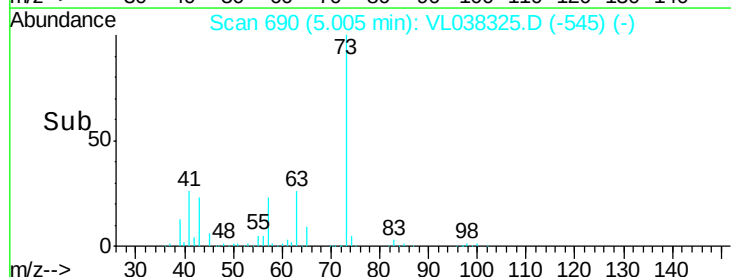







#29
Chloroform
Concen: 8.353 ppbv
RT: 5.72
Delta R.T. MSVOA_L
Lab File: ClientSampleId :
VSTDCCC010EC
Acq: 1 Feb 2022 17:34

Tgt Ion:
Ion Ratio
83 100
85 62.

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 02/07/2022
Supervised By :Mahesh Dadoda 02/07/2022

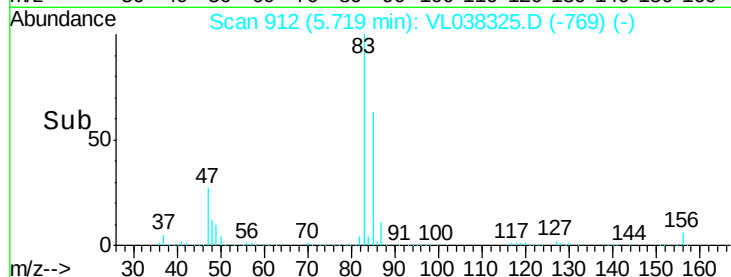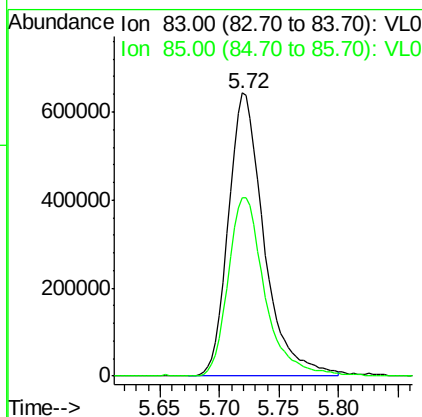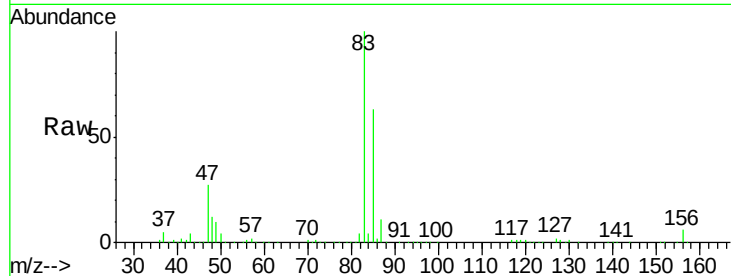

#30
Cyclohexane
Concen: 9.224 ppbv
RT: 7.10 min Scan# 1340
Delta R.T. -0.04 min
Lab File: VL038325.D
Acq: 1 Feb 2022 17:34

Tgt Ion: 84 Resp: 787689
Ion Ratio Lower Upper
84 100
56 136.3 112.7 169.1
41 79.9 71.1 106.7

