


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020122\
 Data File : VL038316.D
 Acq On : 1 Feb 2022 8:46
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL012422AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Jan 24 14:12:48 2022
 Last Update : Mon Jan 24 14:12:48 2022

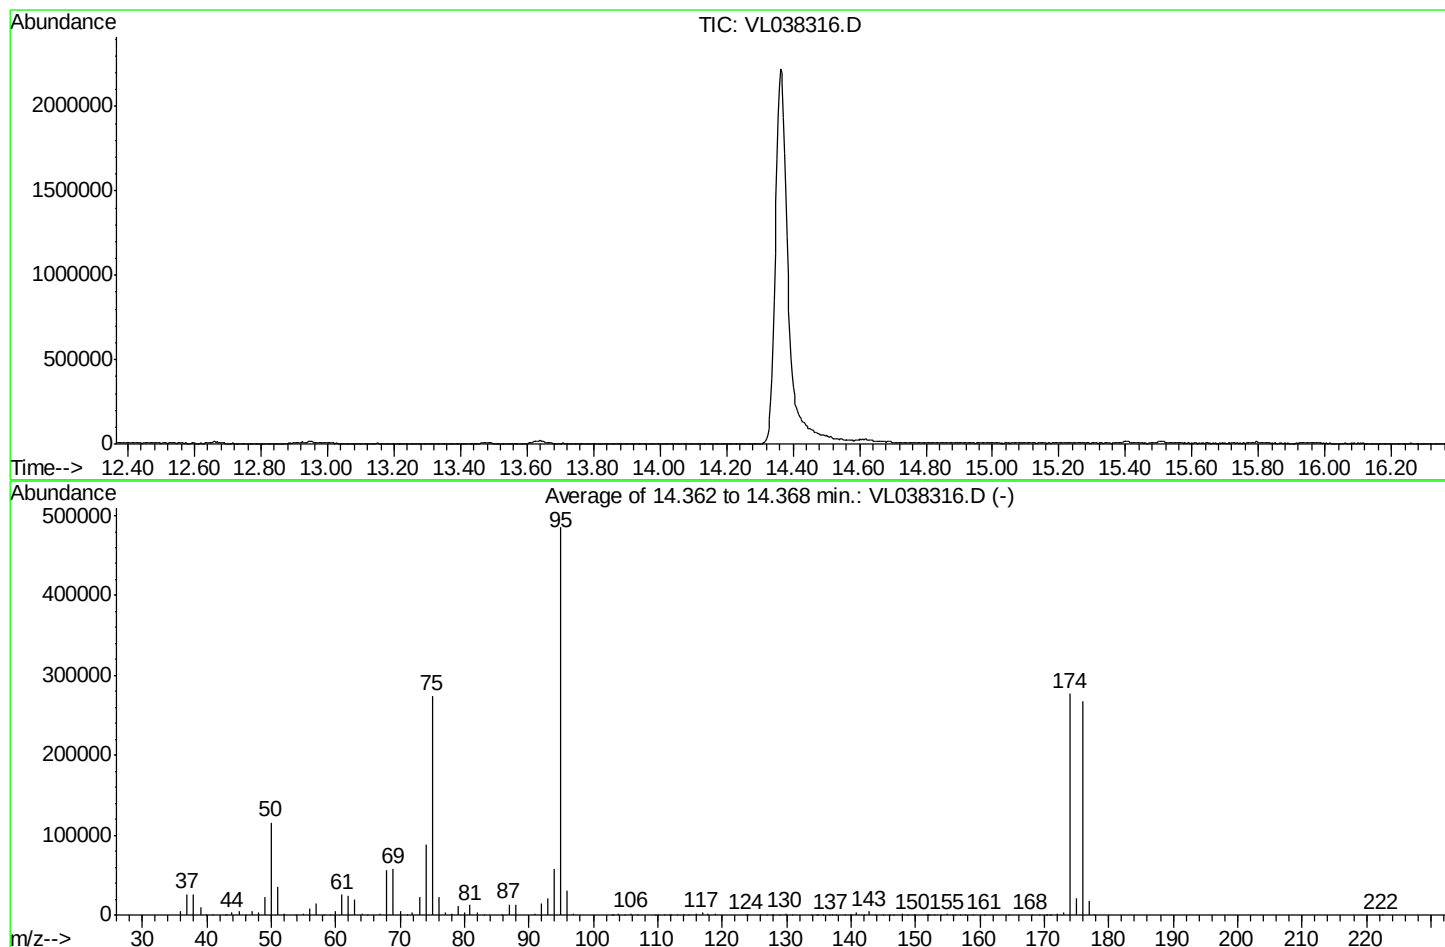

AutoFind: Scans 3600, 3601, 3602; Background Corrected with Scan 3576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	116050	PASS
75	95	30	66	56.5	274410	PASS
95	95	100	100	100.0	485333	PASS
96	95	5	9	6.3	30493	PASS
173	174	0.00	2	1.2	3291	PASS
174	95	50	120	57.1	277034	PASS
175	174	4	9	7.4	20474	PASS
176	174	93	101	96.5	267456	PASS
177	176	5	9	6.4	16992	PASS