


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020321\
 Data File : VL036291.D
 Acq On : 3 Feb 2021 11:20
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL011321AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Thu Jan 14 16:13:38 2021
 Last Update : Thu Jan 14 16:13:38 2021

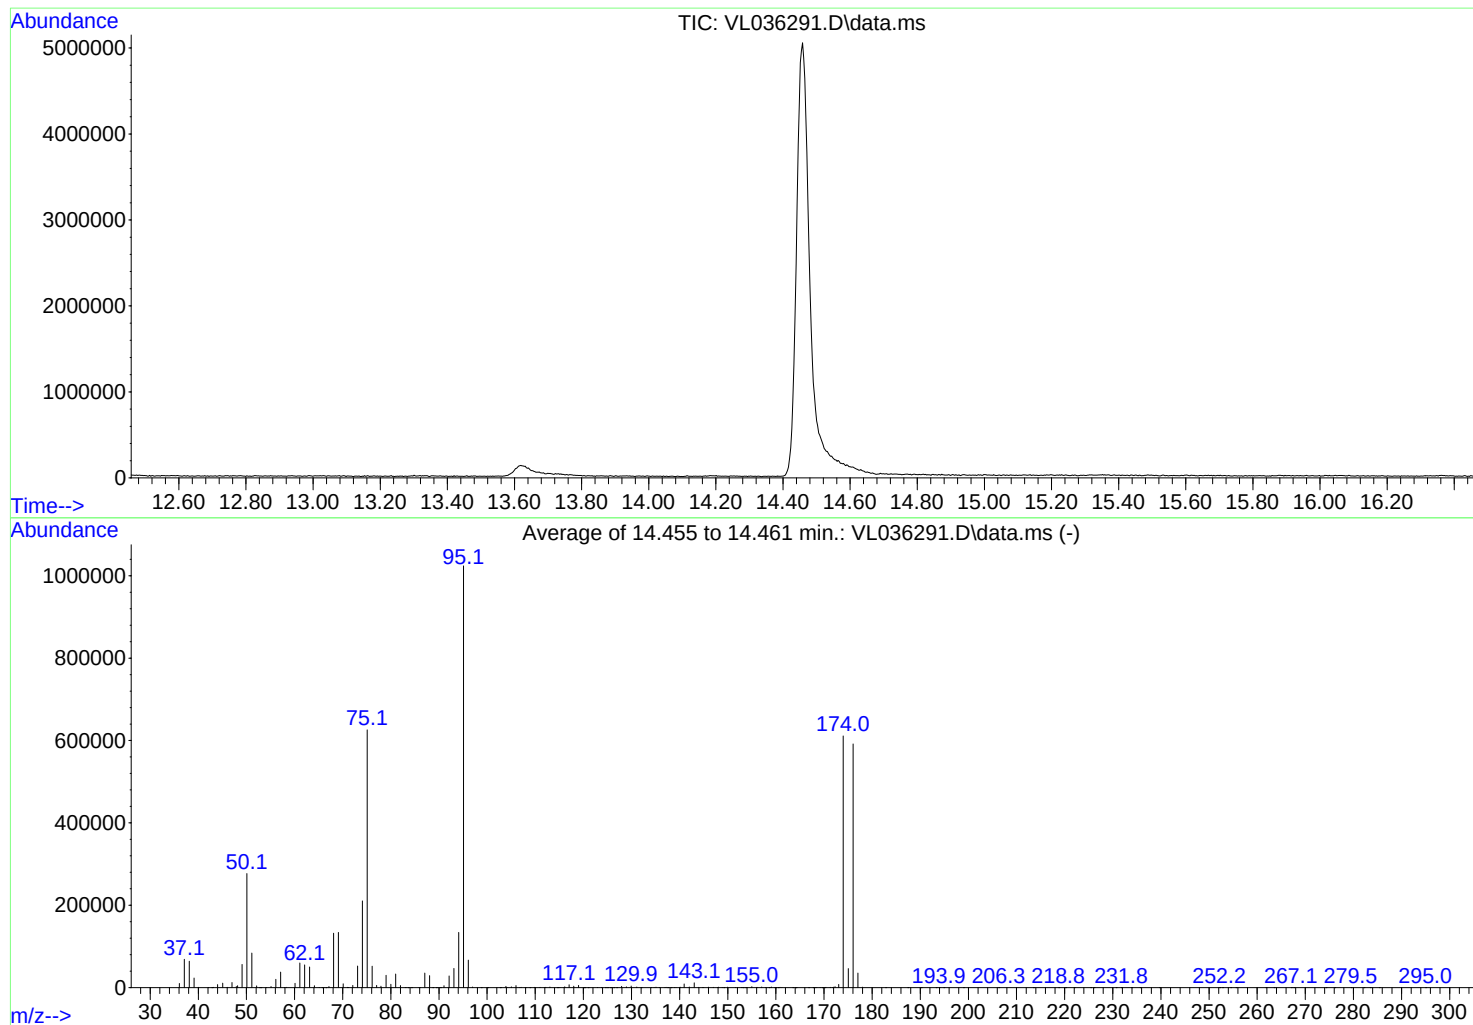

AutoFind: Scans 3629, 3630, 3631; Background Corrected with Scan 3606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.0	276949	PASS
75	95	30	66	61.1	626027	PASS
95	95	100	100	100.0	1024107	PASS
96	95	5	9	6.5	66981	PASS
173	174	0.00	2	1.3	7868	PASS
174	95	50	120	59.7	611200	PASS
175	174	4	9	7.6	46272	PASS
176	174	93	101	96.8	591616	PASS
177	176	5	9	6.0	35541	PASS

Average of 14.455 to 14.461 min.: VL036291.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	10365	47.00	12512	56.10	20173	66.10	285
37.10	68641	47.90	2651	57.10	37753	66.50	156
38.10	63960	48.15	4664	57.90	555	67.15	2650
39.10	23381	49.10	56411	58.25	809	68.10	132205
40.00	960	50.10	276949	60.10	10405	69.10	134163
42.15	301	51.10	84125	61.10	59987	70.10	9346
42.80	212	52.10	4399	62.10	55157	71.00	650
43.15	740	52.70	111	63.10	50155	71.20	329
44.00	7301	53.00	189	64.10	4559	72.10	5340
45.05	10949	54.15	302	65.10	406	73.10	52419
46.00	769	55.10	2942	65.70	172	74.10	210752

Instrument :
MSVOA_L
ClientSampled :
BFB

Average of 14.455 to 14.461 min.: VL036291.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.10	626027	84.30	100	94.10	134168	106.00	5128
76.10	52168	85.85	439	95.10	1.02411e+006	106.80	263
77.05	5582	86.10	596	96.10	66981	107.05	940
77.95	3709	87.05	35408	97.00	1568	107.90	212
79.00	29947	88.05	29192	98.80	59	108.90	84
80.00	8179	88.70	245	100.10	54	109.80	801
81.00	33253	89.45	161	102.70	195	110.00	266
82.00	5240	90.30	125	102.95	269	111.00	698
83.00	409	91.05	4728	103.90	3118	111.90	333
83.15	597	92.10	28488	104.10	994	112.20	676
83.60	188	93.10	46715	105.05	2061	113.05	1443

Average of 14.455 to 14.461 min.: VL036291.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
114.60	205	122.95	585	131.10	1533	139.25	625
114.80	298	123.75	307	132.00	79	140.10	1161
115.10	271	124.60	102	134.15	502	140.95	9077
116.00	924	125.00	82	134.70	560	142.00	1702
116.15	1935	125.60	121	135.10	1238	143.05	11859
117.05	7031	125.90	337	135.80	486	143.95	898
118.00	3624	126.30	184	136.95	635	144.80	297
119.00	5346	126.90	224	137.20	787	145.00	551
120.05	169	127.95	3002	137.50	111	146.00	1402
120.30	104	128.95	1975	138.20	166	147.00	665
121.00	50	129.95	3812	138.90	295	147.90	547

Average of 14.455 to 14.461 min.: VL036291.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.10	1369	155.00	2226	163.50	123	170.40	989
148.85	614	156.05	728	164.00	106	171.30	644
149.20	147	157.05	1782	164.20	162	171.80	632
149.95	1282	157.90	256	166.80	117	172.00	1035
151.65	385	158.60	202	167.75	251	172.30	2404
152.05	292	159.05	1508	168.00	137	173.05	7868
152.85	317	159.75	178	168.50	638	174.00	611200
153.00	394	160.00	50	169.20	420	175.05	46272
153.20	203	160.50	63	169.60	195	176.05	591616
153.70	150	160.85	656	169.80	254	177.05	35541
154.00	583	161.25	576	170.10	184	178.00	1253

Average of 14.455 to 14.461 min.: VL036291.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
182.80	91	222.00	98	255.60	203	295.00	76
187.40	57	225.40	148	261.80	113		
190.20	92	226.10	52	263.50	136		
193.30	51	230.70	67	267.10	200		
193.90	216	231.80	177	267.60	59		
194.90	64	233.90	78	274.30	135		
199.00	52	235.70	58	276.10	81		

206.30	87	239.70	68	279.50	248
213.50	57	252.20	252	282.20	116
218.75	106	252.80	61	283.50	60
220.20	71	254.50	60	285.40	137

Instrument :
MSVOA_L
ClientSampleId :
BFB