


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL020419\
Data File : VL033149.D
Acq On : 4 Feb 2019 9:23
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL020419AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Feb 04 14:41:39 2019
Last Update : Mon Feb 04 14:41:39 2019

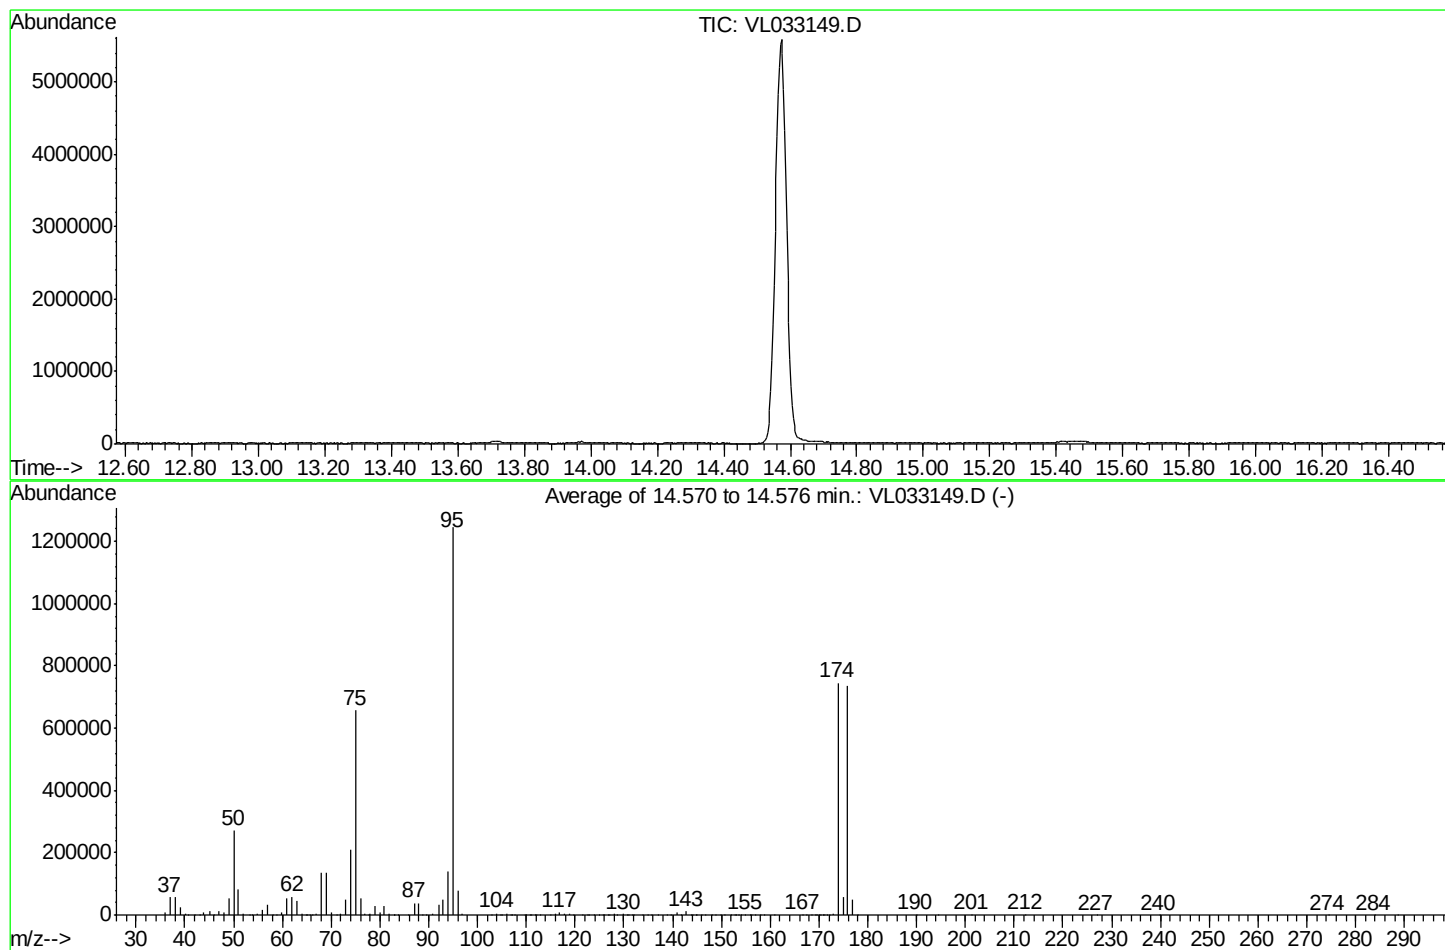

AutoFind: Scans 3618, 3619, 3620; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.8	271104	PASS
75	95	30	66	52.7	656170	PASS
95	95	100	100	100.0	1245184	PASS
96	95	5	9	6.4	79616	PASS
173	174	0.00	2	0.8	5748	PASS
174	95	50	120	59.8	744256	PASS
175	174	4	9	7.6	56234	PASS
176	174	93	101	98.9	736426	PASS
177	176	5	9	6.6	48442	PASS