
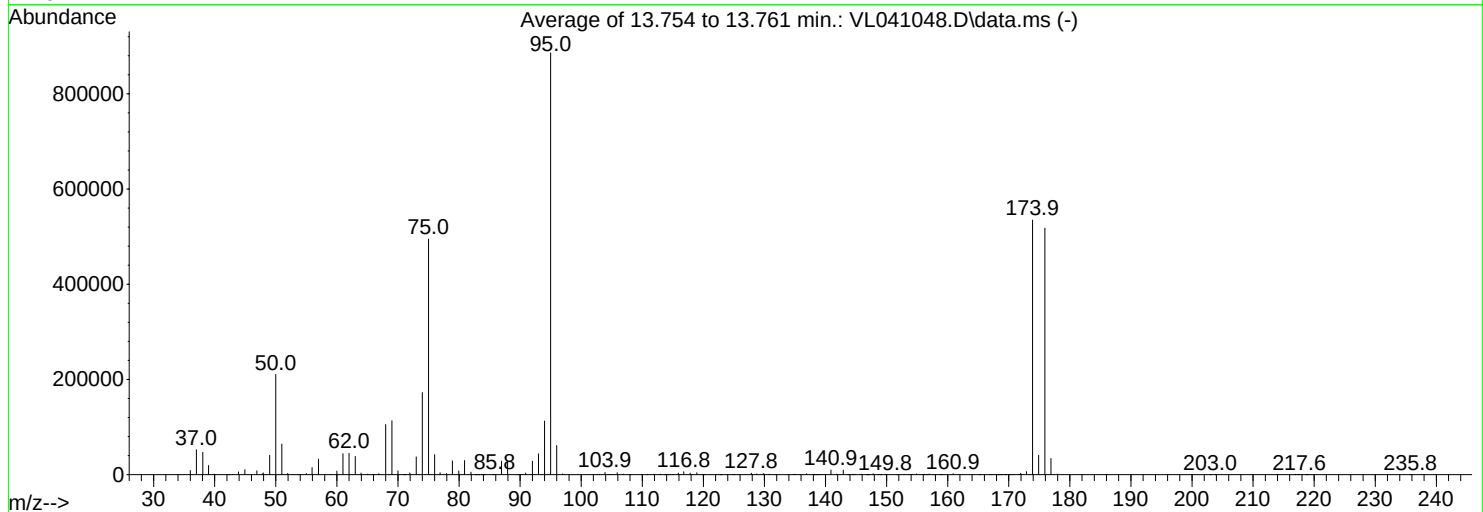


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020924\
Data File : VL041048.D
Acq On : 9 Feb 2024 8:21
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL012324AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Mon Feb 12 01:40:01 2024

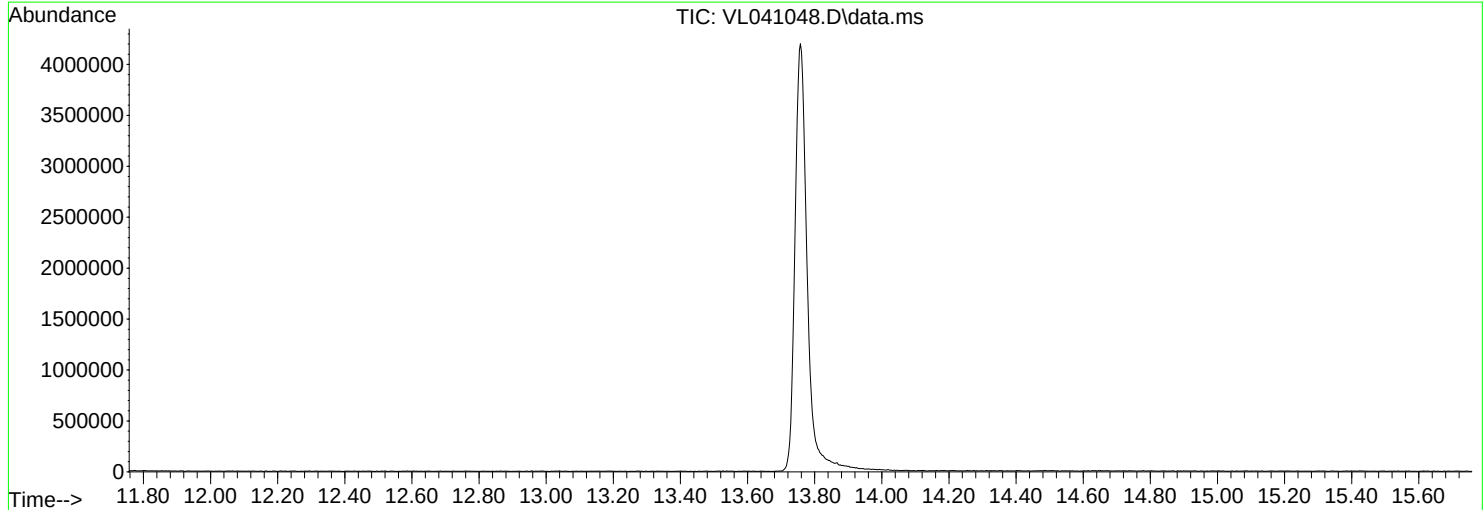

AutoFind: Scans 3468, 3469, 3470; Background Corrected with Scan 3444

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	23.7	210432	PASS
75	95	30	66	55.9	494912	PASS
95	95	100	100	100.0	886080	PASS
96	95	5	9	6.9	61144	PASS
173	174	0.00	2	1.2	6359	PASS
174	95	50	120	60.4	534784	PASS
175	174	4	9	7.6	40619	PASS
176	174	93	101	96.8	517845	PASS
177	176	5	9	6.6	33968	PASS

Average of 13.754 to 13.761 min.: VL041048.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	8835	47.80	1780	57.00	32787	68.00	10527
37.00	52595	47.95	3662	58.05	1099	69.00	11339
38.05	47131	49.00	40648	59.00	218	70.00	800
39.00	19288	50.00	210432	60.00	7389	70.90	42
39.90	1023	51.00	64123	61.00	44131	71.10	148
42.30	139	51.95	2565	62.00	44840	71.95	3829
42.95	406	52.95	419	63.00	38472	73.00	37459
43.90	5605	53.60	65	63.95	3352	74.00	172565
44.95	10293	54.10	203	65.05	985	75.00	494912
46.00	696	55.00	2441	65.90	110	76.00	41968
46.90	8207	55.95	14845	66.85	2049	76.90	3970

Average of 13.754 to 13.761 min.: VL041048.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.95	2357	85.85	759	102.60	329	111.95	894
78.90	28800	86.95	28157	103.05	353	113.00	913
79.95	7779	87.95	27432	103.90	4842	113.70	120
80.90	29581	89.70	50	104.50	343	114.20	71
81.95	5493	90.90	3282	104.70	429	114.60	238
82.70	110	92.00	28299	105.05	707	114.90	526
82.95	555	93.00	43837	105.90	4007	115.05	413
83.20	149	94.00	112645	106.85	1241	115.90	3329
83.70	161	95.00	886080	108.00	99	116.80	6091
84.10	65	96.00	61144	109.85	827	117.85	3546
85.50	168	96.95	1765	110.85	843	118.95	4204

Average of 13.754 to 13.761 min.: VL041048.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.80	88	128.75	1686	138.50	112	145.85	1159
120.00	57	129.80	2532	138.90	156	146.65	327
121.95	173	130.00	1008	139.40	362	146.80	159
122.70	119	130.80	1162	139.95	263	147.00	121
122.90	116	131.85	272	140.90	9648	147.80	2012
123.85	413	133.80	487	141.85	1522	148.60	53
124.80	206	134.70	476	142.90	9563	148.75	373
125.00	151	135.00	1100	143.70	191	149.00	155
125.70	477	135.85	274	143.90	376	149.80	476
126.85	328	136.90	2003	144.50	142	150.00	307
127.85	3177	138.20	138	144.85	693	151.70	128

Average of 13.754 to 13.761 min.: VL041048.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
151.85	349	159.00	167	169.60	207	177.95	1229
152.85	677	160.90	1942	170.20	419	203.00	97
153.60	309	165.20	53	170.40	308	203.80	79
154.00	309	167.00	205	170.85	767	216.80	76
154.90	1660	167.25	202	171.70	721	217.30	63
155.80	291	167.60	255	171.95	2686	217.60	203
156.10	184	168.05	263	172.90	6359	218.60	59
156.50	139	168.30	69	173.90	534784	218.90	67
156.95	1294	168.70	148	174.90	40619	225.80	76
157.85	319	169.10	322	175.90	517845	235.80	114
158.80	859	169.40	162	176.90	33968		