
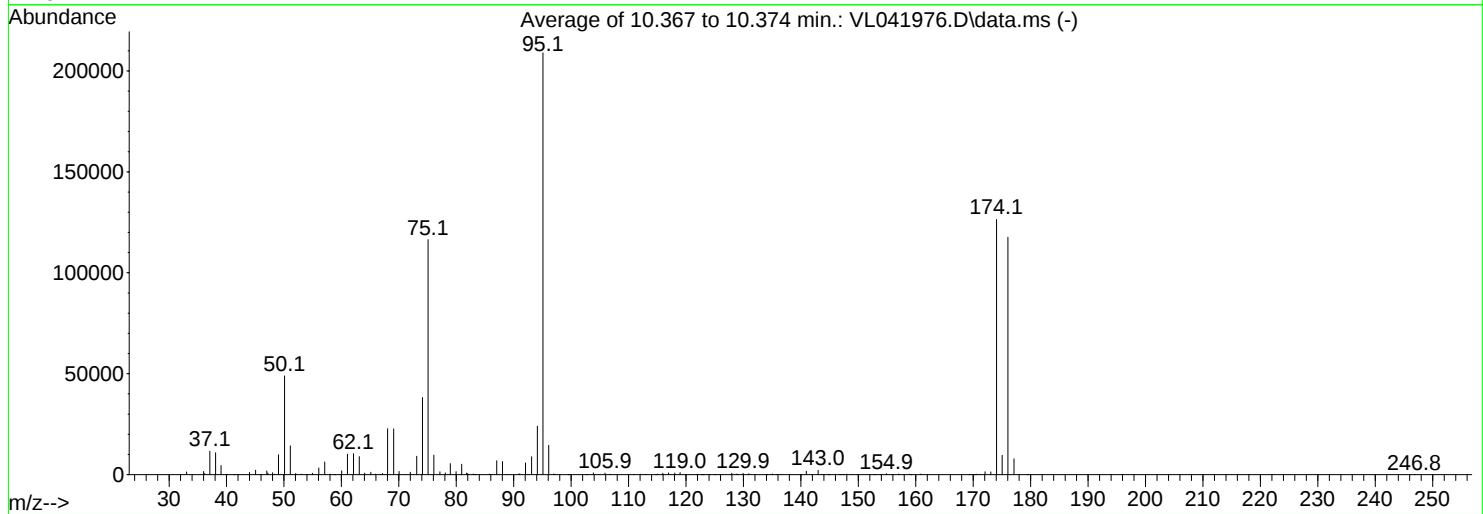


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL021025\
Data File : VL041976.D
Acq On : 10 Feb 2025 07:49
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Tue Jan 14 23:15:42 2025

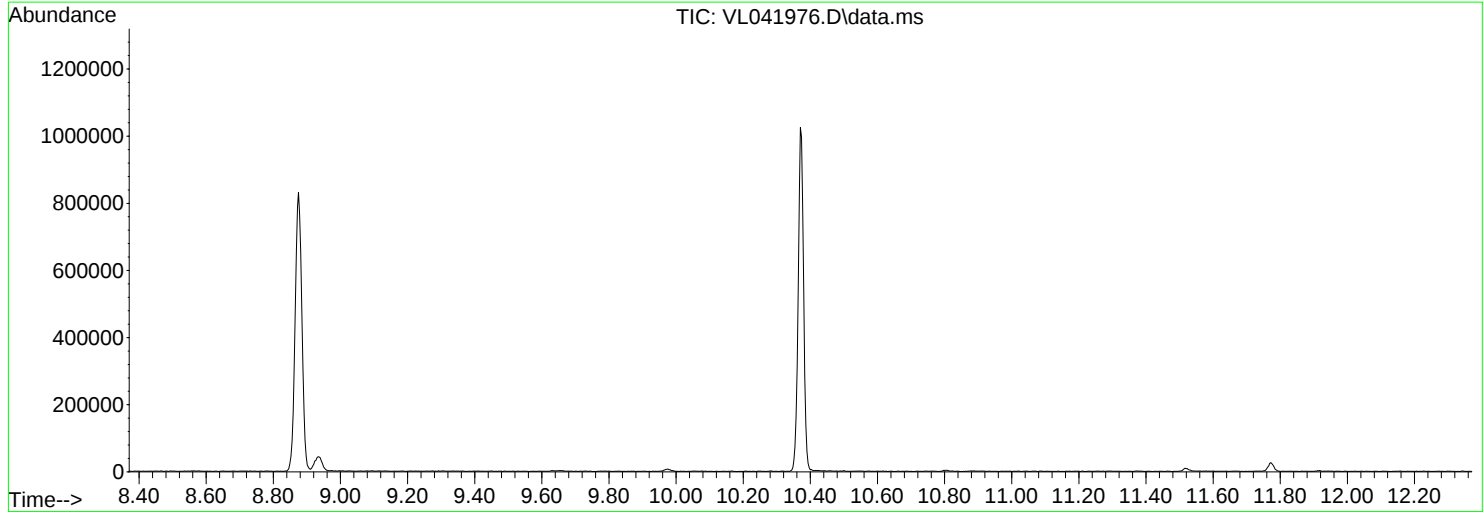

AutoFind: Scans 3176, 3177, 3178; Background Corrected with Scan 3162

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.4	48875	PASS
75	95	30	66	55.7	116459	PASS
95	95	100	100	100.0	208960	PASS
96	95	5	9	7.0	14527	PASS
173	174	0.00	2	1.0	1313	PASS
174	95	50	120	60.5	126461	PASS
175	174	4	9	7.6	9611	PASS
176	174	93	101	93.0	117661	PASS
177	176	5	9	6.6	7817	PASS

Average of 10.367 to 10.374 min.: VL041976.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.05	1370	45.05	2219	53.10	218	63.10	894
36.00	1571	45.90	54	53.80	68	64.05	80
36.20	560	46.15	142	54.10	81	65.10	116
37.10	11604	47.00	1849	54.95	727	65.95	25
38.10	10825	47.20	766	56.05	3348	66.80	110
39.05	4504	48.00	981	57.10	6266	67.15	570
39.95	38	48.30	276	58.05	327	68.05	22720
41.20	34	49.05	9833	58.80	46	69.10	22661
42.00	41	50.10	48875	60.05	1945	70.05	1629
42.85	125	51.10	14243	61.05	10122	71.10	61
44.00	1144	52.05	659	62.10	10390	72.00	1215

Average of 10.367 to 10.374 min.: VL041976.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.10	9120	82.95	281	94.10	24027	108.15	83
74.10	38243	83.20	26	95.10	208960	109.90	19
75.10	116459	85.80	287	96.10	14527	110.95	134
76.10	9663	86.20	57	96.95	281	112.10	259
77.15	1447	87.05	6932	97.20	175	112.90	50
78.10	868	88.05	6523	99.50	43	113.05	131
78.95	5505	88.80	51	102.60	20	114.70	20
79.95	1536	90.80	210	103.85	851	115.10	247
80.95	5128	91.05	412	104.80	97	115.95	754
81.80	762	92.05	5775	105.90	823	116.95	876
82.00	550	93.10	8879	106.80	237	118.05	791

Average of 10.367 to 10.374 min.: VL041976.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.95	1037	129.10	91	143.00	2171	152.05	48
119.90	17	129.95	643	143.80	80	152.70	36
121.90	45	130.95	470	144.80	27	153.10	142
122.70	19	134.00	21	145.05	124	153.85	131
123.00	33	134.80	123	146.00	238	154.90	467
123.80	64	135.05	288	146.70	95	155.80	109
124.20	72	135.80	94	146.90	23	156.15	80
125.00	29	136.70	190	147.40	26	157.05	317
125.90	72	140.10	185	148.00	309	158.00	55
127.95	692	140.95	1714	148.85	86	158.85	214
128.85	351	141.80	121	149.85	110	159.10	41

Average of 10.367 to 10.374 min.: VL041976.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.90	281	178.00	275				
169.30	20	179.40	24				
170.20	34	246.80	20				
170.65	224						
171.20	65						
172.05	1449						
173.05	1313						
174.05	126461						
175.05	9611						
176.05	117661						
177.10	7817						

Instrument :

MSVOA_L

ClientSampleId :

BFB