
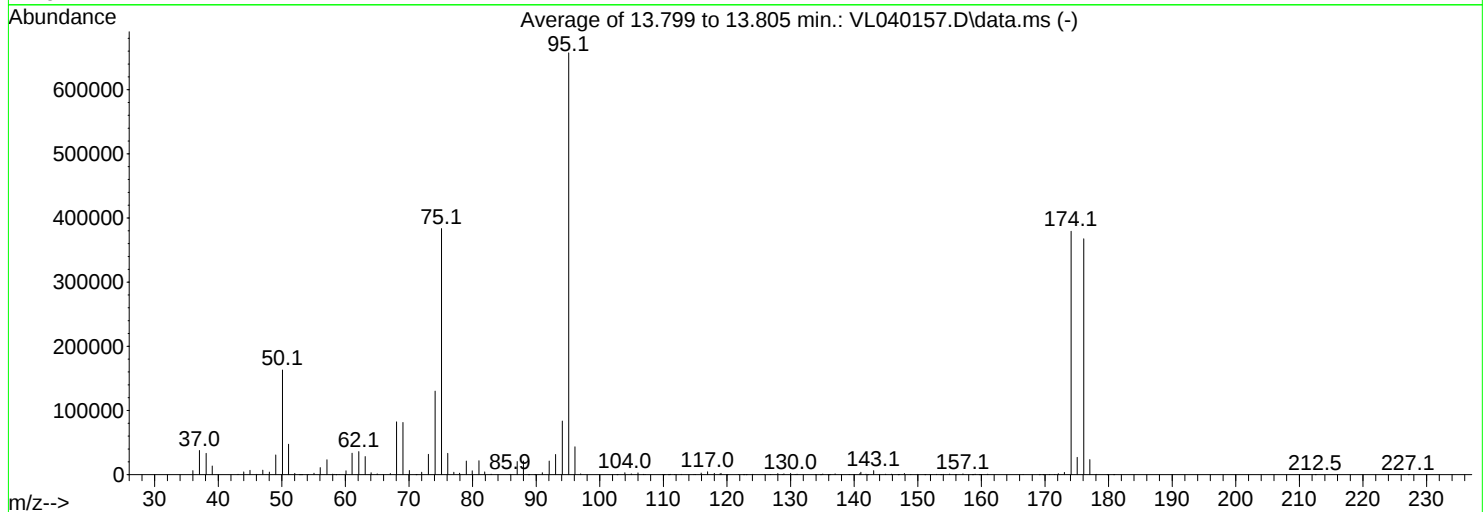


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL021323\
 Data File : VL040157.D
 Acq On : 13 Feb 2023 12:06
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011623AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Tue Feb 14 01:41:11 2023

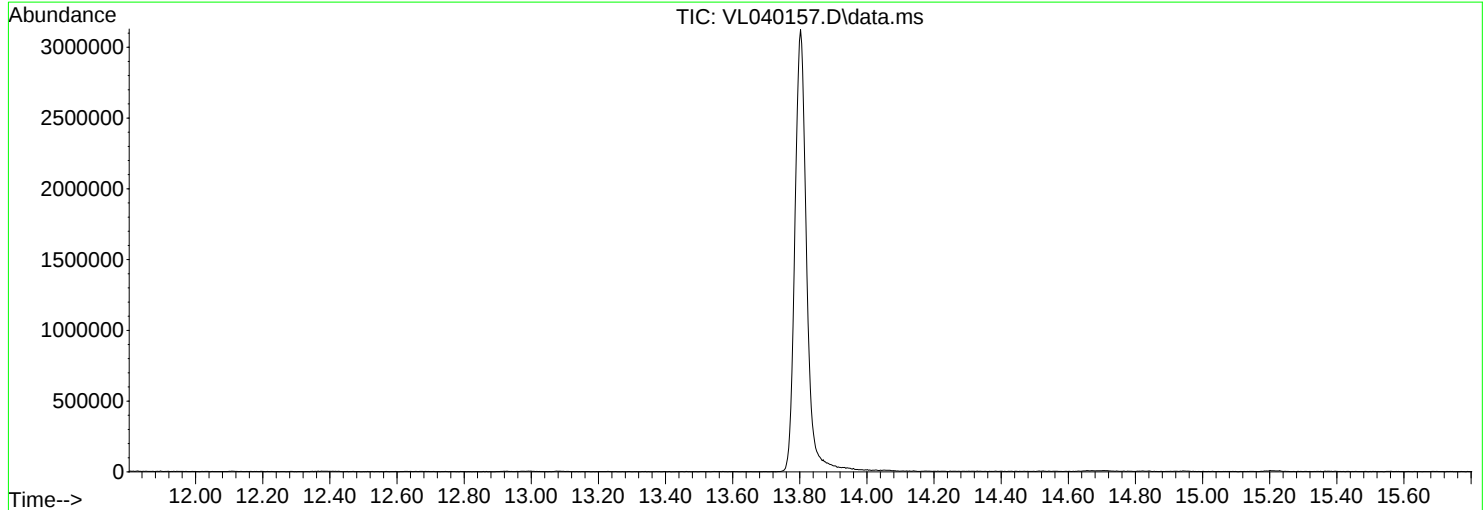

AutoFind: Scans 3482, 3483, 3484; Background Corrected with Scan 3456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.8	162987	PASS
75	95	30	66	58.3	383488	PASS
95	95	100	100	100.0	657387	PASS
96	95	5	9	6.6	43467	PASS
173	174	0.00	2	0.9	3406	PASS
174	95	50	120	57.7	379371	PASS
175	174	4	9	7.1	26933	PASS
176	174	93	101	96.9	367616	PASS
177	176	5	9	6.4	23357	PASS

Average of 13.799 to 13.805 min.: VL040157.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	6355	50.10	162987	58.50	142	69.05	8134
37.05	37773	51.05	47339	59.00	172	70.05	654
38.10	33248	52.05	2012	60.10	6100	71.10	8
39.05	13539	52.80	154	61.05	33413	72.00	369
43.10	474	53.10	72	62.10	35928	73.05	31701
44.00	4316	54.15	220	63.10	28277	74.10	130176
45.00	6658	55.05	2167	64.05	2988	75.10	383488
46.05	484	56.05	11006	65.00	1259	76.10	33101
47.00	6882	57.10	23269	65.95	267	77.05	3665
48.05	4019	58.00	893	67.05	1791	77.95	2327
49.05	30813	58.20	443	68.05	82357	79.00	21096

Average of 13.799 to 13.805 min.: VL040157.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.95	5982	93.05	31445	109.90	281	118.00	1935
81.00	21688	94.10	83581	110.10	138	118.90	1155
81.90	4215	95.10	657387	110.80	157	119.05	2062
82.90	674	96.10	43467	111.10	395	120.00	144
85.90	526	97.00	1171	111.75	277	121.80	161
87.00	20501	102.70	84	112.00	237	122.60	58
88.00	21232	103.95	3034	112.80	513	123.00	82
88.80	88	104.95	1169	114.80	362	124.05	580
89.80	87	106.00	2672	115.00	196	125.90	350
90.95	2886	106.85	627	115.95	2461	126.85	209
92.05	21224	107.10	242	116.95	4434	128.00	1859

Average of 13.799 to 13.805 min.: VL040157.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
128.70	346	139.20	187	147.10	192	156.10	216
128.95	1248	140.00	333	147.90	1860	157.10	1159
130.00	1913	140.90	1670	148.90	311	158.60	110
130.70	328	141.05	3887	150.00	503	159.00	770
131.00	857	141.85	668	151.10	94	159.70	76
133.90	61	142.10	142	151.95	263	160.00	167
134.70	156	143.05	6313	152.95	486	161.00	745
135.05	1073	143.95	435	153.60	75	166.55	233
135.90	124	144.95	697	154.00	500	169.10	87
136.10	92	145.85	654	155.00	1133	169.70	152
137.00	1230	146.90	66	155.90	155	170.70	276

Average of 13.799 to 13.805 min.: VL040157.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
171.55	330	227.10	56				
172.10	1625						
173.05	3406						
174.10	379371						
175.05	26933						
176.10	367616						
177.05	23357						
178.05	625						
179.80	107						
180.80	149						
212.50	94						

Instrument :

MSVOA_L

ClientSampleId :

BFB