
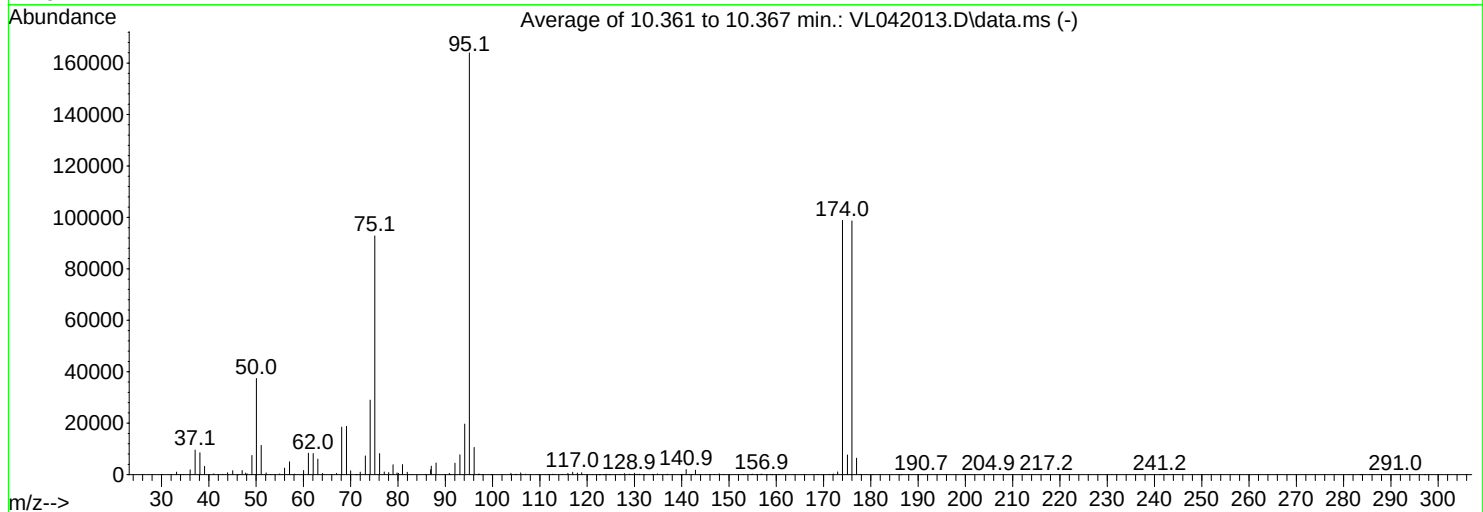


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL021425\
 Data File : VL042013.D
 Acq On : 14 Feb 2025 11:20
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL021425AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Sat Feb 15 01:55:33 2025

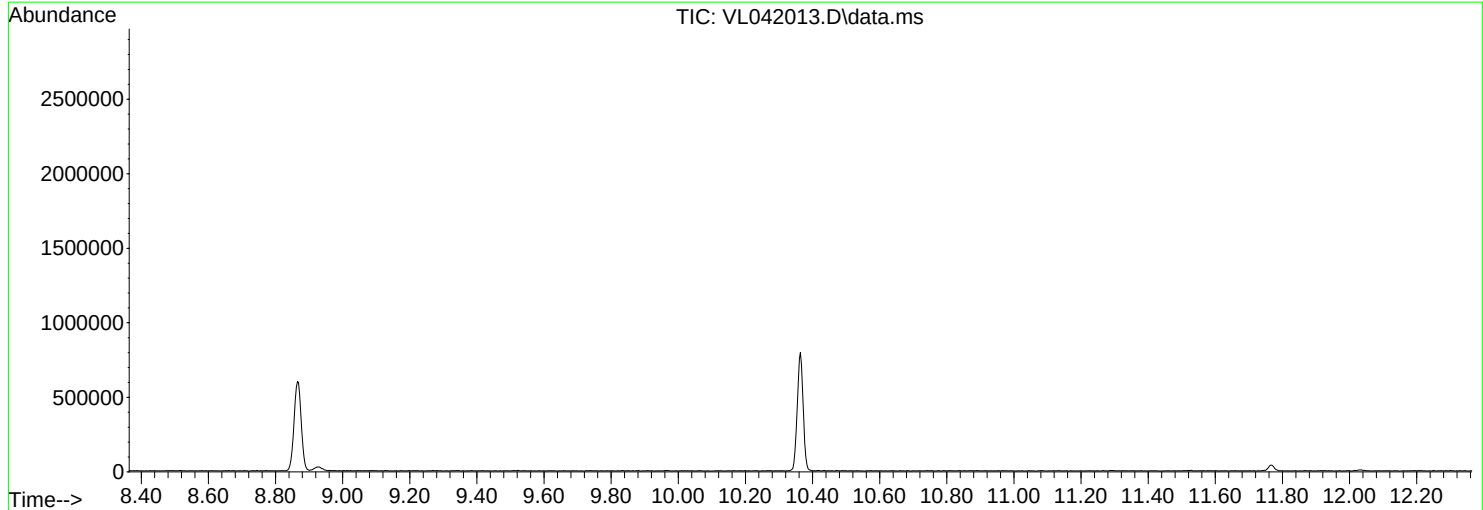

AutoFind: Scans 3174, 3175, 3176; Background Corrected with Scan 3159

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.8	37366	PASS
75	95	30	66	56.6	92800	PASS
95	95	100	100	100.0	163968	PASS
96	95	5	9	6.4	10570	PASS
173	174	0.00	2	1.1	1077	PASS
174	95	50	120	60.3	98829	PASS
175	174	4	9	7.7	7640	PASS
176	174	93	101	99.8	98632	PASS
177	176	5	9	6.5	6409	PASS

Average of 10.361 to 10.367 min.: VL042013.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.15	1009	45.05	1559	53.95	78	68.10	1846
34.05	52	46.10	25	55.00	340	69.10	1877
34.65	43	47.05	1647	56.00	2548	70.00	147
36.05	1877	47.80	603	57.05	4962	71.15	1
37.10	9589	48.10	288	58.15	181	72.00	984
38.10	8517	49.10	7463	60.05	1627	73.10	7272
39.10	3263	50.05	37366	61.05	8319	74.10	29000
41.05	302	51.05	11360	62.05	8229	75.10	92800
42.00	126	52.10	679	63.05	6031	76.10	8232
42.95	155	53.00	42	64.05	491	77.10	1057
43.95	766	53.20	42	67.00	529	78.05	840

Average of 10.361 to 10.367 min.: VL042013.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	3840	91.10	41	104.85	154	116.95	925
79.80	668	92.05	4502	105.10	148	117.95	636
80.10	511	93.10	7696	105.95	670	118.85	780
80.95	3901	94.10	19651	107.00	169	121.10	54
81.95	921	95.10	163968	109.60	56	122.50	21
83.05	46	96.10	10570	111.20	66	122.70	20
85.85	118	97.00	167	111.75	54	123.50	24
86.90	1928	97.15	251	112.75	176	124.15	178
87.05	3321	97.80	39	113.20	40	124.70	25
88.05	4543	99.70	29	114.75	102	127.05	41
90.85	481	103.90	474	115.95	476	127.90	441

Average of 10.361 to 10.367 min.: VL042013.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
128.90	214	140.15	115	148.85	151	160.65	74
129.10	104	140.95	1972	150.00	51	163.80	58
130.05	599	141.70	157	153.05	59	165.90	43
130.60	125	142.20	47	154.80	115	168.70	83
131.05	205	142.90	1734	154.95	185	168.90	88
132.00	19	143.70	62	155.80	53	169.80	36
133.80	18	145.00	95	156.70	124	171.30	148
134.90	299	145.90	40	156.95	256	171.90	112
136.70	69	146.10	58	157.90	28	172.15	231
136.95	183	146.95	65	158.80	133	173.00	1077
139.80	19	147.95	334	159.10	28	174.00	98829

Average of 10.361 to 10.367 min.: VL042013.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
175.05	7640	242.80	49				
176.00	98632	281.10	56				
177.00	6409	283.50	18				
177.90	75	285.55	78				
180.45	59	291.00	79				
186.35	39	297.10	39				
190.70	52						
204.90	77						
217.20	51						
231.00	55						
241.15	71						