
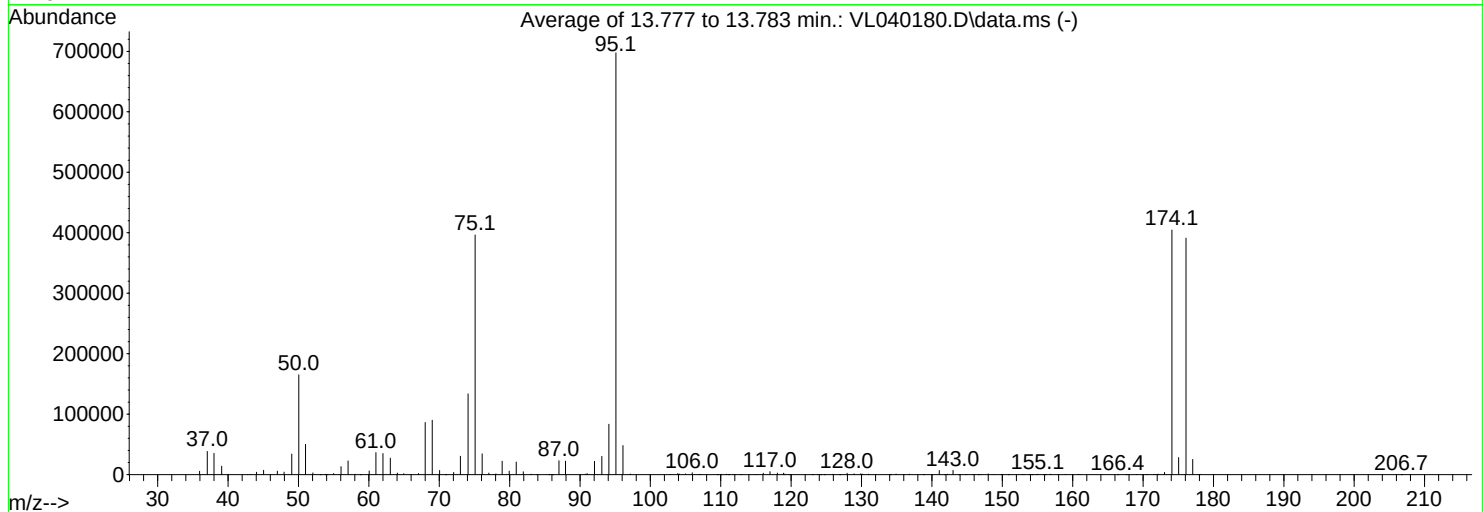


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL021623\
Data File : VL040180.D
Acq On : 16 Feb 2023 12:52
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL021523AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Feb 15 17:01:01 2023

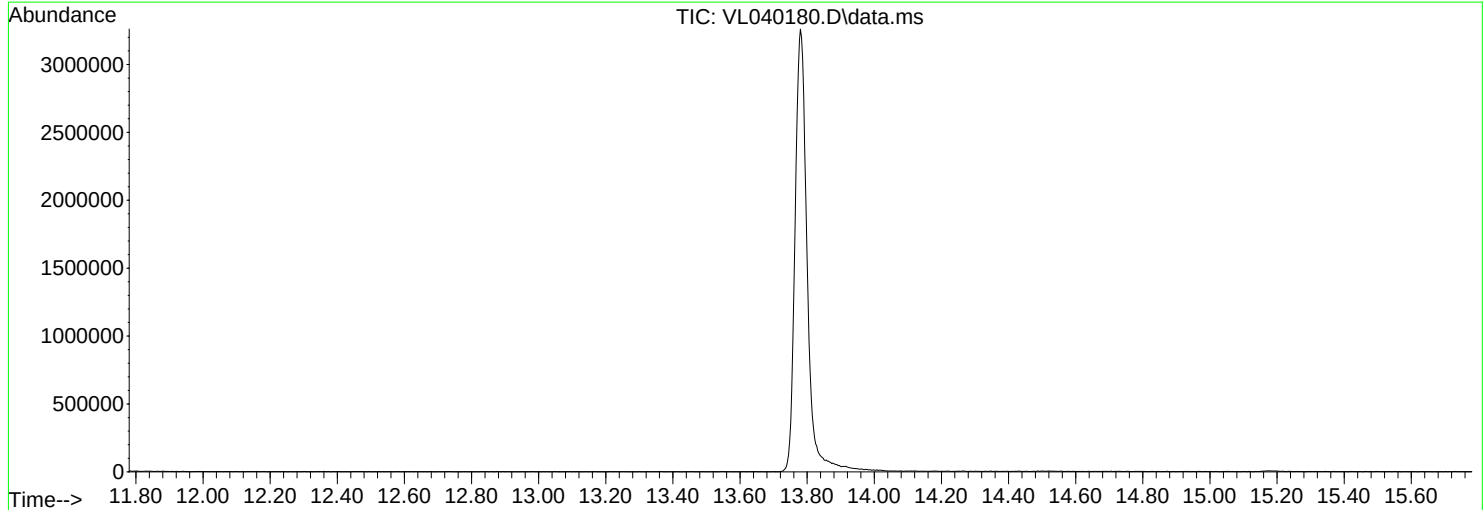

AutoFind: Scans 3475, 3476, 3477; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.7	164992	PASS
75	95	30	66	56.8	396352	PASS
95	95	100	100	100.0	697557	PASS
96	95	5	9	6.9	48221	PASS
173	174	0.00	2	0.9	3719	PASS
174	95	50	120	58.0	404544	PASS
175	174	4	9	7.0	28472	PASS
176	174	93	101	96.7	391168	PASS
177	176	5	9	6.5	25272	PASS

Average of 13.777 to 13.783 min.: VL040180.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	5618	47.95	4304	58.05	840	69.00	9005
37.05	38445	49.05	34120	58.80	118	70.05	701
38.00	35219	50.05	164992	60.05	6182	70.90	15
39.10	13988	51.00	49989	61.00	36469	71.05	20
40.00	469	52.05	2887	62.00	34968	72.05	3622
42.80	251	53.10	116	63.05	27328	73.00	30496
43.15	237	53.80	96	64.05	2611	74.10	133781
44.05	4006	54.15	179	64.95	1563	75.10	396352
45.05	7294	55.00	1891	65.90	228	76.10	34445
46.05	663	56.05	13298	67.05	1851	77.05	2761
47.00	5781	57.05	22787	68.00	86384	77.80	629

Average of 13.777 to 13.783 min.: VL040180.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.05	1422	90.80	689	105.00	1286	113.00	301
78.95	22139	91.00	1954	105.95	3246	114.75	269
79.95	5833	92.05	22083	106.90	196	115.15	250
80.95	21040	93.10	30269	107.05	521	116.05	2357
81.95	4657	94.10	83376	109.50	69	117.00	4930
83.05	823	95.10	697557	110.05	670	118.05	2730
83.85	208	96.10	48221	110.85	679	118.90	2381
85.60	74	97.15	1044	111.10	84	119.10	1124
86.10	127	102.85	366	111.75	412	119.80	58
87.00	22987	103.90	2000	112.10	186	122.10	218
87.95	22128	104.10	1044	112.80	299	123.00	64

Average of 13.777 to 13.783 min.: VL040180.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.75	364	134.10	53	144.05	383	150.85	150
124.20	92	134.90	1000	144.80	204	152.05	194
124.70	66	135.90	142	144.95	410	152.85	387
125.90	555	136.80	859	145.85	558	153.10	179
126.90	127	138.80	55	146.10	285	153.85	377
127.95	2451	140.10	311	146.60	73	154.20	121
128.95	1242	141.05	6913	147.00	377	154.80	333
129.90	1664	141.80	154	148.00	1402	155.05	920
130.10	866	142.20	879	148.85	325	155.85	258
131.00	909	143.00	7103	149.85	477	156.10	91
132.00	180	143.80	144	150.10	355	156.90	694

Average of 13.777 to 13.783 min.: VL040180.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.90	210	171.70	320				
159.00	645	172.00	446				
160.80	457	172.15	924				
161.05	349	173.05	3719				
166.40	68	174.10	404544				
167.60	67	175.05	28472				
168.00	218	176.10	391168				
169.10	176	177.05	25272				
170.40	230	177.90	249				
170.60	202	178.10	621				
171.50	287	206.70	52				