


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL021920\
 Data File : VL034647.D
 Acq On : 19 Feb 2020 10:30
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL013020AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Thu Jan 30 17:16:44 2020
 Last Update : Thu Jan 30 17:16:44 2020

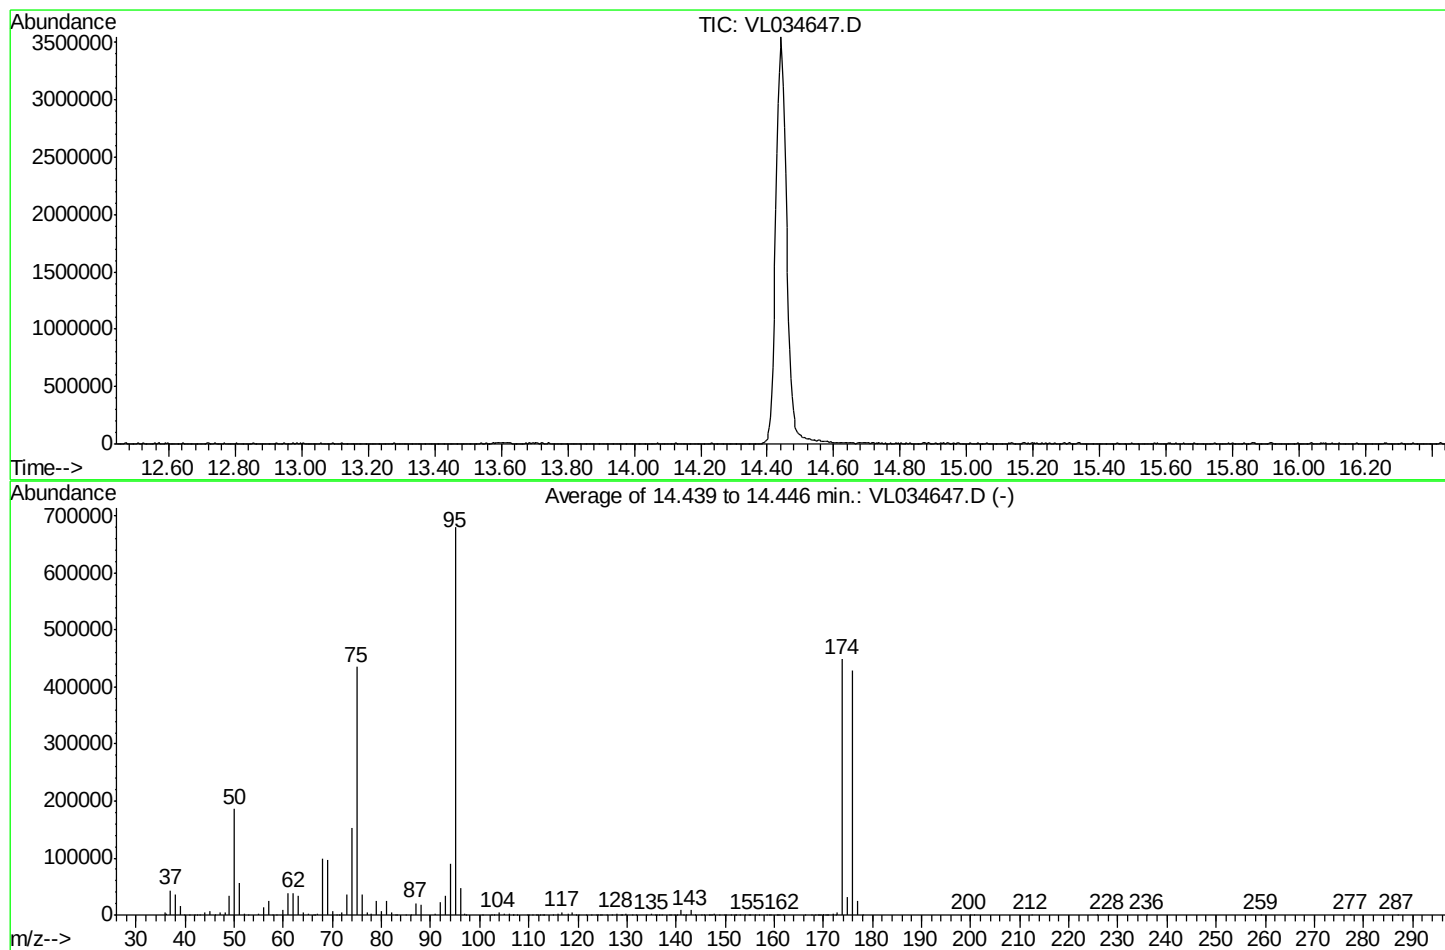

AutoFind: Scans 3624, 3625, 3626; Background Corrected with Scan 3600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.4	186304	PASS
75	95	30	66	63.9	434858	PASS
95	95	100	100	100.0	680149	PASS
96	95	5	9	6.8	46178	PASS
173	174	0.00	2	0.9	3833	PASS
174	95	50	120	65.9	448426	PASS
175	174	4	9	6.8	30538	PASS
176	174	93	101	95.5	428309	PASS
177	176	5	9	6.0	25728	PASS