

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022322\
 Data File : VL038422.D
 Acq On : 24 Feb 2022 00:30
 Operator : SY/AP
 Sample : VIBLK
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VIBLK

Quant Time: Feb 24 07:33:25 2022
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL022222AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
 QLast Update : Tue Feb 22 19:45:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.645	49	821119	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	7.150	114	2020173	10.000	ppbv	0.00
55) Chlorobenzene-d5	12.057	117	1687580	10.000	ppbv	# 0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.384	95	1353403	9.693	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	96.900%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022322\
Data File : VL038422.D
Acq On : 24 Feb 2022 00:30
Operator : SY/AP
Sample : VIBLK
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Quant Time: Feb 24 07:33:25 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL022222AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
QLast Update : Tue Feb 22 19:45:51 2022
Response via : Initial Calibration




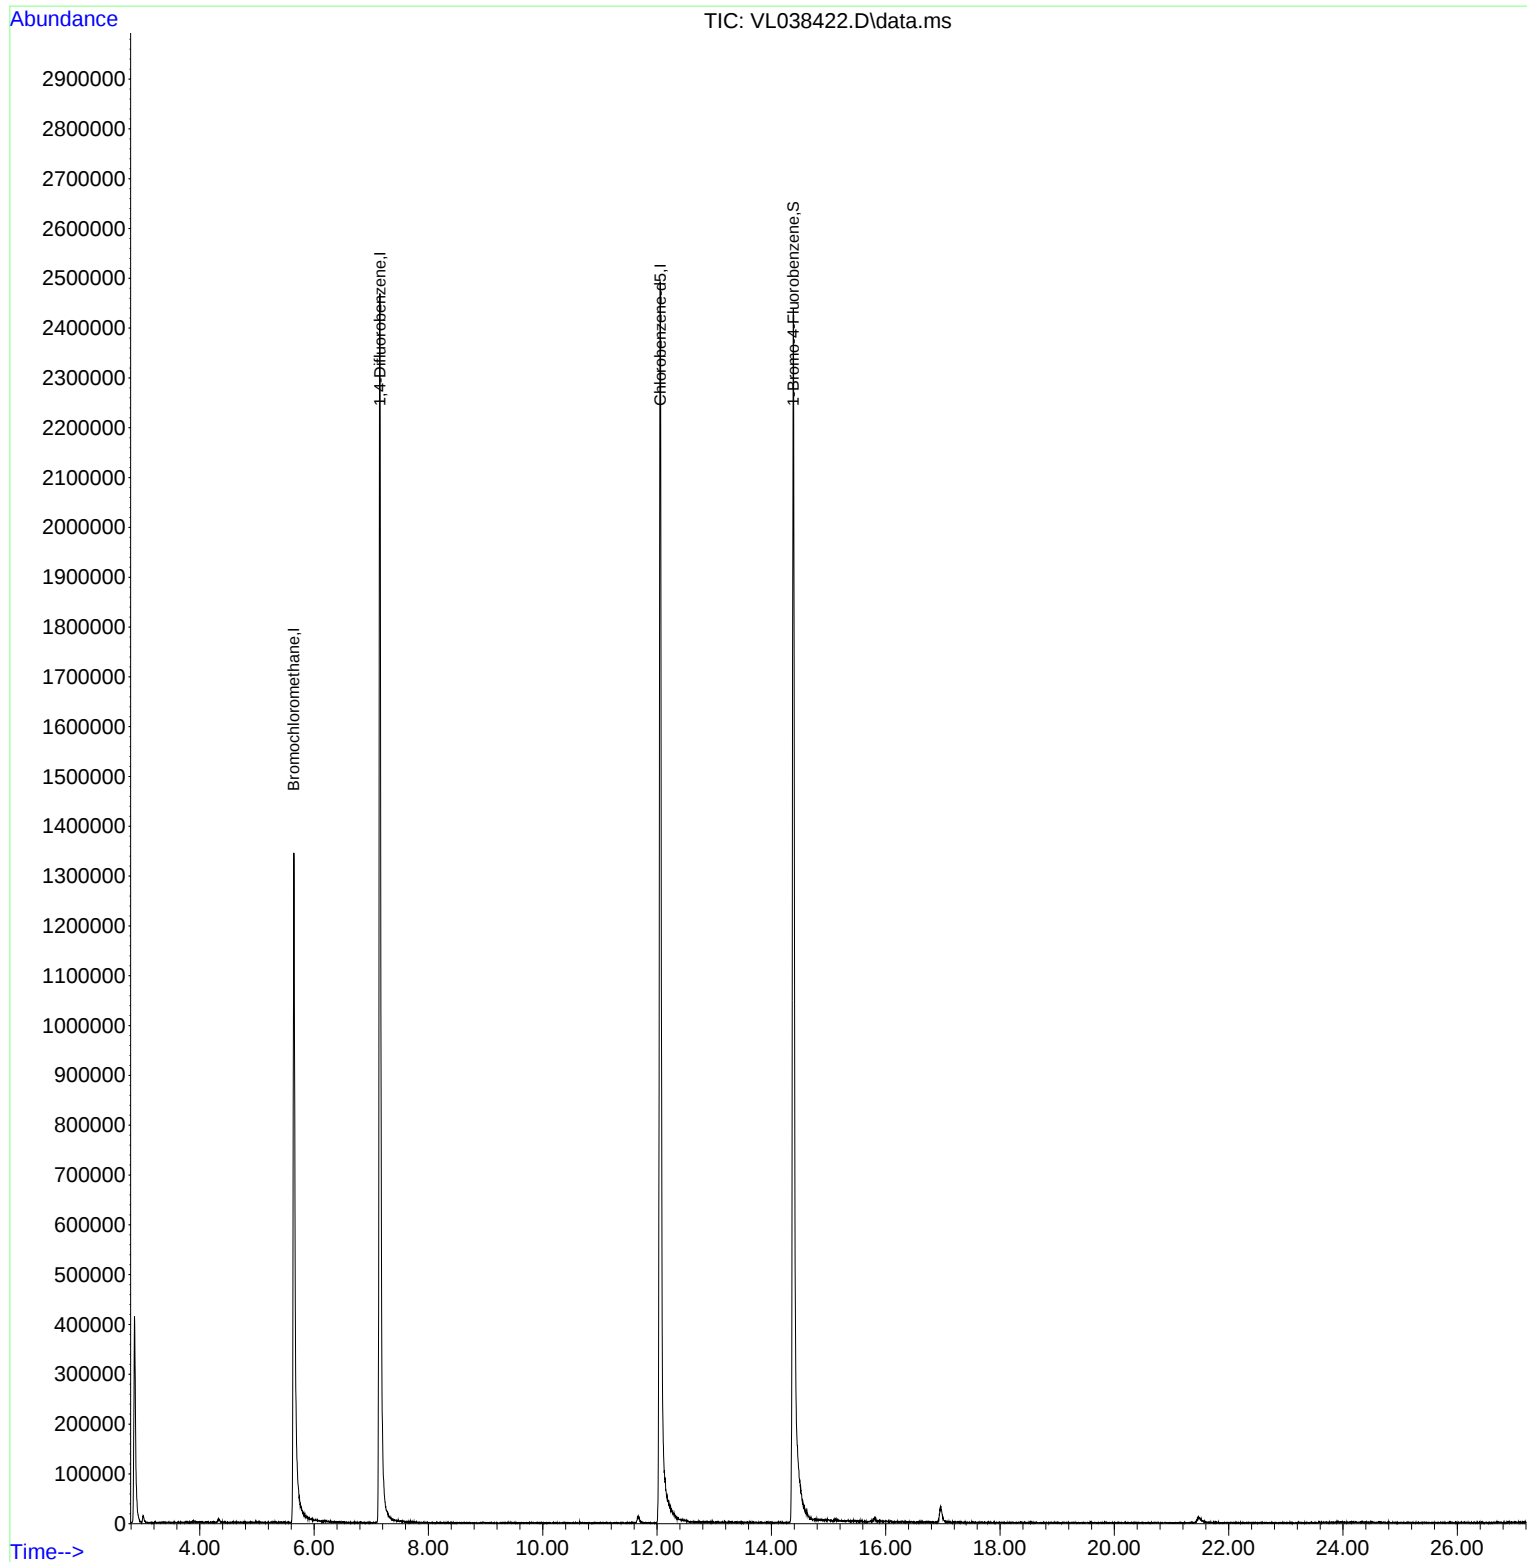


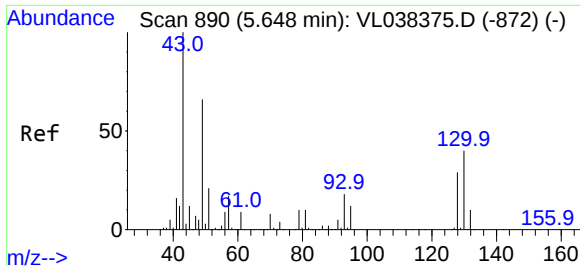

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.645 min Scan# 81
Delta R.T. -0.003 min
Lab File: VL038422.D
Acq: 24 Feb 2022 00:30




Instrument :
MSVOA_L
ClientSampleId :
VIBLK


Tgt Ion: 49 Resp: 821119
Ion Ratio Lower Upper
49 100
128 48.3 24.3 72.9
130 61.2 30.1 90.5

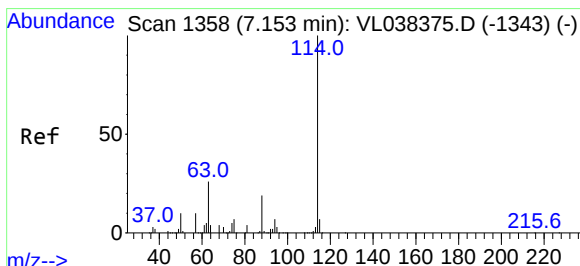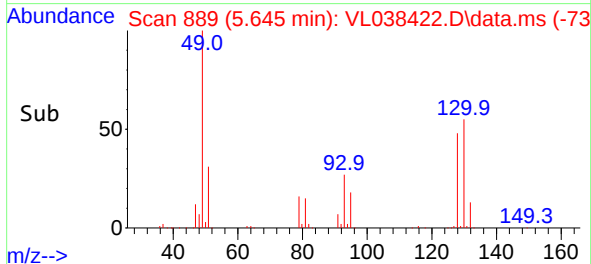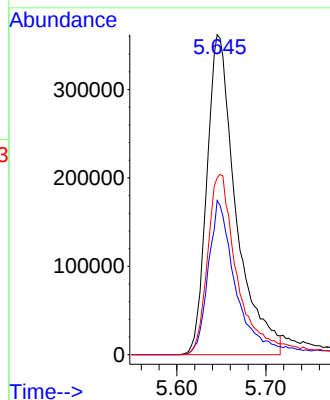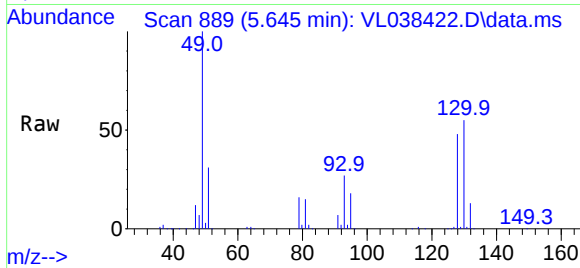

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.150 min Scan# 1357
Delta R.T. -0.003 min
Lab File: VL038422.D
Acq: 24 Feb 2022 00:30

Tgt Ion: 114 Resp: 2020173
Ion Ratio Lower Upper
114 100
63 27.9 22.2 33.2
88 18.8 15.2 22.8


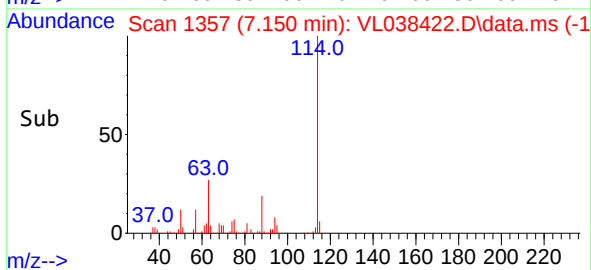
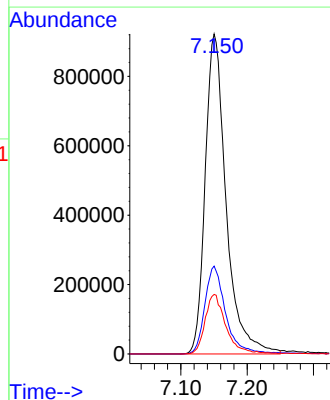
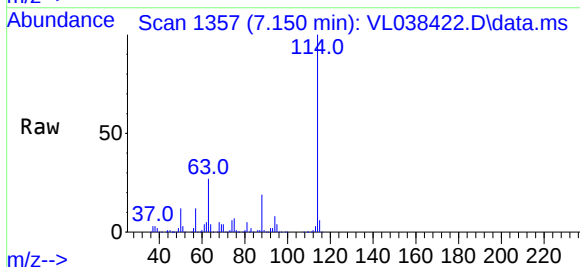


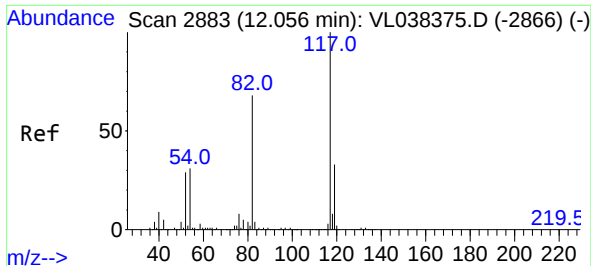

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.057 min Scan# 21
Delta R.T. 0.000 min
Lab File: VL038422.D
Acq: 24 Feb 2022 00:30

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 1687580
Ion Ratio Lower Upper
117 100
82 72.8 54.9 82.3
119 33.5 46.1 69.1#

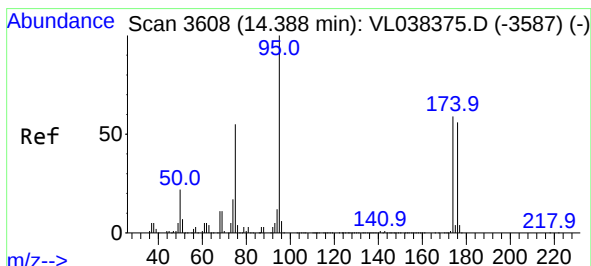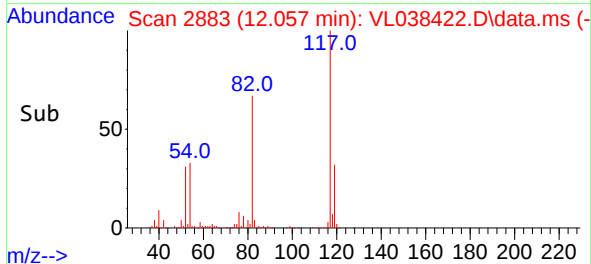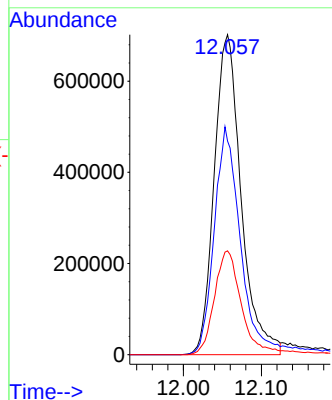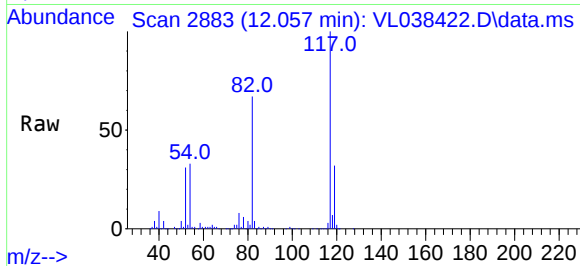

#68
1-Bromo-4-Fluorobenzene
Concen: 9.693 ppbv
RT: 14.384 min Scan# 3607
Delta R.T. -0.003 min
Lab File: VL038422.D
Acq: 24 Feb 2022 00:30

Tgt Ion: 95 Resp: 1353403
Ion Ratio Lower Upper
95 100
174 61.2 49.0 73.4
175 4.4 3.6 5.4

