


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022322\
 Data File : VL038404.D
 Acq On : 23 Feb 2022 8:55
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL022222AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
 Last Update : Tue Feb 22 19:45:51 2022

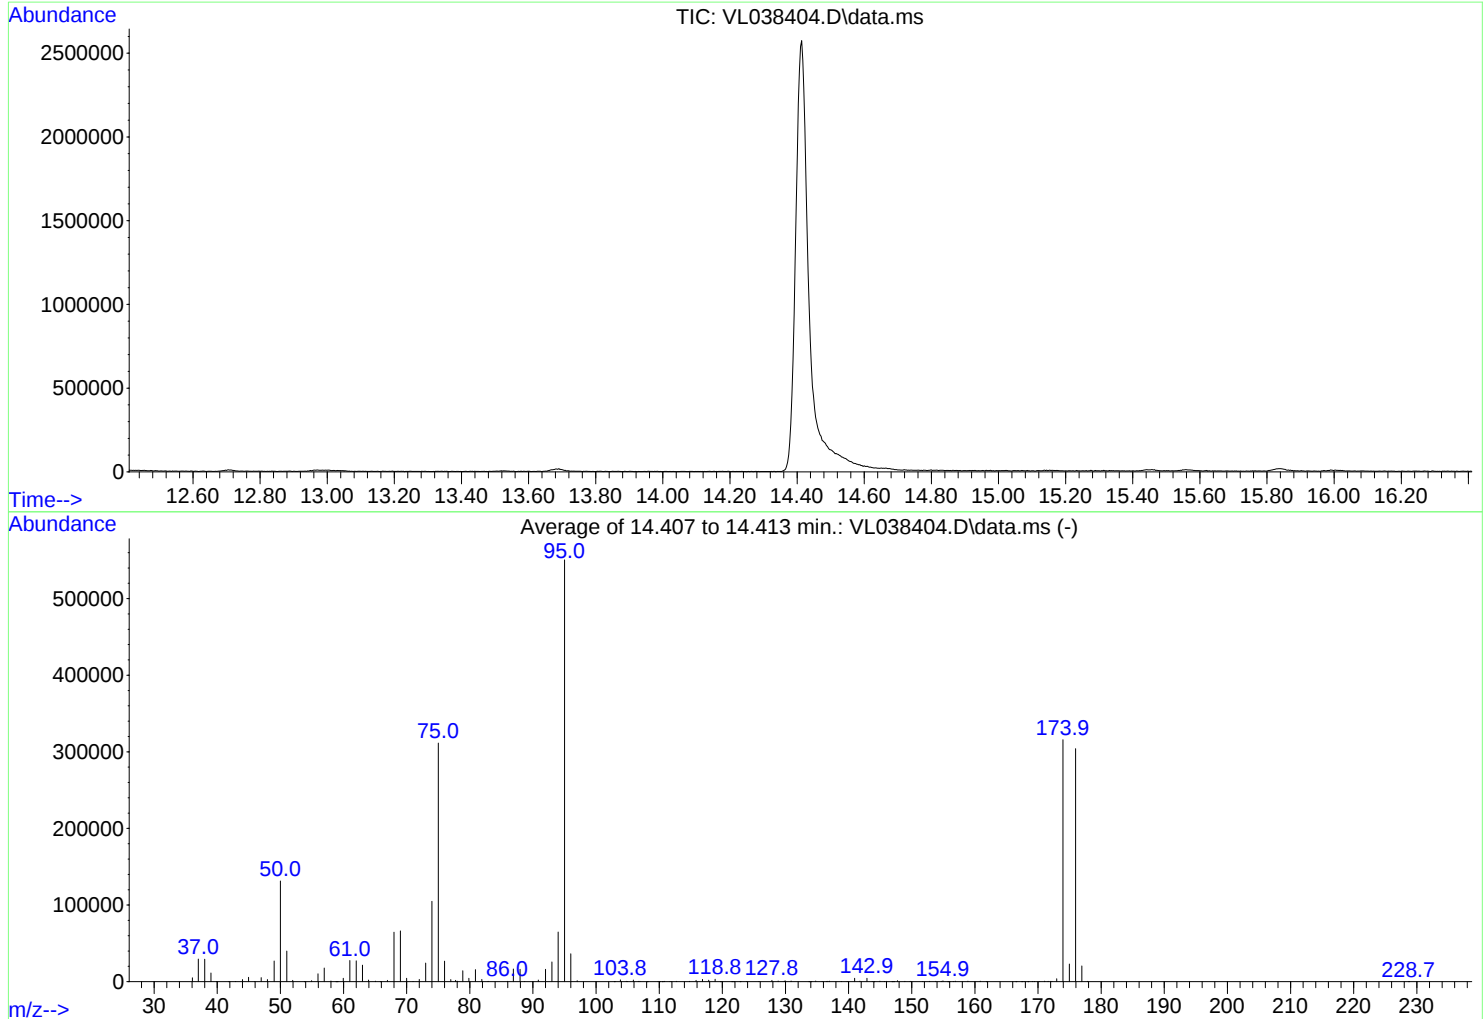

AutoFind: Scans 3614, 3615, 3616; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	131331	PASS
75	95	30	66	56.5	311339	PASS
95	95	100	100	100.0	550613	PASS
96	95	5	9	6.6	36472	PASS
173	174	0.00	2	1.2	3780	PASS
174	95	50	120	57.4	315861	PASS
175	174	4	9	7.3	22965	PASS
176	174	93	101	96.3	304213	PASS
177	176	5	9	6.8	20595	PASS

Average of 14.407 to 14.413 min.: VL038404.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	4979	47.95	2775	59.00	70	70.00	4434
37.00	29413	49.00	26899	59.95	4448	71.00	2118
38.00	29195	50.00	131331	61.00	27512	72.00	2871
39.00	11293	51.00	39819	62.00	27256	73.00	2426
39.90	141	51.95	1780	63.00	21472	74.00	104952
41.80	64	53.80	50	63.95	2049	75.00	311339
42.90	278	54.95	1317	65.05	575	76.00	26789
44.00	2822	55.95	10167	65.80	91	77.00	2788
44.95	5578	56.95	17773	66.95	1639	77.75	1697
45.95	263	58.00	790	68.00	64557	78.00	574
46.95	5332	58.80	58	69.00	66219	78.90	14165

Average of 14.407 to 14.413 min.: VL038404.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.85	4332	94.00	64749	108.10	62	117.85	1858
80.90	15730	95.00	550613	109.80	229	118.85	3088
81.90	3008	96.00	36472	110.00	116	119.70	52
82.90	527	97.00	1212	110.50	120	121.50	122
85.95	524	102.90	98	110.85	336	121.80	62
86.90	16549	103.85	2209	111.70	258	122.80	72
87.95	16084	104.80	496	111.90	151	123.85	265
88.70	179	105.00	239	112.75	492	125.80	258
90.85	2141	105.90	2022	114.80	436	127.85	1760
92.00	16083	106.70	396	115.85	1763	128.85	855
93.00	25640	106.95	503	116.85	2885	129.80	574

Average of 14.407 to 14.413 min.: VL038404.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
129.95	1159	140.95	4493	148.90	415	158.90	636
130.90	898	141.80	711	149.75	505	160.85	624
133.70	55	142.90	4511	151.75	274	161.80	71
134.00	65	143.75	179	152.85	363	166.50	80
134.80	890	144.00	76	153.80	333	167.40	87
135.80	194	144.95	616	154.70	450	167.80	201
136.50	181	145.70	287	154.95	969	168.40	78
136.70	377	146.00	356	155.70	83	169.10	174
136.95	557	146.85	122	155.90	66	169.45	284
138.85	233	147.10	80	156.60	221	170.25	255
139.75	285	147.75	1196	156.90	732	171.05	674

Average of 14.407 to 14.413 min.: VL038404.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
171.60	389						
172.00	408						
172.20	428						
172.95	3780						
173.95	315861						
174.95	22965						
175.95	304213						
176.95	20595						
177.85	434						
228.70	63						

Instrument :

MSVOA_L

ClientSampleId :

BFB