


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022323\
Data File : VL040215.D
Acq On : 23 Feb 2023 9:36
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL021523AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Feb 24 00:45:34 2023

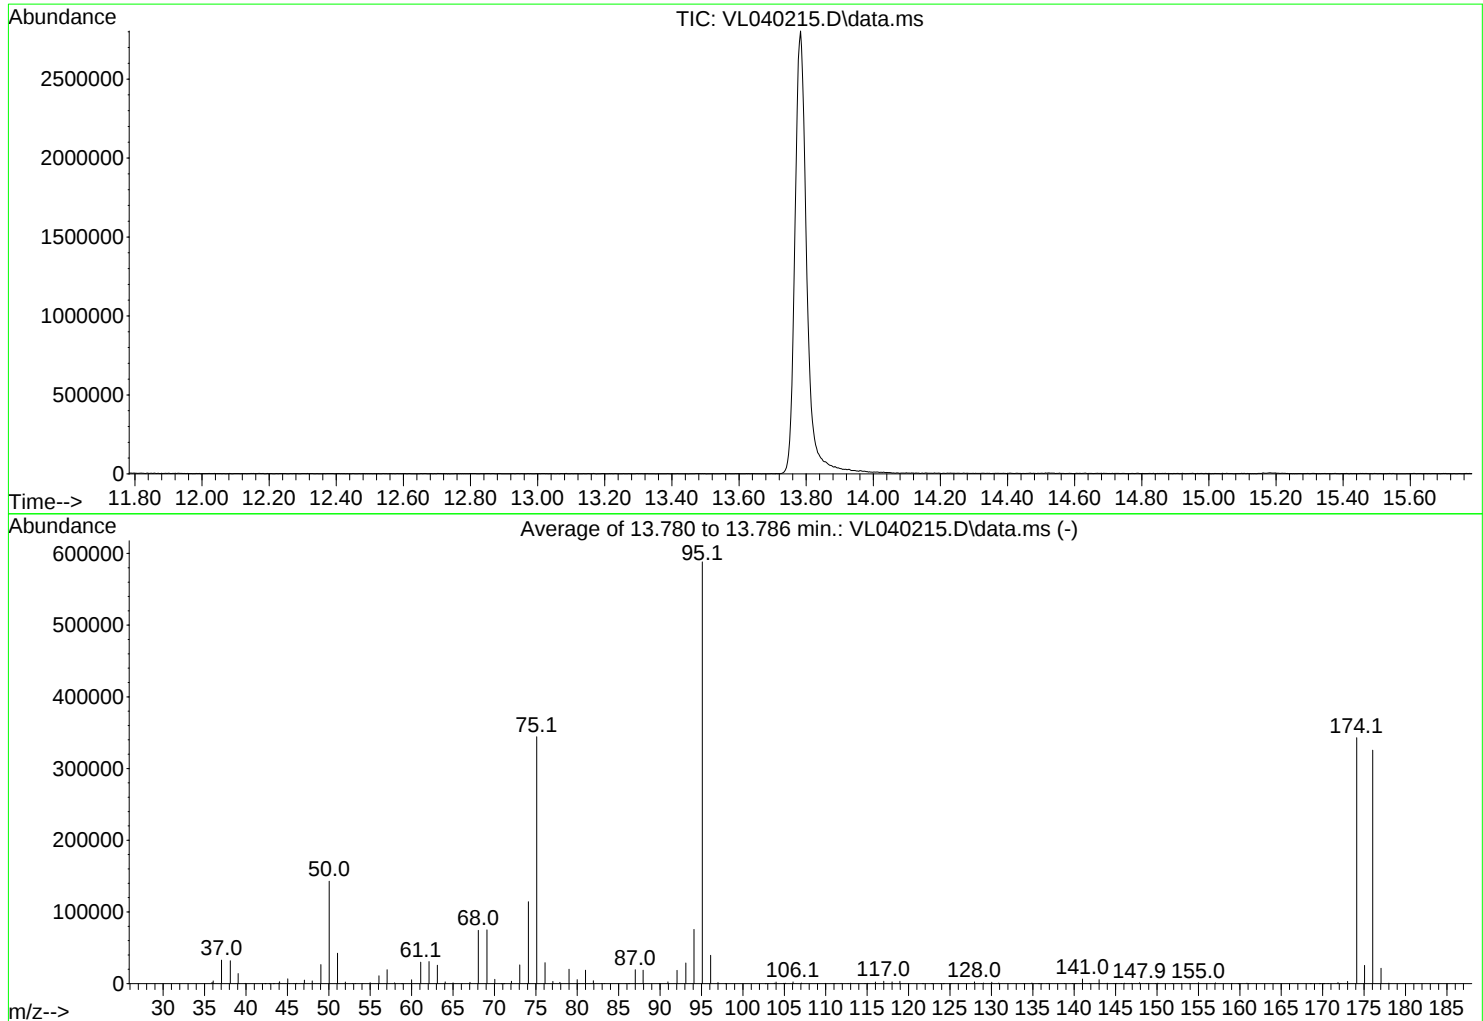

AutoFind: Scans 3476, 3477, 3478; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.3	142933	PASS
75	95	30	66	58.5	344448	PASS
95	95	100	100	100.0	588309	PASS
96	95	5	9	6.7	39488	PASS
173	174	0.00	2	0.9	3086	PASS
174	95	50	120	58.3	343104	PASS
175	174	4	9	7.4	25461	PASS
176	174	93	101	94.9	325589	PASS
177	176	5	9	6.6	21469	PASS

Average of 13.780 to 13.786 min.: VL040215.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	1827	45.05	6664	54.10	296	65.00	1033
36.05	3781	45.80	206	55.00	1249	66.10	154
37.05	32808	46.10	389	56.05	10985	67.05	177
38.10	31864	47.05	5005	57.05	19520	68.05	7436
39.05	14102	48.00	3809	57.95	1101	69.10	75016
39.90	572	49.05	26640	58.80	79	70.05	6033
42.30	53	50.05	142933	60.00	5300	70.80	124
42.80	64	51.05	42368	61.10	29920	71.10	61
43.30	107	52.00	2232	62.10	30720	72.05	3387
43.90	755	52.85	272	63.10	25731	73.05	26024
44.05	2813	53.20	171	64.05	2547	74.10	114259

Average of 13.780 to 13.786 min.: VL040215.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.10	344448	86.20	51	97.90	118	111.10	255
76.10	29248	87.00	19333	102.70	108	111.85	497
77.05	3048	87.95	18779	103.05	294	112.70	181
77.90	1828	89.90	57	103.80	791	113.00	589
79.00	20067	90.95	2376	104.00	2164	114.75	284
80.00	5538	92.05	18597	104.90	369	115.05	445
81.00	18688	93.10	28765	105.10	600	116.00	2195
81.95	3955	94.10	75725	106.05	2415	117.00	3357
82.95	215	95.10	588309	107.05	812	118.00	2495
83.25	270	96.10	39488	109.95	493	118.95	3330
85.90	251	97.00	1523	110.90	194	121.70	75

Average of 13.780 to 13.786 min.: VL040215.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
122.80	67	135.70	83	144.80	264	152.95	511
123.85	168	136.00	114	145.05	385	153.90	291
124.20	104	136.70	283	145.70	233	155.00	1333
125.05	111	136.95	447	146.05	587	156.00	184
127.95	2517	138.85	228	146.90	358	157.05	1172
128.80	233	139.80	284	147.90	1416	159.05	501
129.05	986	140.20	263	148.70	227	159.80	62
130.05	2115	141.00	6471	148.95	388	160.85	586
130.90	824	141.85	476	149.80	229	161.10	242
133.90	98	143.00	5597	150.10	641	168.50	83
134.90	847	144.00	614	151.85	248	169.60	81

Average of 13.780 to 13.786 min.: VL040215.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.10	75						
170.65	277						
171.85	1534						
172.20	351						
173.00	3086						
174.10	343104						
175.05	25461						
176.05	325589						
177.05	21469						
178.00	715						

Instrument :

MSVOA_L

ClientSampleId :

BFB