


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL022421\
 Data File : VL036343.D
 Acq On : 24 Feb 2021 8:46
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL021021AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Feb 10 16:04:02 2021
 Last Update : Wed Feb 10 16:04:02 2021

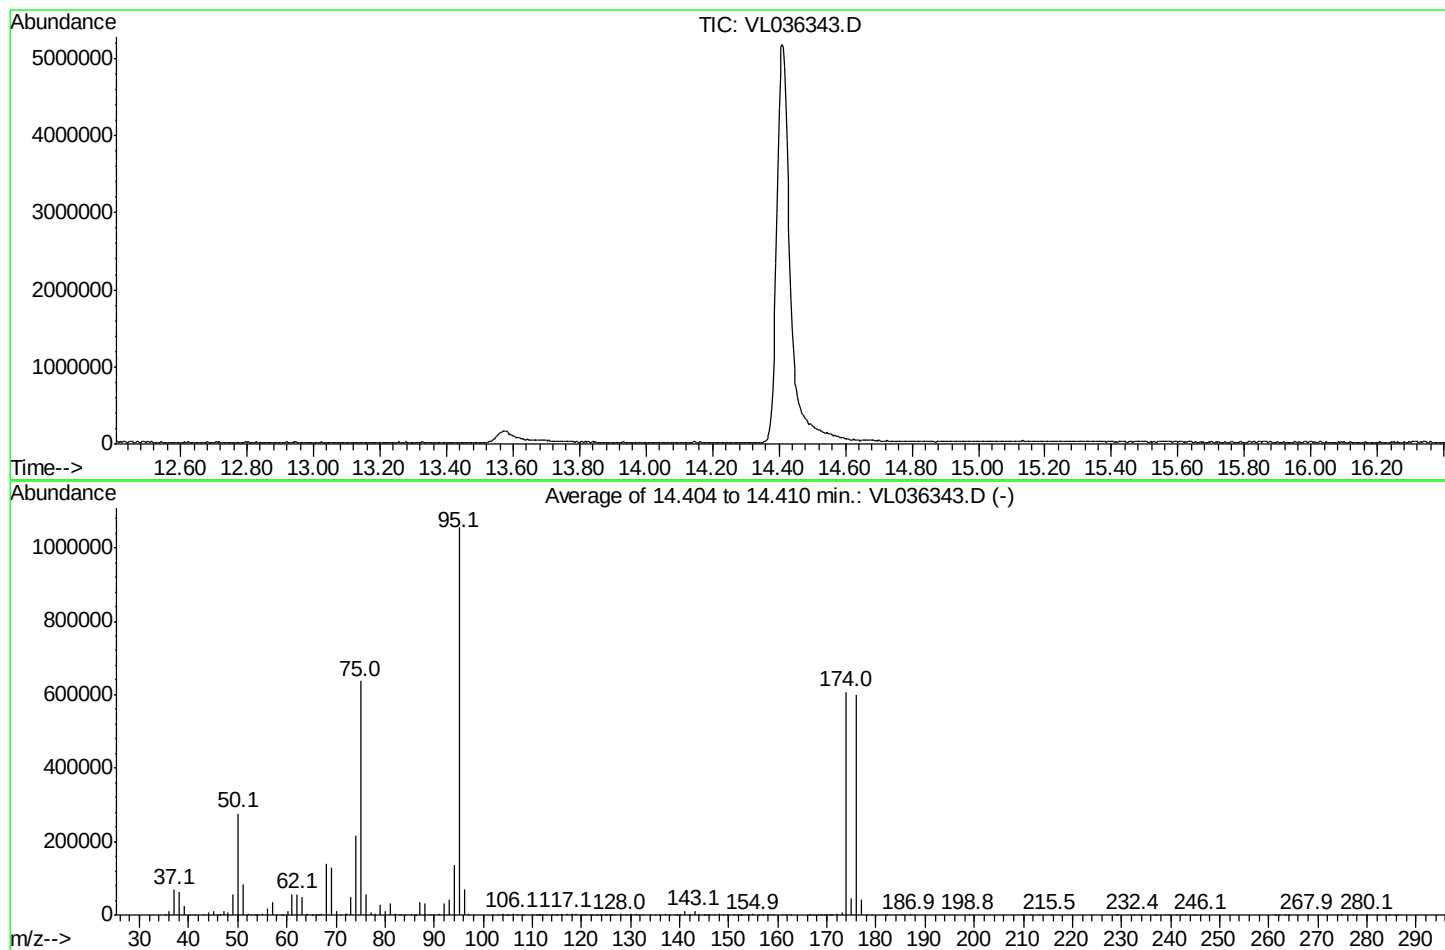

AutoFind: Scans 3613, 3614, 3615; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.2	276160	PASS
75	95	30	66	60.4	637371	PASS
95	95	100	100	100.0	1055637	PASS
96	95	5	9	6.8	71488	PASS
173	174	0.00	2	1.0	5809	PASS
174	95	50	120	57.5	607381	PASS
175	174	4	9	7.6	46263	PASS
176	174	93	101	98.9	600490	PASS
177	176	5	9	7.1	42890	PASS