


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022422\
 Data File : VL038430.D
 Acq On : 24 Feb 2022 10:30
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL022222AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
 Last Update : Tue Feb 22 19:45:51 2022

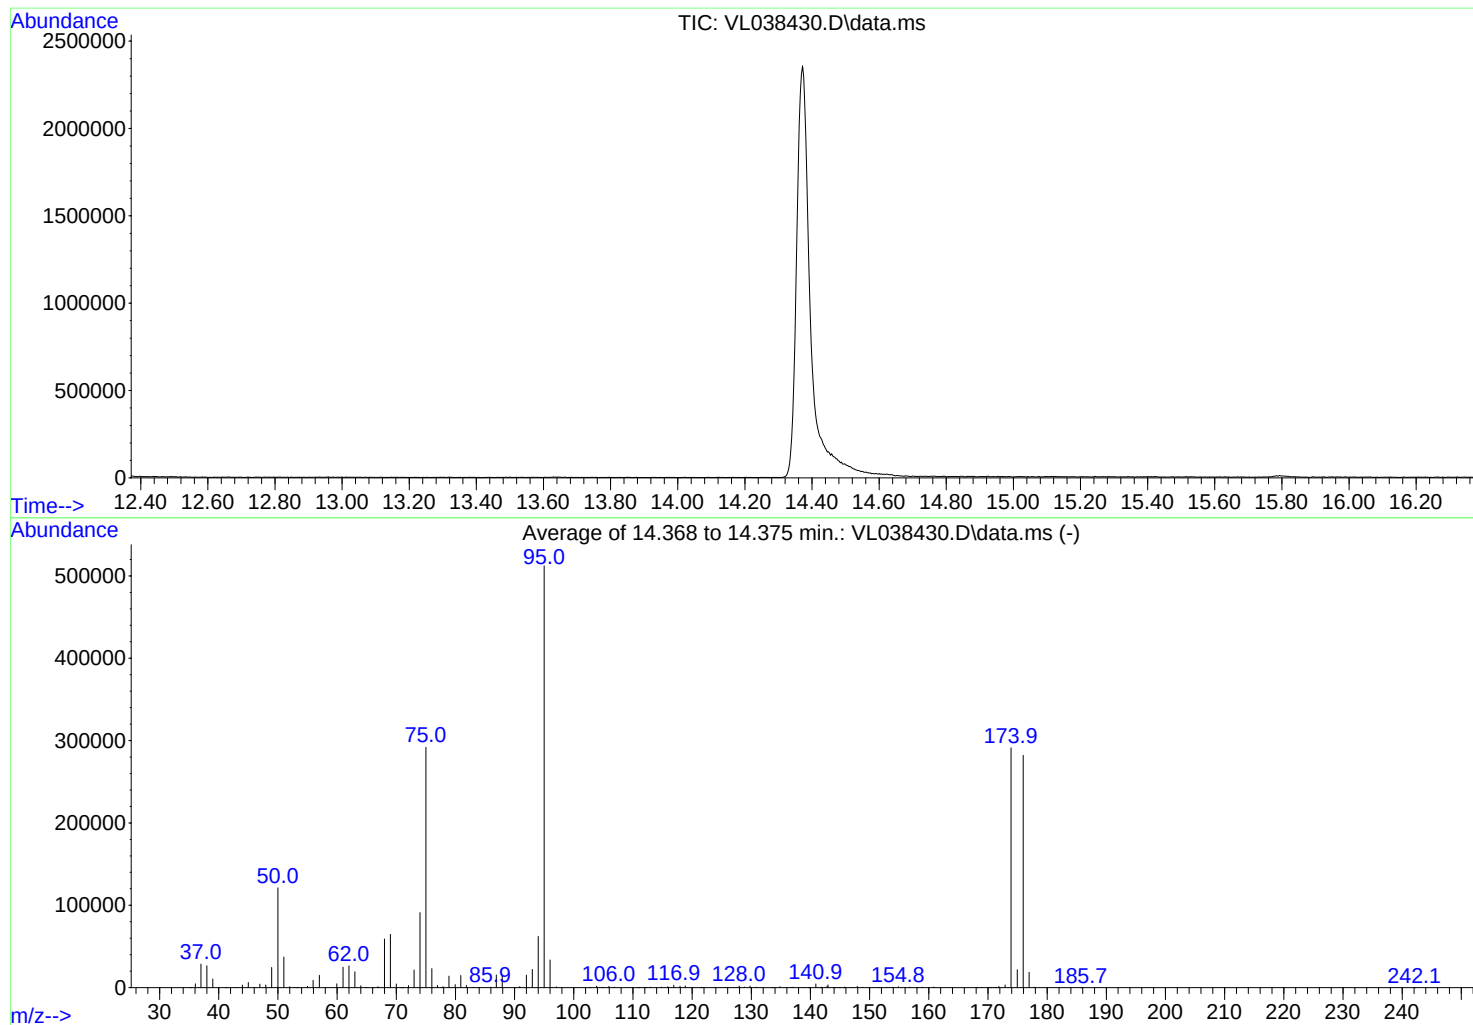

AutoFind: Scans 3602, 3603, 3604; Background Corrected with Scan 3579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.7	121291	PASS
75	95	30	66	57.0	291904	PASS
95	95	100	100	100.0	512213	PASS
96	95	5	9	6.6	33704	PASS
173	174	0.00	2	1.1	3280	PASS
174	95	50	120	56.9	291264	PASS
175	174	4	9	7.5	21861	PASS
176	174	93	101	96.9	282112	PASS
177	176	5	9	6.6	18621	PASS

Average of 14.368 to 14.375 min.: VL038430.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.20	54	46.95	4366	58.05	491	68.00	5905
36.05	4690	47.95	3402	59.95	4717	69.00	6482
37.00	28520	48.95	24499	61.00	24872	70.00	447
38.00	26637	50.00	121291	62.00	26413	70.80	12
39.00	10459	51.00	37144	63.00	19288	71.10	56
40.00	267	52.00	1106	64.00	2411	72.05	2586
41.20	110	52.85	231	64.80	249	73.00	21472
42.85	199	53.20	76	64.95	392	74.00	91197
44.00	3211	55.00	1608	66.00	55	75.00	291904
45.00	6169	55.95	8934	66.80	525	76.00	23203
45.90	479	57.00	14952	66.95	986	76.95	2677

Average of 14.368 to 14.375 min.: VL038430.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.70	495	90.80	1232	105.00	353	116.90	2865
77.90	1120	91.00	547	105.95	1600	117.95	1747
78.90	13927	92.00	15119	106.85	584	118.85	2146
79.95	3686	93.00	22136	110.00	192	120.10	143
80.90	14728	94.00	62208	110.80	300	121.50	78
81.85	2846	95.00	512213	111.00	115	121.85	141
83.00	428	96.00	33704	111.80	285	123.85	413
83.85	120	97.05	1037	112.10	102	124.85	161
85.90	574	102.70	59	112.95	603	125.60	137
86.90	15417	103.85	1844	114.85	542	126.00	190
87.90	15010	104.75	511	115.90	1241	126.95	210

Average of 14.368 to 14.375 min.: VL038430.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
127.95	1990	140.90	4559	146.85	246	158.85	561
128.85	882	141.70	122	147.90	1505	160.85	728
129.80	1866	141.90	569	148.85	372	168.10	92
130.90	574	142.80	1788	149.85	434	168.90	167
133.50	76	142.95	3307	151.65	209	170.20	318
134.85	1105	143.90	263	152.80	424	170.50	109
136.75	466	144.10	52	153.85	265	170.95	399
137.05	590	144.60	279	154.85	1115	171.30	99
139.05	164	144.90	94	156.00	278	171.85	1380
139.70	54	145.60	105	156.80	642	172.90	3280
140.00	293	145.80	741	158.00	68	173.90	291264

Average of 14.368 to 14.375 min.: VL038430.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.95	21861						
175.95	282112						
176.95	18621						
177.90	652						
185.70	51						
242.10	65						