


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL022621\
 Data File : VL036395.D
 Acq On : 26 Feb 2021 9:09
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL021021AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Feb 10 16:04:02 2021
 Last Update : Wed Feb 10 16:04:02 2021

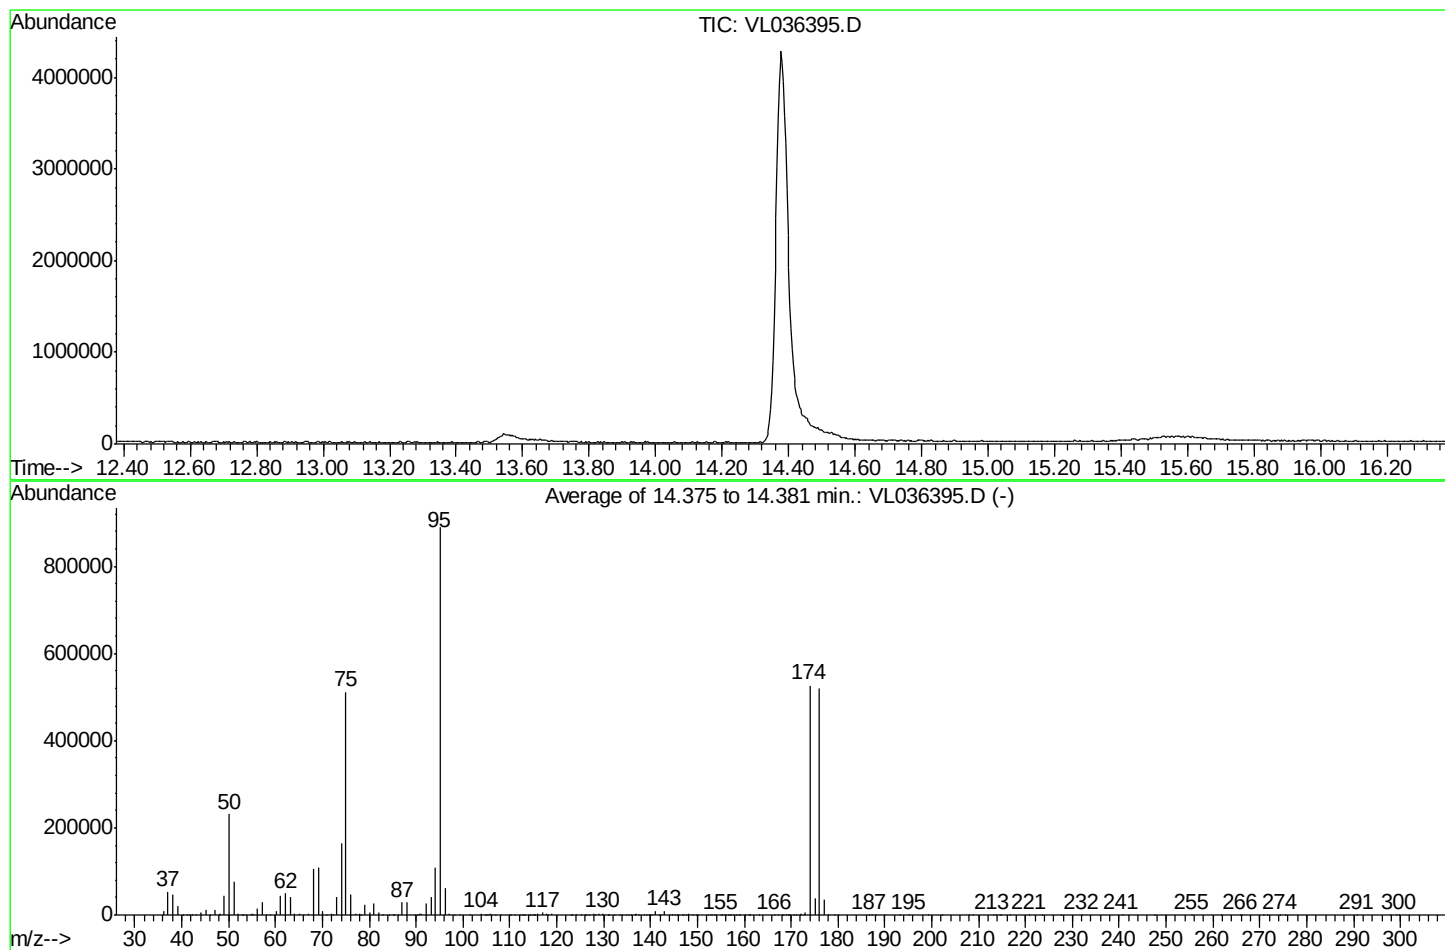

AutoFind: Scans 3604, 3605, 3606; Background Corrected with Scan 3582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.9	230677	PASS
75	95	30	66	57.6	512250	PASS
95	95	100	100	100.0	889338	PASS
96	95	5	9	6.8	60456	PASS
173	174	0.00	2	1.2	6076	PASS
174	95	50	120	59.2	526250	PASS
175	174	4	9	7.4	38738	PASS
176	174	93	101	98.6	518890	PASS
177	176	5	9	6.7	34912	PASS