

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022625\
 Data File : VL042058.D
 Acq On : 26 Feb 2025 13:21
 Operator : SY/MD
 Sample : Q1430-06
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 OA1

Quant Time: Feb 27 00:29:18 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL022525AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Wed Feb 26 01:08:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	2.797	49	158058	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.971	114	369297	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.898	117	320901	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.390	95	250640	10.152	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.500%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.502	85	7122	0.433	ppbv	96
3) Chlorodifluoromethane	1.479	51	24763	1.078	ppbv #	81
4) Chloromethane	1.538	50	8995	1.480	ppbv	92
6) Bromomethane	1.673	94	101	0.037	ppbv #	55
7) Chloroethane	1.706	64	183	0.078	ppbv #	39
9) Propene	1.489	41	12657	1.352	ppbv	87
10) Heptane	4.997	43	2857	0.098	ppbv #	77
11) Trichlorofluoromethane	1.884	101	3953	0.240	ppbv	89
12) 1,1,2-Trichlorotrifluo...	2.149	101	899	0.068	ppbv	97
13) Ethanol	1.725	45	38875	65.437	ppbv	90
15) Acetone	1.842	43	132778	9.513	ppbv	99
16) 1,3-Butadiene	1.609	39	2679	0.412	ppbv #	57
17) tert-Butyl alcohol	2.052	59	4414	0.253	ppbv	95
19) Isopropyl Alcohol	1.894	45	42856	5.345	ppbv #	46
20) Methylene Chloride	2.068	84	10038	1.901	ppbv	94
21) Allyl Chloride	2.088	41	317	0.031	ppbv #	4
23) Vinyl Acetate	2.460	43	13121	1.337	ppbv #	83
25) Ethyl Acetate	2.842	43	18702	0.335	ppbv #	92
26) Hexane	2.835	57	13945	0.617	ppbv #	59
29) Chloroform	2.855	83	3270	0.108	ppbv	100
30) Cyclohexane	3.874	84	933	0.051	ppbv #	1
34) 2-Butanone	2.570	43	21157	0.735	ppbv	95
35) Carbon Tetrachloride	3.777	117	1237	0.049	ppbv #	72
36) Benzene	3.674	78	12783	0.331	ppbv	98
39) 1,2-Dichloropropane	3.971	63	100377	6.841	ppbv #	24
43) Methyl Methacrylate	4.907	69	994	0.066	ppbv #	1
44) 2,2,4-Trimethylpentane	4.661	57	9419	0.138	ppbv #	71
52) Tetrachloroethene	8.244	164	688	0.052	ppbv #	61
53) Toluene	6.959	91	35528	0.822	ppbv	97
58) Ethyl Benzene	9.564	91	4573	0.077	ppbv	92
59) m/p-Xylene	9.548	91	11312	0.241	ppbv #	100
60) o-Xylene	9.975	91	5607	0.119	ppbv	99
74) 1,2,4-Trimethylbenzene	11.548	105	5213	0.092	ppbv #	61
79) Naphthalene	13.526	128	1374	0.036	ppbv #	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022625\
Data File : VL042058.D
Acq On : 26 Feb 2025 13:21
Operator : SY/MD
Sample : Q1430-06
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
OA1

Quant Time: Feb 27 00:29:18 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL022525AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Wed Feb 26 01:08:36 2025
Response via : Initial Calibration




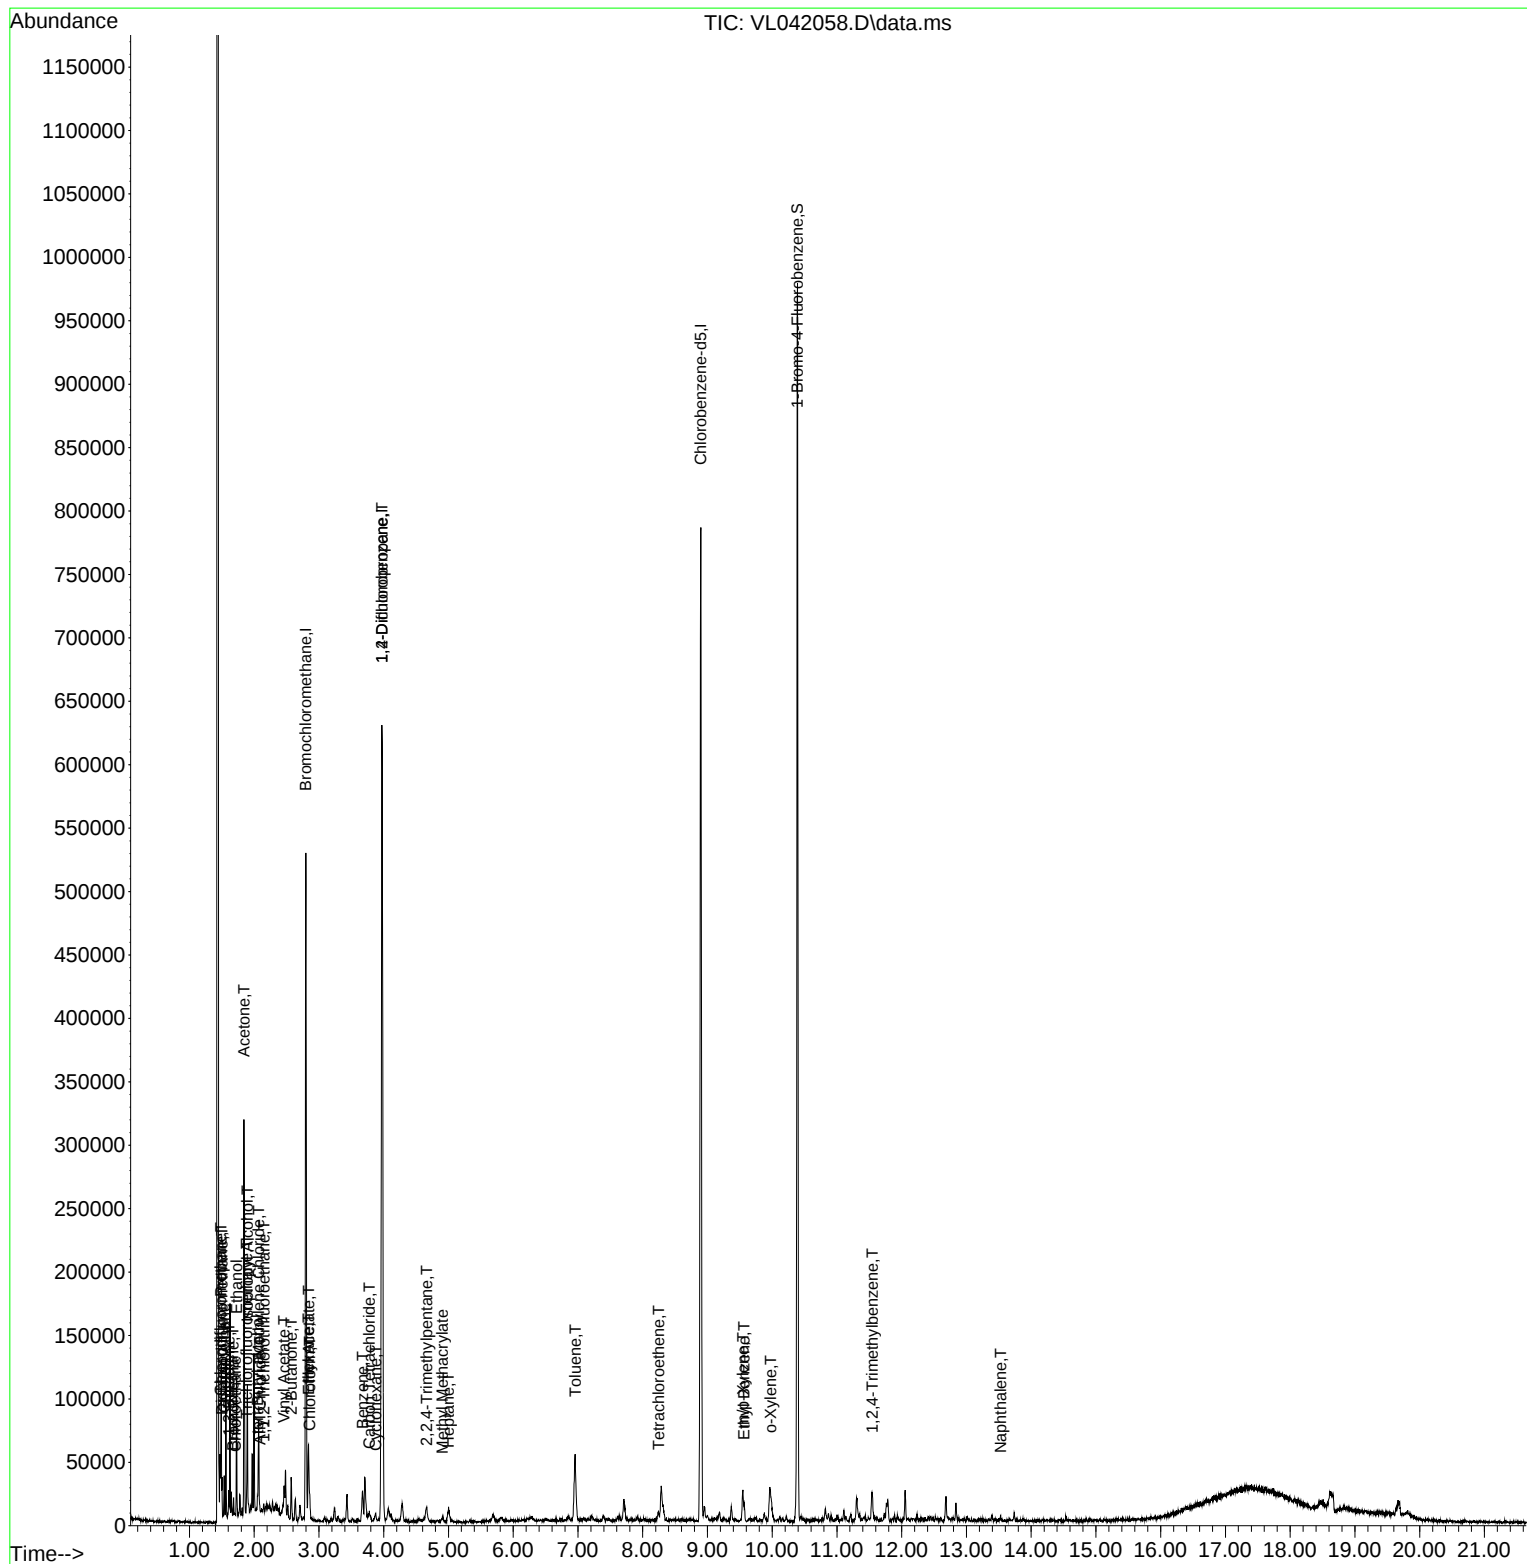




#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.797 min Scan# 81
Delta R.T. -0.003 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21




Instrument :
MSVOA_L
ClientSampleId :
OA1


Tgt Ion: 49 Resp: 158058
Ion Ratio Lower Upper
49 100
128 41.2 21.6 64.8
130 52.5 27.8 83.4

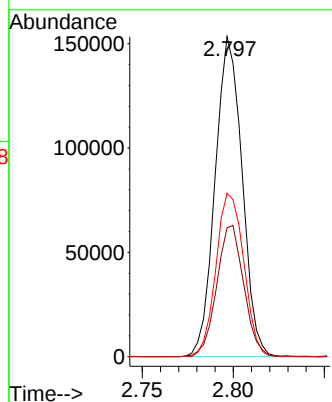

#2
Dichlorodifluoromethane
Concen: 0.433 ppbv
RT: 1.502 min Scan# 437
Delta R.T. -0.000 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21

Tgt Ion: 85 Resp: 7122
Ion Ratio Lower Upper
85 100
87 30.7 26.4 39.6



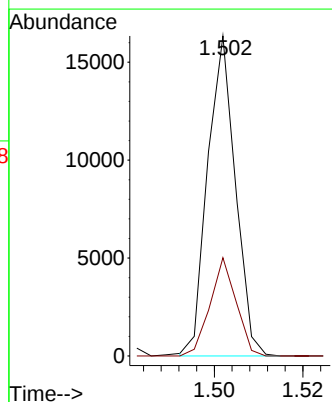





#3
Chlorodifluoromethane
Concen: 1.078 ppbv
RT: 1.479 min Scan# 41
Delta R.T. -0.000 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21




Instrument :
MSVOA_L
ClientSampleId :
OA1


Tgt Ion: 51 Resp: 24763
Ion Ratio Lower Upper
51 100
67 8.9 13.7 20.5#

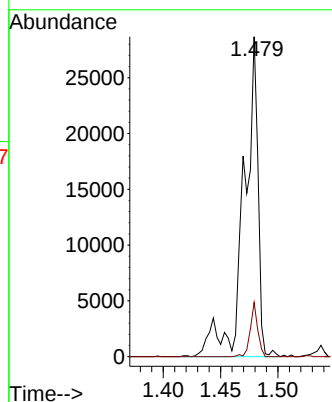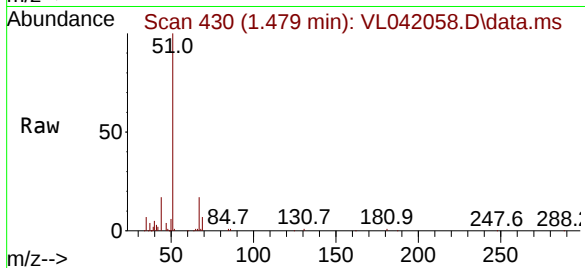

#4
Chloromethane
Concen: 1.480 ppbv
RT: 1.538 min Scan# 448
Delta R.T. -0.000 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21

Tgt Ion: 50 Resp: 8995
Ion Ratio Lower Upper
50 100
52 35.9 25.4 38.0


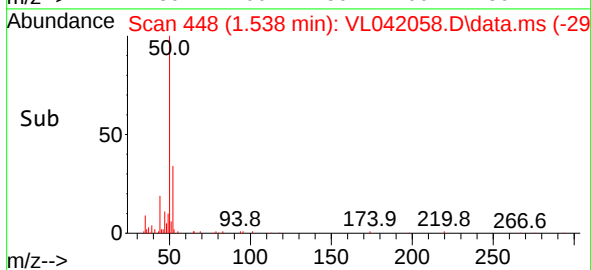
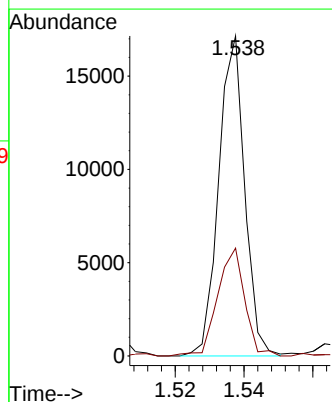
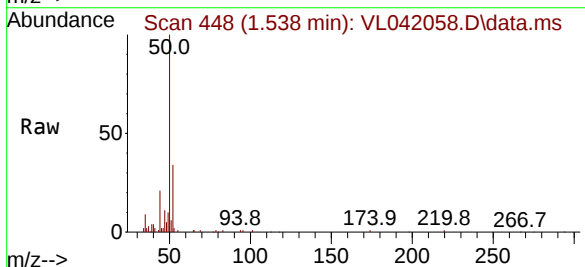




#6
Bromomethane
Concen: 0.037 ppbv
RT: 1.673 min Scan# 490
Delta R.T. -0.000 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21




Instrument :
MSVOA_1
ClientSampleId :
OA1


Tgt Ion: 94 Resp: 101
Ion Ratio Lower Upper
94 100
96 52.1 76.5 114.7#

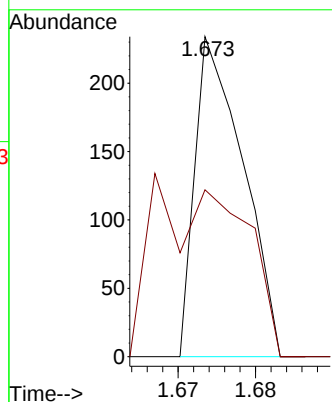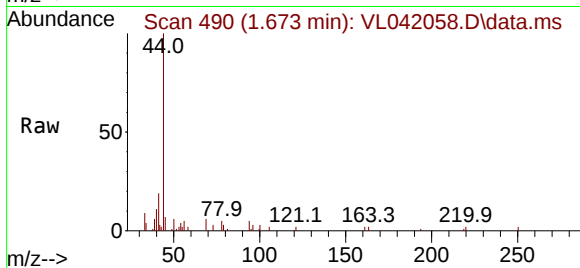

#7
Chloroethane
Concen: 0.078 ppbv
RT: 1.706 min Scan# 500
Delta R.T. -0.003 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21

Tgt Ion: 64 Resp: 183
Ion Ratio Lower Upper
64 100
66 0.0 28.4 42.6#

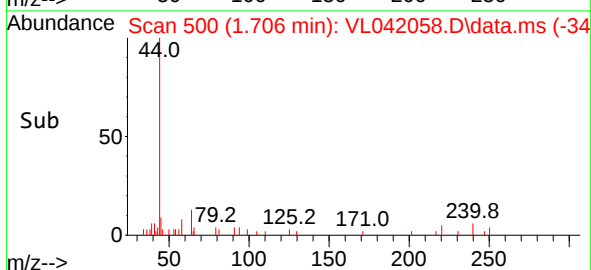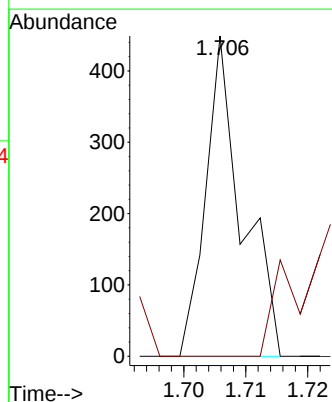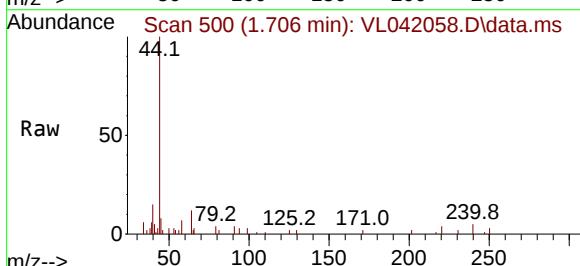



#9

Propene

Concen: 1.352 ppbv

RT: 1.489 min Scan# 41

Delta R.T. -0.000 min

Lab File: VL042058.D

Acq: 26 Feb 2025 13:21

Instrument :

MSVOA_L

ClientSampleId :





OA1

Tgt Ion: 41 Resp: 12657

Ion Ratio Lower Upper

41 100

42 59.2 55.8 83.6

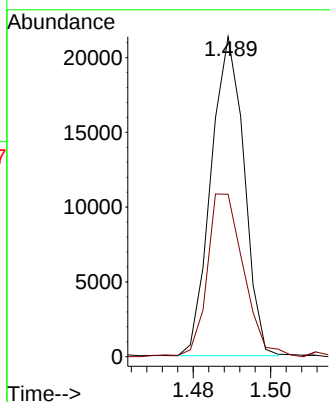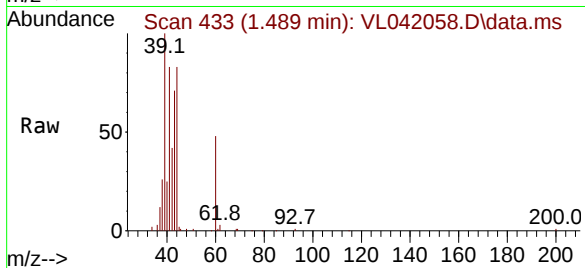

#10

Heptane

Concen: 0.098 ppbv

RT: 4.997 min Scan# 1517

Delta R.T. -0.010 min

Lab File: VL042058.D




Acq: 26 Feb 2025 13:21


Tgt Ion: 43 Resp: 2857

Ion Ratio Lower Upper

43 100

57 64.8 39.4 59.0#


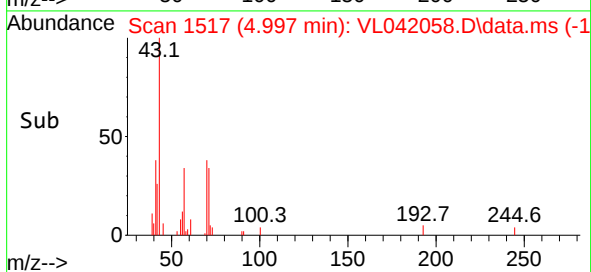
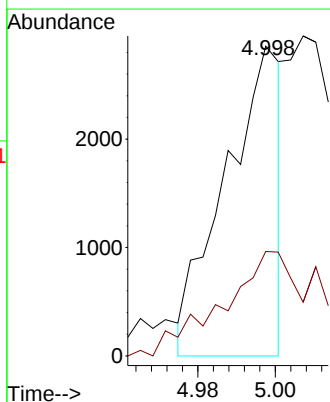
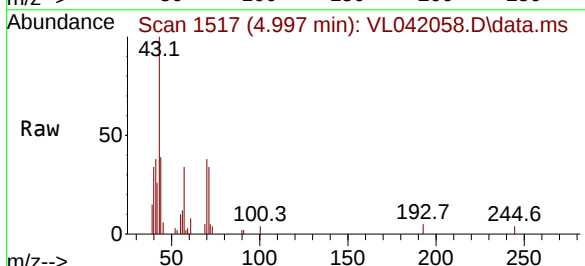




#11
 Trichlorofluoromethane
 Concen: 0.240 ppbv
 RT: 1.884 min Scan# 511
 Delta R.T. -0.000 min
 Lab File: VL042058.D
 Acq: 26 Feb 2025 13:21




Instrument :
 MSVOA_L
 ClientSampleId :
 OA1


Tgt Ion:101 Resp: 3953
 Ion Ratio Lower Upper
 101 100
 103 71.8 50.6 75.8

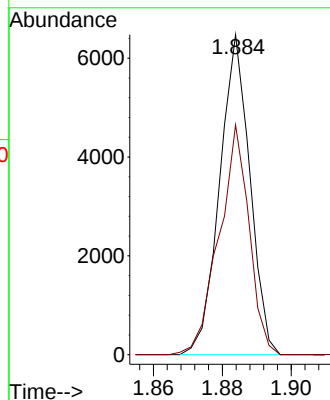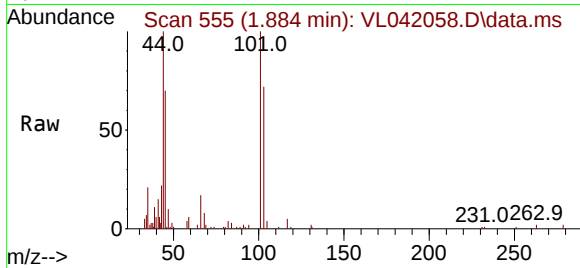

#12
 1,1,2-Trichlorotrifluoroethane
 Concen: 0.068 ppbv
 RT: 2.149 min Scan# 637
 Delta R.T. 0.003 min
 Lab File: VL042058.D
 Acq: 26 Feb 2025 13:21

Tgt Ion:101 Resp: 899
 Ion Ratio Lower Upper
 101 100
 151 75.9 62.6 94.0



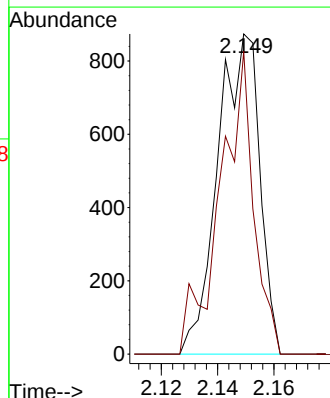
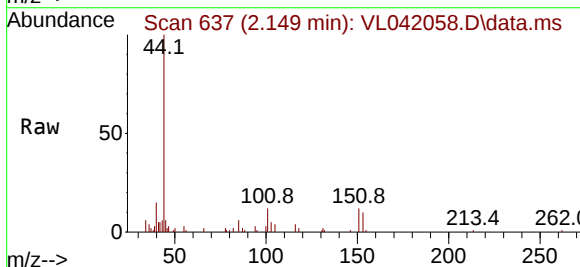




#13
Ethanol
Concen: 65.437 ppbv
RT: 1.725 min Scan# 507
Delta R.T. -0.003 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21




Instrument :
MSVOA_L
ClientSampleId :
OA1


Tgt Ion: 45 Resp: 38875
Ion Ratio Lower Upper
45 100
46 36.6 17.1 68.3

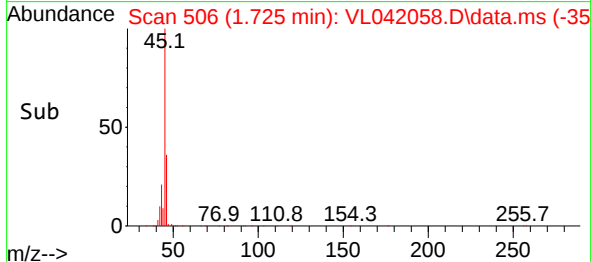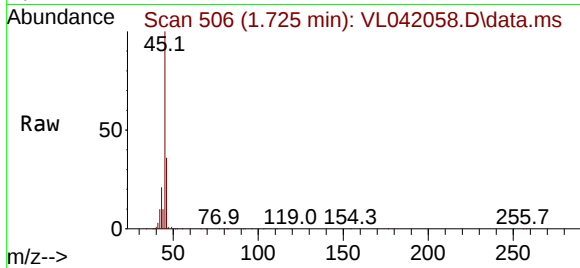

#15
Acetone
Concen: 9.513 ppbv
RT: 1.842 min Scan# 542
Delta R.T. -0.000 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21

Tgt Ion: 43 Resp: 132778
Ion Ratio Lower Upper
43 100
58 25.6 20.7 31.1




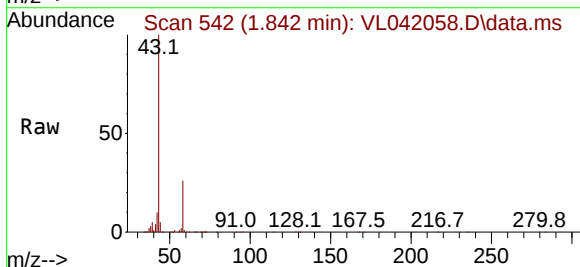




#16
1,3-Butadiene
Concen: 0.412 ppbv
RT: 1.609 min Scan# 41
Delta R.T. -0.007 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21




Instrument :
MSVOA_L
ClientSampleId :
OA1


Tgt Ion: 39 Resp: 2679
Ion Ratio Lower Upper
39 100
54 38.4 59.6 89.4#

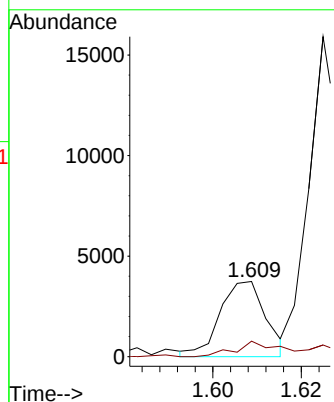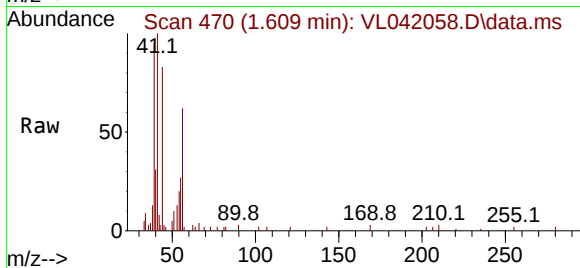

#17
tert-Butyl alcohol
Concen: 0.253 ppbv
RT: 2.052 min Scan# 607
Delta R.T. 0.003 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21

Tgt Ion: 59 Resp: 4414
Ion Ratio Lower Upper
59 100
57 13.7 9.3 13.9



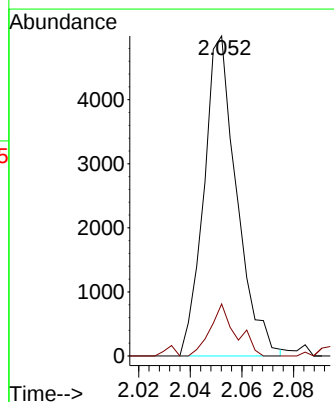
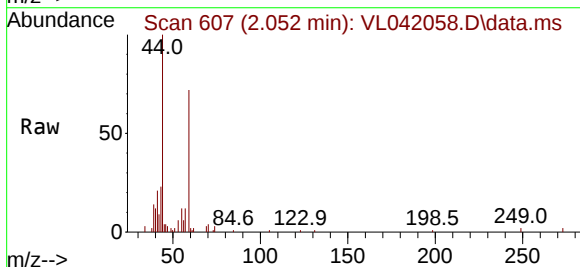




#19
Isopropyl Alcohol
Concen: 5.345 ppbv
RT: 1.894 min Scan# 511
Delta R.T. -0.000 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21




Instrument :
MSVOA_1
ClientSampleId :
OA1


Tgt Ion: 45 Resp: 42856
Ion Ratio Lower Upper
45 100
58 79.3 35.3 52.9#

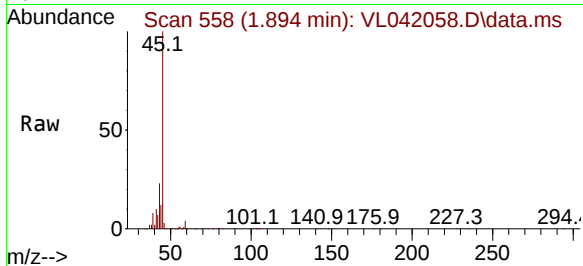

#20
Methylene Chloride
Concen: 1.901 ppbv
RT: 2.068 min Scan# 612
Delta R.T. -0.000 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21

Tgt Ion: 84 Resp: 10038
Ion Ratio Lower Upper
84 100
49 150.9 130.0 195.0
51 48.0 37.4 56.0
86 61.4 48.6 72.8

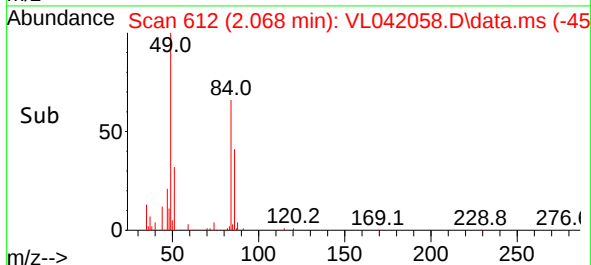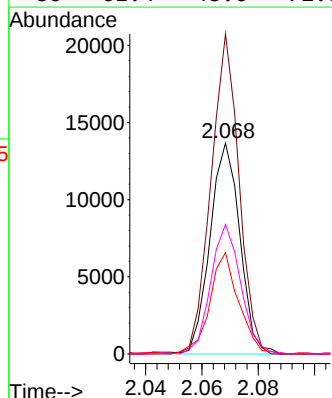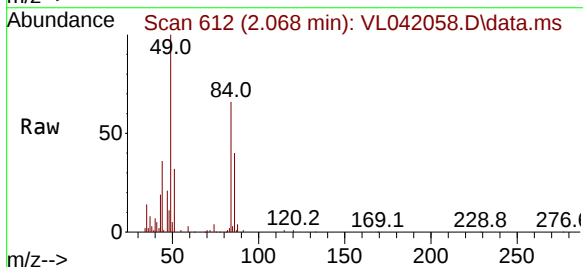



#21

Allyl Chloride

Concen: 0.031 ppbv

RT: 2.088 min Scan# 618

Delta R.T. -0.016 min

Lab File: VL042058.D

Acq: 26 Feb 2025 13:21

Instrument :

MSVOA_L

ClientSampleId :

OA1





Tgt Ion: 41 Resp: 317

Ion Ratio Lower Upper

41 100

76 0.0 23.8 35.6#

39 178.2 63.8 95.6#

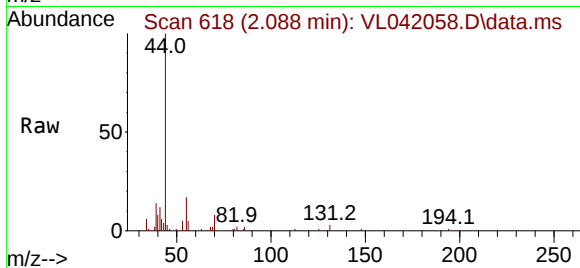

#23

Vinyl Acetate

Concen: 1.337 ppbv

RT: 2.460 min Scan# 733

Delta R.T. -0.013 min

Lab File: VL042058.D

Acq: 26 Feb 2025 13:21

Tgt Ion: 43 Resp: 13121




Ion Ratio Lower Upper


43 100

86 5.9 7.0 10.4#

42 7.9 7.6 11.4

44 22.8 5.0 7.4#


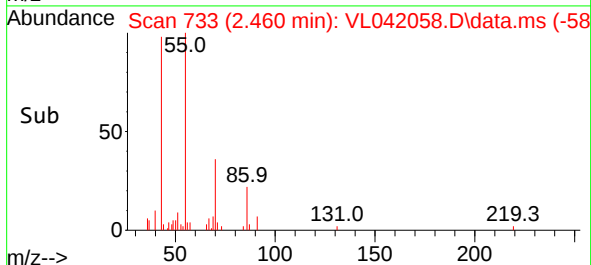
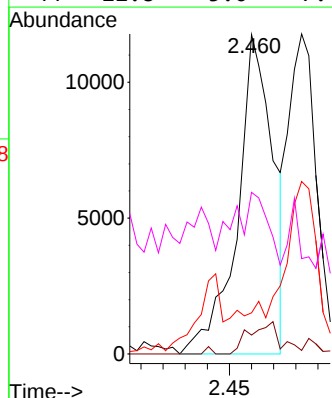
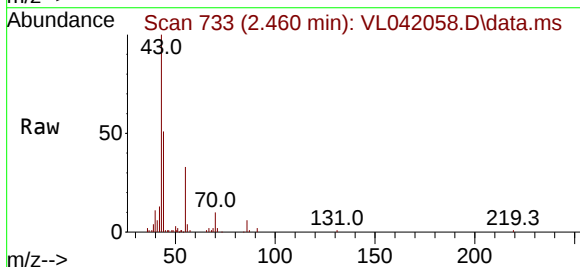




#25
Ethyl Acetate
Concen: 0.335 ppbv
RT: 2.842 min Scan# 81
Delta R.T. -0.010 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21




Instrument :
MSVOA_L
ClientSampleId :
OA1


Tgt Ion: 43	Resp: 18702
Ion Ratio	Lower Upper
43 100	
45 12.4	8.1 12.1#
61 4.7	7.2 10.8#
70 6.3	6.7 10.1#

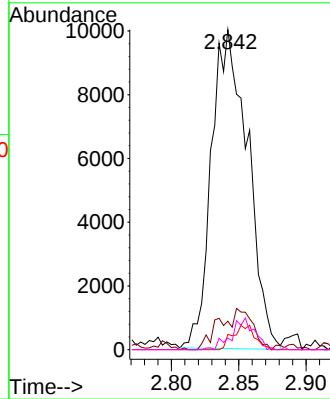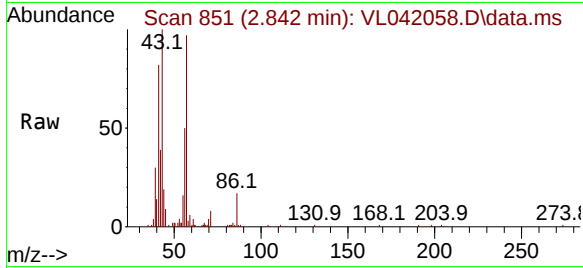

#26
Hexane
Concen: 0.617 ppbv
RT: 2.835 min Scan# 849
Delta R.T. -0.003 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21

Tgt Ion: 57	Resp: 13945
Ion Ratio	Lower Upper
57 100	
41 89.2	70.6 106.0
43 140.0	199.4 299.0#
56 58.7	42.6 64.0

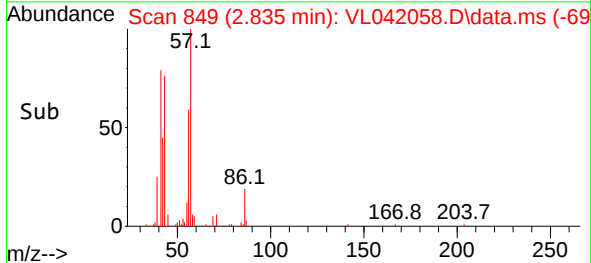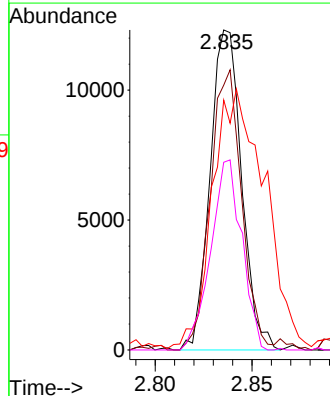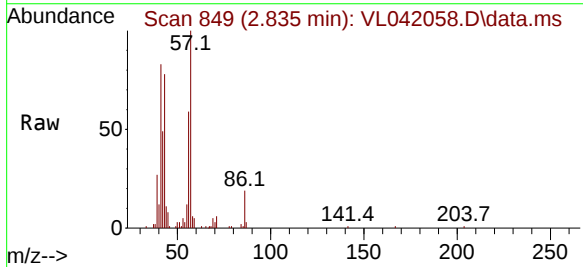



#29

Chloroform

Concen: 0.108 ppbv

RT: 2.855 min Scan# 8

Delta R.T. -0.007 min

Lab File: VL042058.D

Acq: 26 Feb 2025 13:21

Instrument :

MSVOA_L

ClientSampleId :





OA1

Tgt Ion: 83 Resp: 3270

Ion Ratio Lower Upper

83 100

85 64.3 51.2 76.8

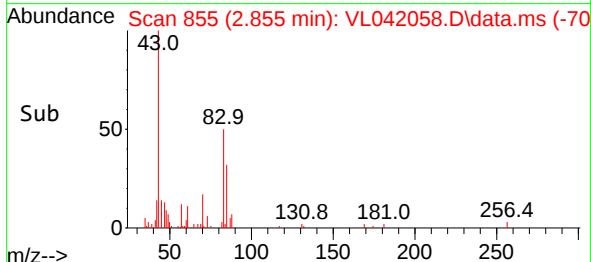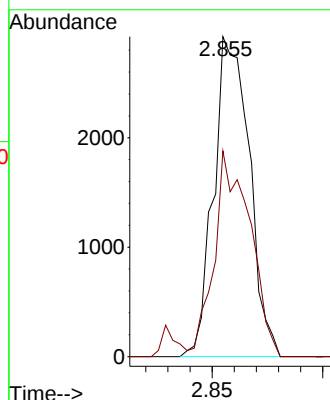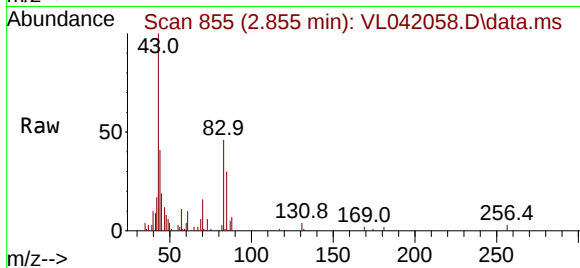

#30

Cyclohexane

Concen: 0.051 ppbv

RT: 3.874 min Scan# 1170

Delta R.T. -0.000 min

Lab File: VL042058.D

Acq: 26 Feb 2025 13:21




Tgt Ion: 84 Resp: 933


Ion Ratio Lower Upper

84 100

56 279.1 101.5 152.3#

41 262.1 62.6 93.8#


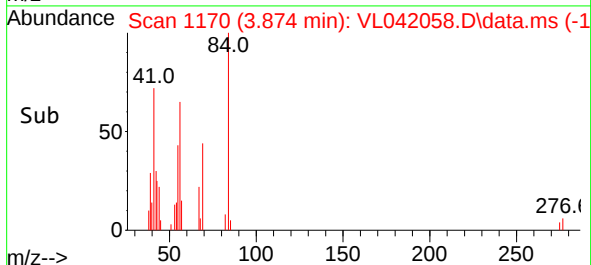
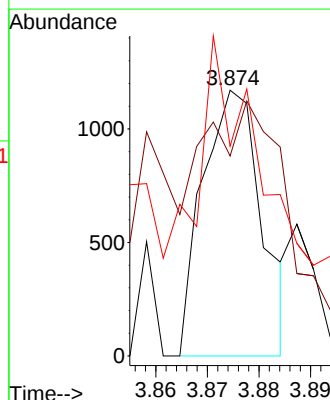
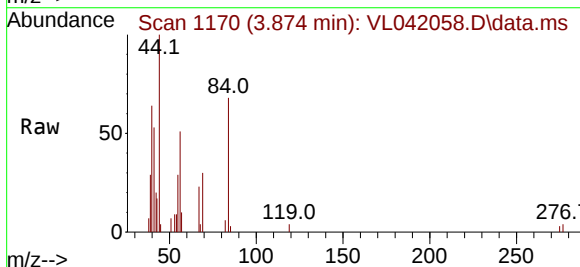




#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 3.971 min Scan# 114
 Delta R.T. -0.007 min
 Lab File: VL042058.D
 Acq: 26 Feb 2025 13:21




Instrument :
 MSVOA_L
 ClientSampleId :
 OA1


Tgt Ion:114 Resp: 369297
 Ion Ratio Lower Upper
 114 100
 63 27.2 20.1 30.1
 88 18.7 14.3 21.5

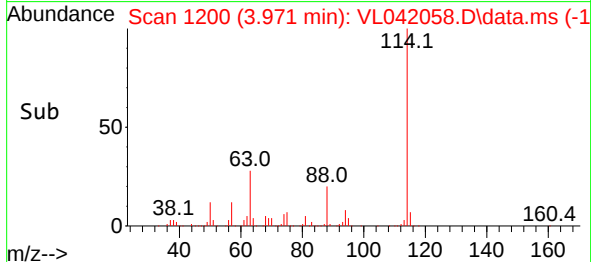

#34
 2-Butanone
 Concen: 0.735 ppbv
 RT: 2.570 min Scan# 767
 Delta R.T. -0.000 min
 Lab File: VL042058.D
 Acq: 26 Feb 2025 13:21

Tgt Ion: 43 Resp: 21157
 Ion Ratio Lower Upper
 43 100
 72 20.9 18.5 27.7









#35
Carbon Tetrachloride
Concen: 0.049 ppbv
RT: 3.777 min Scan# 1141
Delta R.T. -0.003 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21




Instrument :
MSVOA_L
ClientSampleId :
OA1


Tgt Ion:117 Resp: 1237
Ion Ratio Lower Upper
117 100
119 131.1 77.8 116.8#
121 32.1 23.4 35.0



#36
Benzene
Concen: 0.331 ppbv
RT: 3.674 min Scan# 1108
Delta R.T. -0.000 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21

Tgt Ion: 78 Resp: 12783
Ion Ratio Lower Upper
78 100
77 23.3 17.7 26.5
50 17.7 13.9 20.9

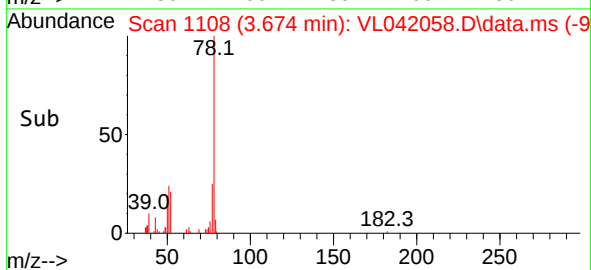



#39

1,2-Dichloropropane

Concen: 6.841 ppbv

RT: 3.971 min Scan# 11

Delta R.T. -0.366 min

Lab File: VL042058.D

Acq: 26 Feb 2025 13:21

Instrument :

MSVOA_L

ClientSampleId :

OA1





Tgt Ion: 63 Resp: 100377

Ion Ratio Lower Upper

63 100

41 0.0 60.1 90.1#

62 17.7 55.8 83.8#

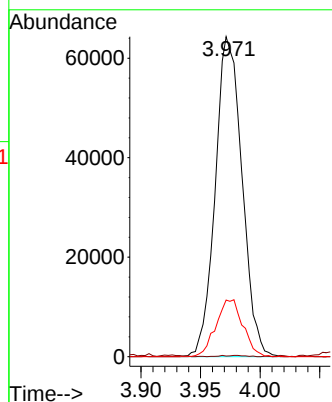

#43

Methyl Methacrylate

Concen: 0.066 ppbv

RT: 4.907 min Scan# 1489

Delta R.T. -0.000 min

Lab File: VL042058.D

Acq: 26 Feb 2025 13:21




Tgt Ion: 69 Resp: 994


Ion Ratio Lower Upper

69 100

41 0.0 118.2 177.4#

100 0.0 27.0 40.4#


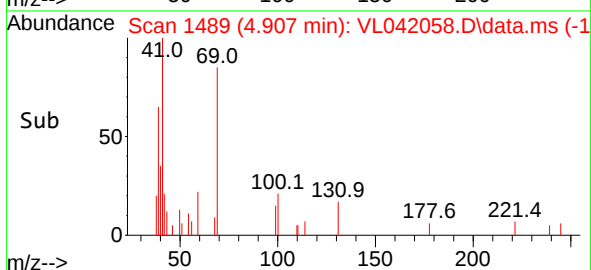






#44
2,2,4-Trimethylpentane
Concen: 0.138 ppbv
RT: 4.661 min Scan# 1413
Delta R.T. -0.000 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21




Instrument :
MSVOA_L
ClientSampleId :
OA1


Tgt Ion: 57 Resp: 9419
Ion Ratio Lower Upper
57 100
41 51.3 24.4 36.6#
56 44.7 26.5 39.7#

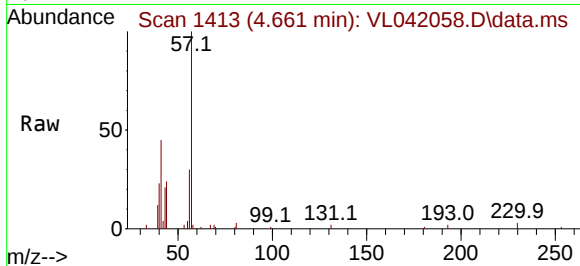

#52
Tetrachloroethene
Concen: 0.052 ppbv
RT: 8.244 min Scan# 2520
Delta R.T. -0.000 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21

Tgt Ion: 164 Resp: 688
Ion Ratio Lower Upper
164 100
166 96.3 95.7 143.5
129 30.7 77.1 115.7#
131 62.7 76.0 114.0#




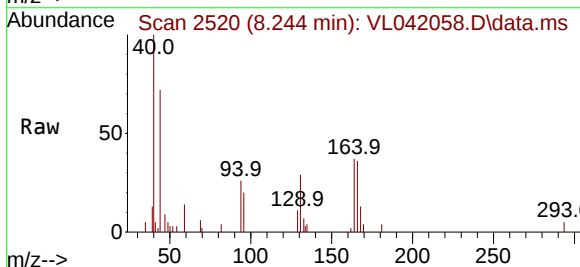




#53
Toluene
Concen: 0.822 ppbv
RT: 6.959 min Scan# 2123
Delta R.T. -0.000 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21




Instrument :
MSVOA_L
ClientSampleId :
OA1


Tgt Ion: 91 Resp: 35528
Ion Ratio Lower Upper
91 100
92 58.8 49.0 73.6

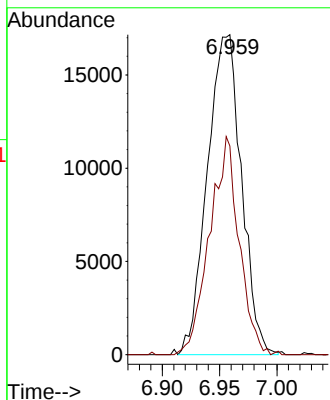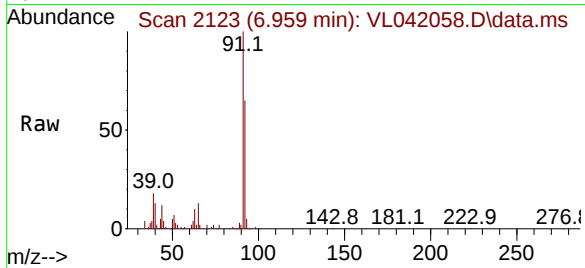

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.898 min Scan# 2722
Delta R.T. -0.003 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21

Tgt Ion: 117 Resp: 320901
Ion Ratio Lower Upper
117 100
82 68.3 55.0 82.6
119 31.7 25.9 38.9


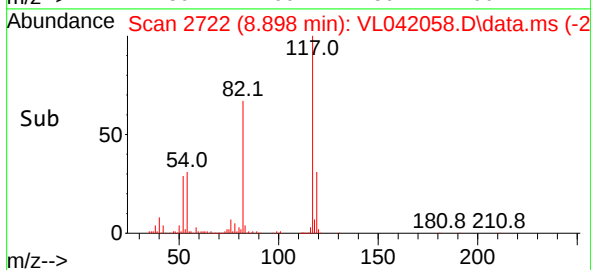
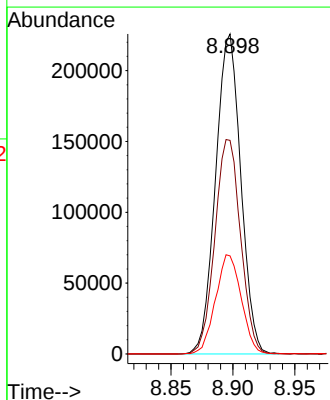
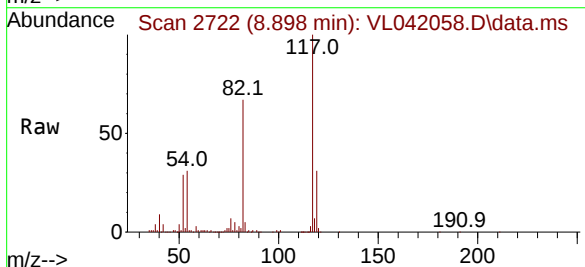




#58
Ethyl Benzene
Concen: 0.077 ppbv
RT: 9.564 min Scan# 2928
Delta R.T. 0.191 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21




Instrument :
MSVOA_L
ClientSampleId :
OA1


Tgt Ion: 91 Resp: 4573
Ion Ratio Lower Upper
91 100
106 34.5 24.2 36.2

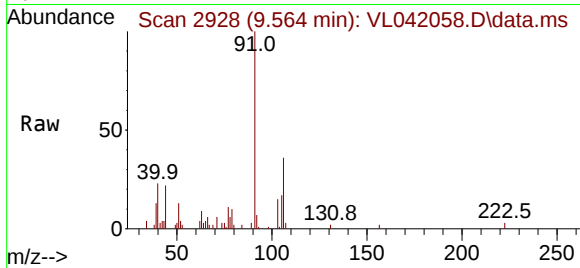

#59
m/p-Xylene
Concen: 0.241 ppbv
RT: 9.548 min Scan# 2923
Delta R.T. -0.003 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21

Tgt Ion: 91 Resp: 11312
Ion Ratio Lower Upper
91 100
106 63.9 0.0 0.0#




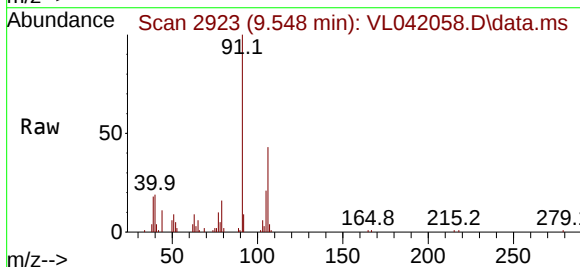




#60
o-Xylene
Concen: 0.119 ppbv
RT: 9.975 min Scan# 3057
Delta R.T. -0.007 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21




Instrument :
MSVOA_L
ClientSampleId :
OA1


Tgt Ion: 91 Resp: 5607
Ion Ratio Lower Upper
91 100
106 44.1 22.3 66.8

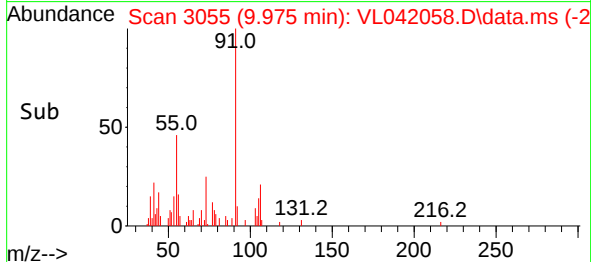

#68
1-Bromo-4-Fluorobenzene
Concen: 10.152 ppbv
RT: 10.390 min Scan# 3183
Delta R.T. -0.003 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21

Tgt Ion: 95 Resp: 250640
Ion Ratio Lower Upper
95 100
174 61.8 51.8 77.6
175 4.5 3.9 5.9


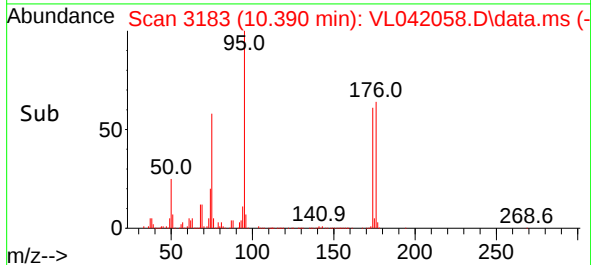






#74
1,2,4-Trimethylbenzene
Concen: 0.092 ppbv
RT: 11.548 min Scan# 3541
Delta R.T. -0.003 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21

Instrument :
MSVOA_L
ClientSampleId :
OA1

Tgt Ion:105 Resp: 5213
Ion Ratio Lower Upper
105 100
120 42.1 40.2 60.2
91 9.2 51.4 77.2#
77 19.3 20.1 30.1#

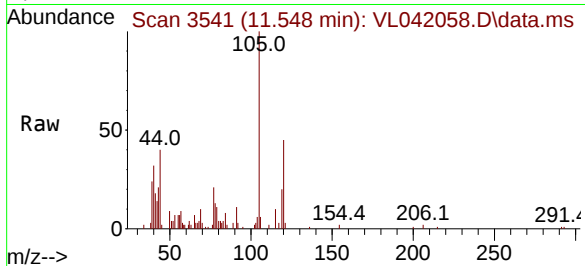

#79
Naphthalene
Concen: 0.036 ppbv
RT: 13.526 min Scan# 4152
Delta R.T. -0.000 min
Lab File: VL042058.D
Acq: 26 Feb 2025 13:21

Tgt Ion:128 Resp: 1374
Ion Ratio Lower Upper
128 100
127 7.4 9.8 14.6#
129 8.3 8.6 12.8#

