


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL022720\
 Data File : VL034703.D
 Acq On : 27 Feb 2020 9:42
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL022620AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Feb 28 01:15:02 2020
 Last Update : Fri Feb 28 01:15:02 2020

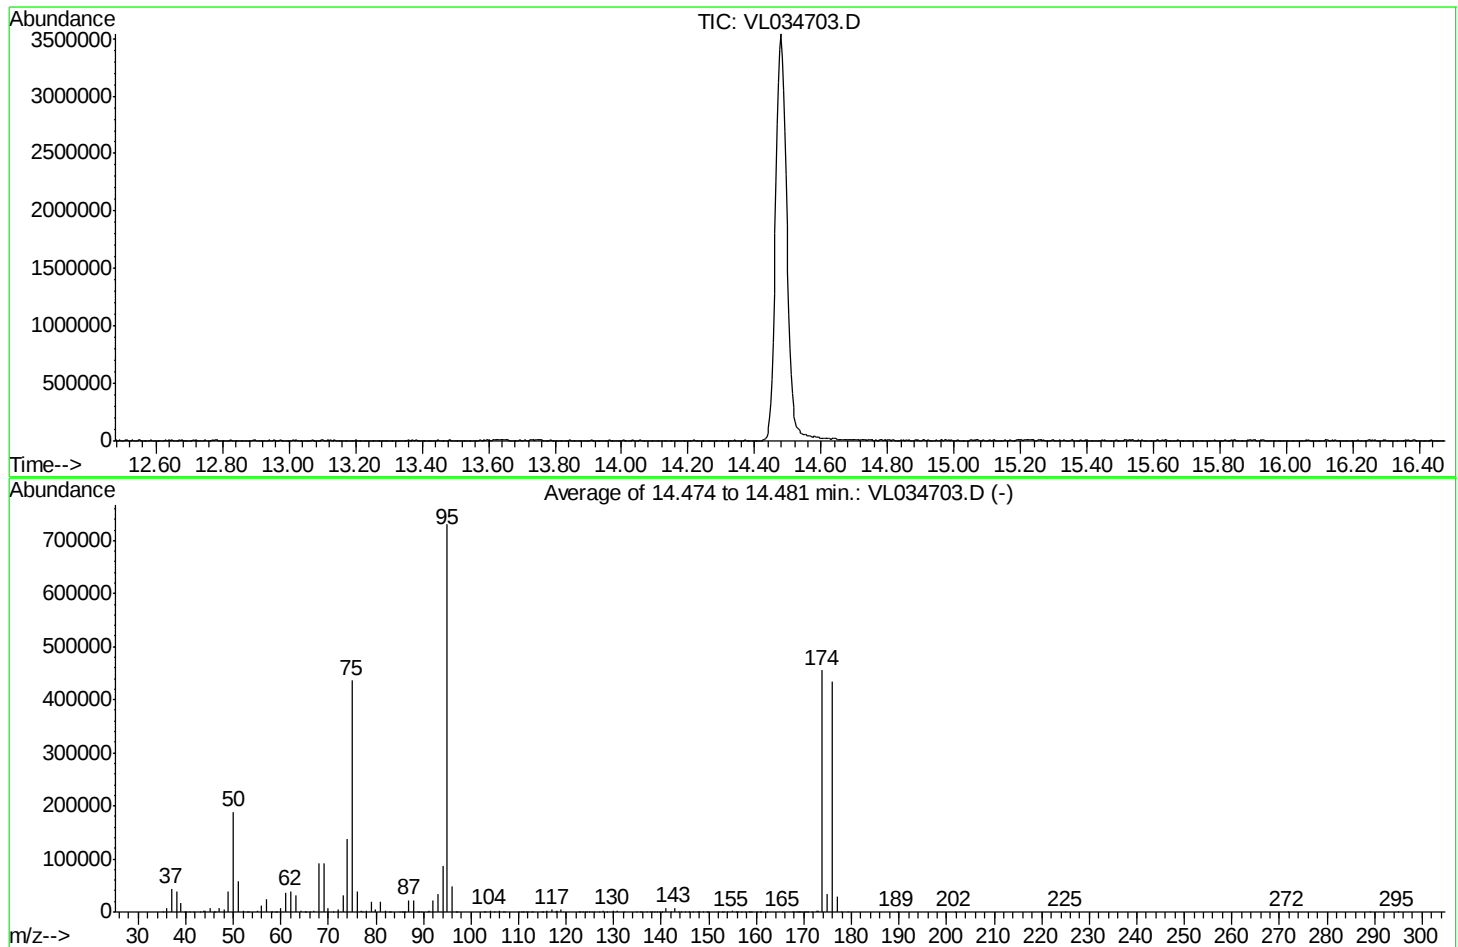

AutoFind: Scans 3635, 3636, 3637; Background Corrected with Scan 3612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.9	189120	PASS
75	95	30	66	59.6	435520	PASS
95	95	100	100	100.0	730538	PASS
96	95	5	9	6.6	48445	PASS
173	174	0.00	2	0.6	2807	PASS
174	95	50	120	62.3	455466	PASS
175	174	4	9	7.2	32973	PASS
176	174	93	101	95.4	434304	PASS
177	176	5	9	6.8	29413	PASS