
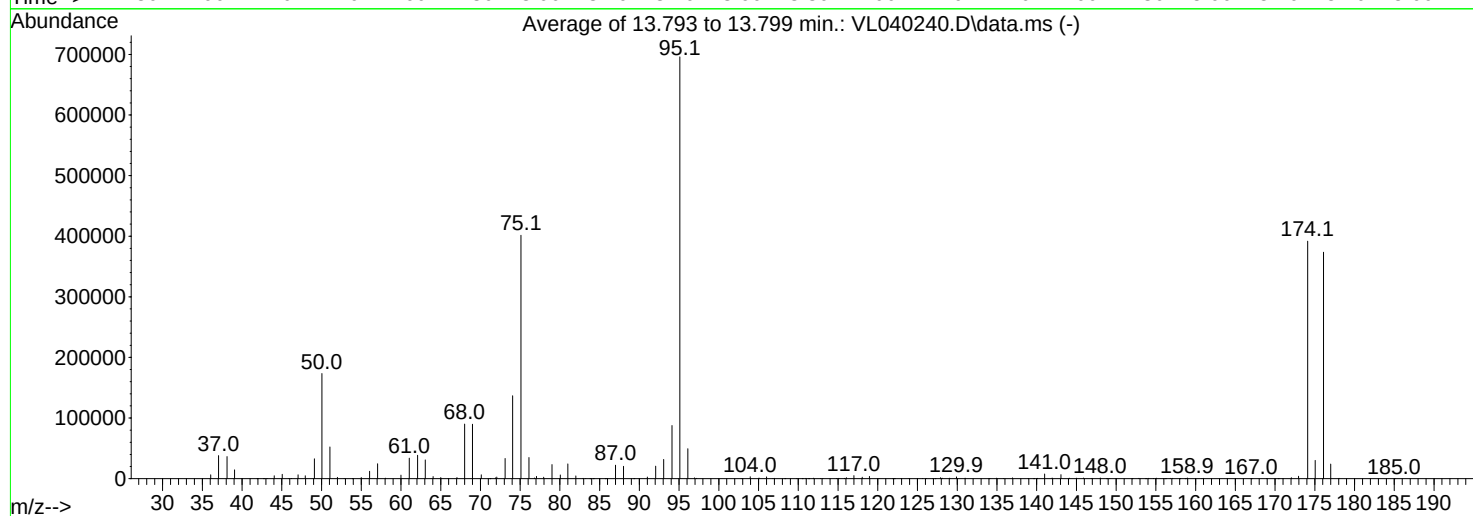


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022823\
 Data File : VL040240.D
 Acq On : 28 Feb 2023 8:21
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL021523AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Wed Mar 01 04:21:39 2023

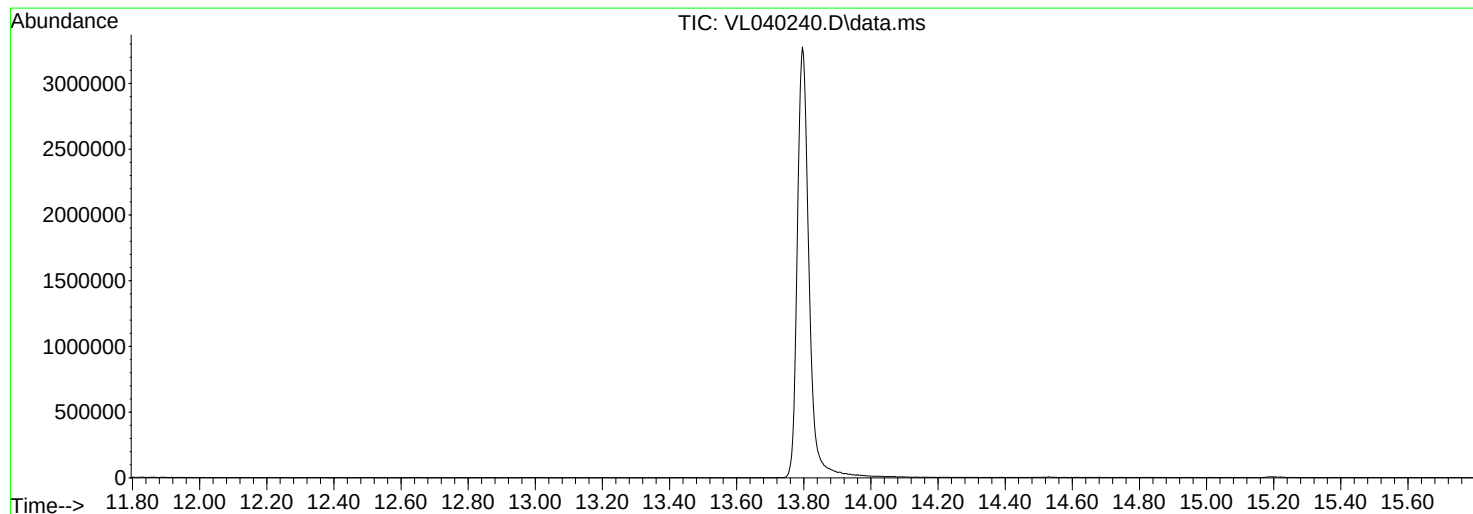

AutoFind: Scans 3480, 3481, 3482; Background Corrected with Scan 3456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.9	173504	PASS
75	95	30	66	57.7	401493	PASS
95	95	100	100	100.0	695979	PASS
96	95	5	9	7.1	49355	PASS
173	174	0.00	2	1.0	3867	PASS
174	95	50	120	56.3	391744	PASS
175	174	4	9	7.7	30107	PASS
176	174	93	101	95.4	373696	PASS
177	176	5	9	6.4	23979	PASS

Average of 13.793 to 13.799 min.: VL040240.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	6274	46.20	347	57.05	24619	69.00	8982
37.05	38067	47.05	6443	58.05	782	70.10	649
38.10	36347	47.95	4729	60.00	5821	71.20	6
39.05	14659	49.10	32736	61.05	33773	71.90	140
40.00	248	50.05	173504	62.10	38565	72.05	2642
41.90	59	51.05	52179	63.05	30832	73.10	33360
42.70	51	52.00	2220	64.05	3503	74.05	136845
43.15	310	52.85	218	65.00	1946	75.10	401493
44.05	4811	53.90	86	65.95	232	76.10	34979
45.05	7039	55.00	1847	67.05	1934	76.80	1089
45.90	369	56.05	12091	68.00	89955	77.05	3769

Average of 13.793 to 13.799 min.: VL040240.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.95	2507	87.00	22309	102.80	203	111.30	93
79.00	23320	88.00	20387	103.00	254	111.90	674
80.05	5960	89.30	63	103.95	3178	112.80	326
81.00	24232	91.00	2569	105.05	1069	113.10	313
82.00	4597	92.05	20659	106.00	2959	114.80	209
82.90	668	93.05	31613	106.80	296	115.10	652
83.25	410	94.10	87680	107.00	561	115.80	609
83.80	66	95.10	695979	108.30	53	116.05	1618
84.20	111	96.10	49355	109.80	405	117.00	5055
85.70	117	96.95	1433	110.50	87	118.05	2437
85.95	246	97.20	542	110.95	658	118.95	3611

Average of 13.793 to 13.799 min.: VL040240.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
120.15	187	129.05	877	141.95	1118	152.85	435
121.90	123	129.90	2820	143.05	6631	153.70	116
122.10	66	131.00	809	144.10	681	154.10	422
122.95	267	134.00	77	145.00	861	154.70	318
123.95	383	134.95	951	145.90	1108	155.05	796
125.65	184	135.80	167	146.95	576	156.00	295
126.10	218	136.95	1230	148.00	1143	156.20	155
126.95	193	138.95	287	148.80	78	156.80	485
127.20	88	139.60	116	149.20	261	157.10	534
127.90	1704	140.10	659	150.00	314	158.00	114
128.10	797	141.00	7607	152.00	117	158.70	91

Average of 13.793 to 13.799 min.: VL040240.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
158.95	981	176.10	373696				
160.80	258	177.00	23979				
161.00	530	178.05	516				
167.00	53	185.00	77				
168.95	175						
170.40	85						
171.00	342						
172.05	1596						
172.95	3867						
174.10	391744						
175.05	30107						

Instrument :

MSVOA_L

ClientSampleId :

BFB