


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_L\DATA\VL030121\
 Data File : VL036407.D
 Acq On : 1 Mar 2021 8:45
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL021021AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Feb 10 16:04:02 2021
 Last Update : Wed Feb 10 16:04:02 2021

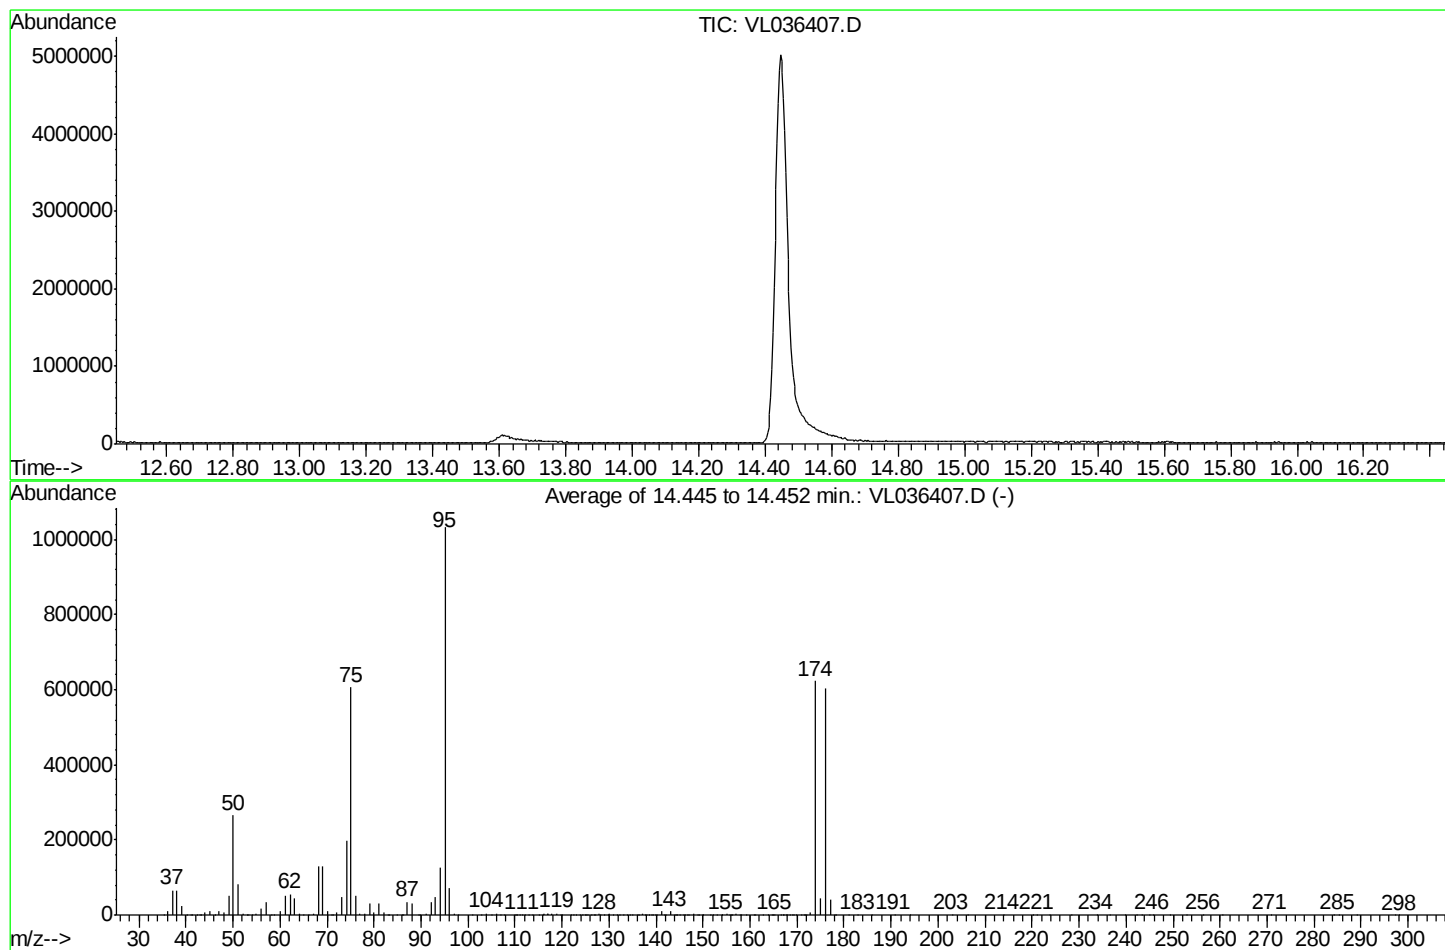

AutoFind: Scans 3626, 3627, 3628; Background Corrected with Scan 3600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.8	265962	PASS
75	95	30	66	58.7	606592	PASS
95	95	100	100	100.0	1032768	PASS
96	95	5	9	7.1	73264	PASS
173	174	0.00	2	0.9	5362	PASS
174	95	50	120	60.3	623274	PASS
175	174	4	9	7.1	44552	PASS
176	174	93	101	96.9	603968	PASS
177	176	5	9	6.6	40128	PASS