


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL030222\
 Data File : VL038474.D
 Acq On : 2 Mar 2022 9:03
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL022222AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
 Last Update : Tue Feb 22 19:45:51 2022

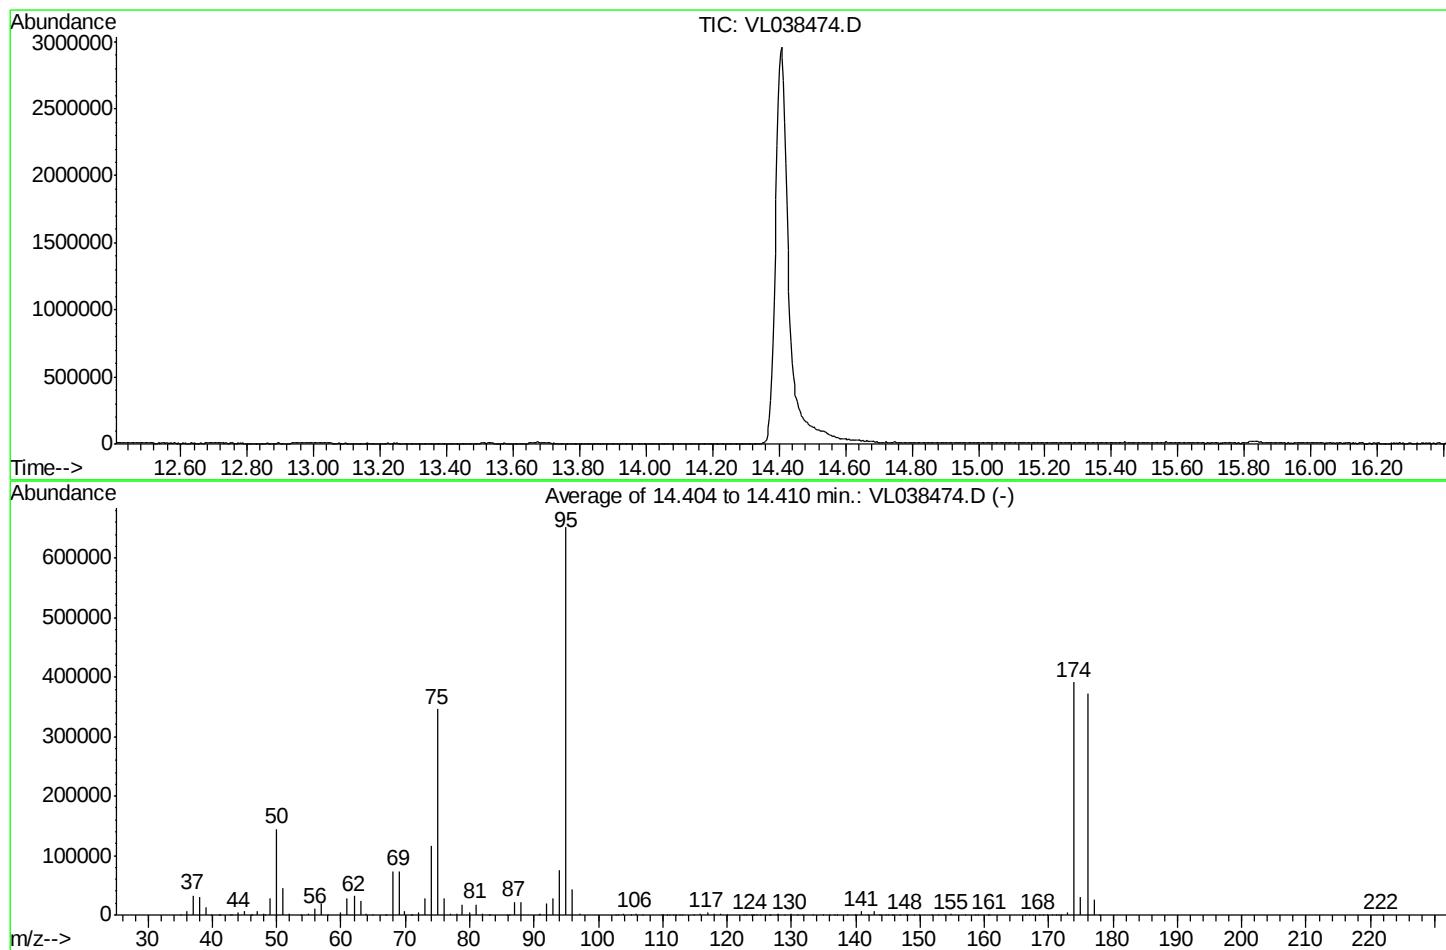

AutoFind: Scans 3613, 3614, 3615; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.3	145344	PASS
75	95	30	66	53.1	346496	PASS
95	95	100	100	100.0	651989	PASS
96	95	5	9	6.6	42941	PASS
173	174	0.00	2	1.1	4225	PASS
174	95	50	120	60.1	391680	PASS
175	174	4	9	7.6	29840	PASS
176	174	93	101	95.4	373568	PASS
177	176	5	9	7.0	25965	PASS