

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL030320\
 Data File : VL034764.D
 Acq On : 3 Mar 2020 15:10
 Operator : SY/AP
 Sample : L1704-03DUP
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :

Quant Time: Mar 04 05:46:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL022620AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Feb 28 01:15:02 2020
 QLast Update : Fri Feb 28 01:15:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.69	49	894315	10.00	ppbv	0.02
33) 1,4-Difluorobenzene	7.21	114	1860443	10.00	ppbv	0.02
55) Chlorobenzene-d5	12.14	117	1768812	10.00	ppbv	0.03

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.48	95	1532543	10.57	ppbv	0.03
Spiked Amount	10.000	Range	65 - 135	Recovery	=	105.70%


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	3.02	85	42498	0.301	ppbv #	85
3) Chlorodifluoromethane	2.93	51	220019	2.280	ppbv #	67
4) Chloromethane	3.11	50	46066	0.853	ppbv	99
7) Chloroethane	3.54	64	562	0.029	ppbv #	1
9) Propene	3.18	41	289710	7.181	ppbv	98
11) Trichlorofluoromethane	3.94	101	18799	0.152	ppbv	98
13) Ethanol	3.59	45	409606	32.139	ppbv	98
15) Acetone	3.83	43	9781398	95.983	ppbv #	69
16) 1,3-Butadiene	3.29	39	45288	0.960	ppbv #	12
17) tert-Butyl alcohol	4.32	59	2045	0.026	ppbv #	1
19) Isopropyl Alcohol	3.97	45	18713	0.308	ppbv #	94
20) Methylene Chloride	4.34	84	69217	1.826	ppbv	94
23) Vinyl Acetate	5.08	43	100864	0.728	ppbv #	93
25) Ethyl Acetate	5.69	43	5738	0.032	ppbv #	62
26) Hexane	5.69	57	5507	0.066	ppbv #	59
30) Cyclohexane	7.16	84	3830	0.059	ppbv #	27
34) 2-Butanone	5.26	43	9749	0.083	ppbv #	72
39) 1,2-Dichloropropane	7.21	63	548549	8.581	ppbv #	24
53) Toluene	9.85	91	5189	0.030	ppbv #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL030320\
Data File : VL034764.D
Acq On : 3 Mar 2020 15:10
Operator : SY/AP
Sample : L1704-03DUP
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :

Quant Time: Mar 04 05:46:40 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL022620AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Feb 28 01:15:02 2020
QLast Update : Fri Feb 28 01:15:02 2020
Response via : Initial Calibration

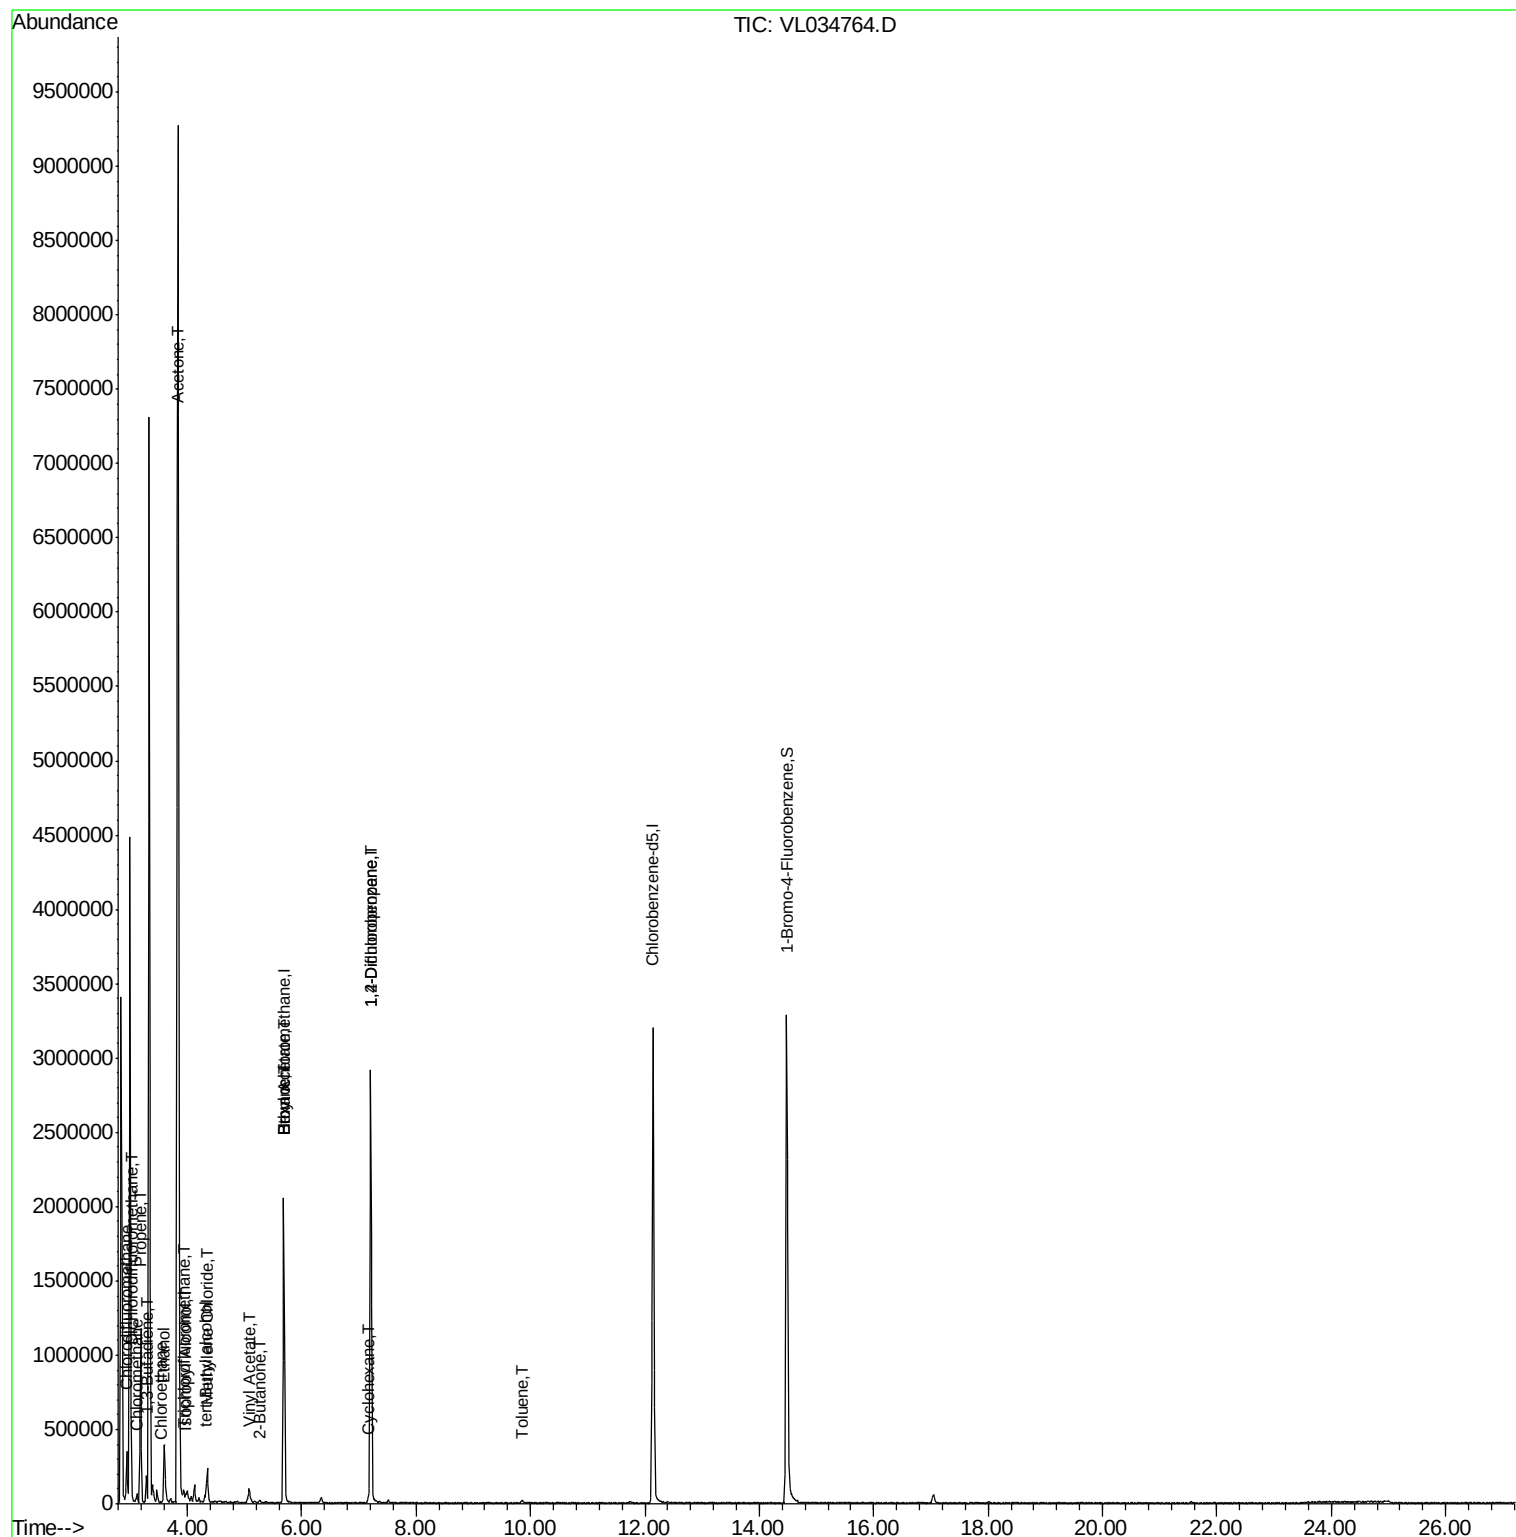

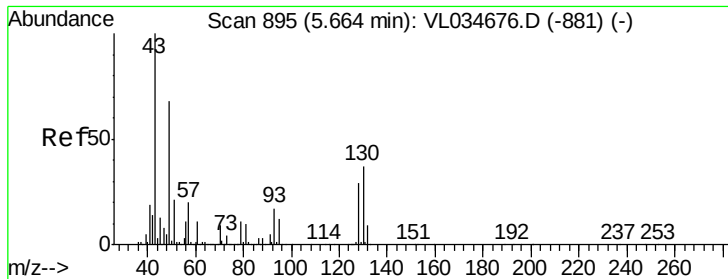

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.69 min Scan# 902

Delta R.T. 0.02 min

Lab File: VL034764.D

Acq: 3 Mar 2020 15:10

Instrument :
MSVOA_L
ClientSampleId :


Tot Ion: 49 Resp: 894315

Ion Ratio Lower Upper

49 100

128 44.3 21.6 65.0

130 57.4 27.7 83.1

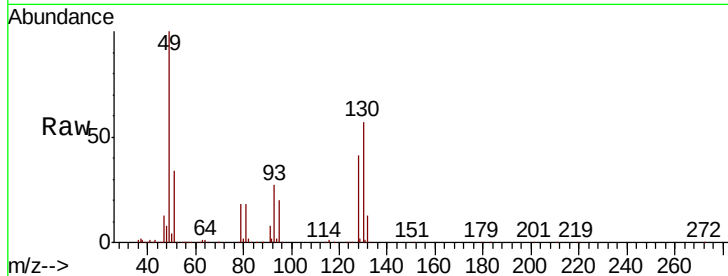

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

5.69



600000

400000

200000

0

Time-->

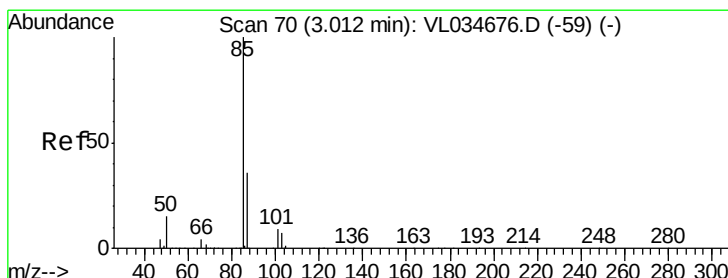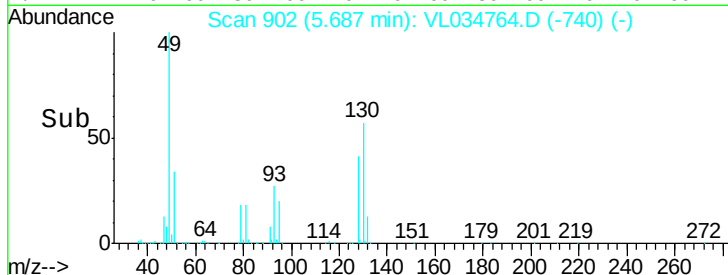

#2

Dichlorodifluoromethane

Concen: 0.301 ppbv

RT: 3.02 min Scan# 74

Delta R.T. 0.01 min

Lab File: VL034764.D


Acq: 3 Mar 2020 15:10

Tgt Ion: 85 Resp: 42498

Ion Ratio Lower Upper

85 100

87 27.5 29.2 43.8#

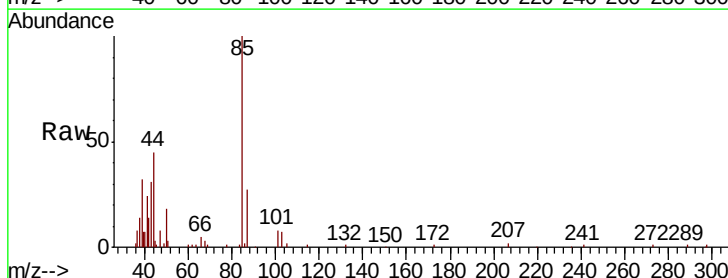

Abundance Ion 85.00 (84.70 to 85.70): VL0

Ion 87.00 (86.70 to 87.70): VL0

3.02


30000


20000

10000

0

Time-->

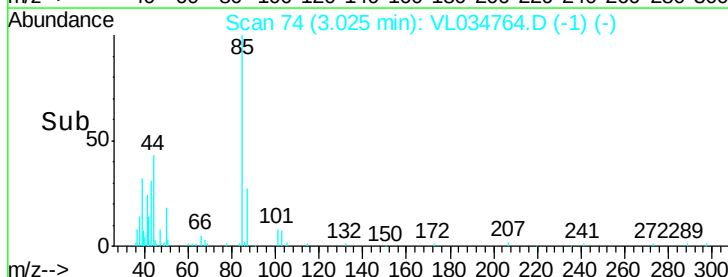

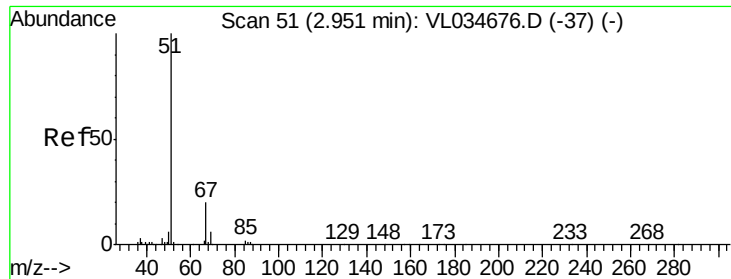

#3

Chlorodifluoromethane

Concen: 2.280 ppbv

RT: 2.93 min Scan# 46

Delta R.T. -0.02 min

Lab File: VL034764.D

Acq: 3 Mar 2020 15:10

Instrument :

MSVOA_L


ClientSampleId :

Tot Ion: 51 Resp: 220019

Ion Ratio Lower Upper




51 100

67 4.2 15.5 23.3#

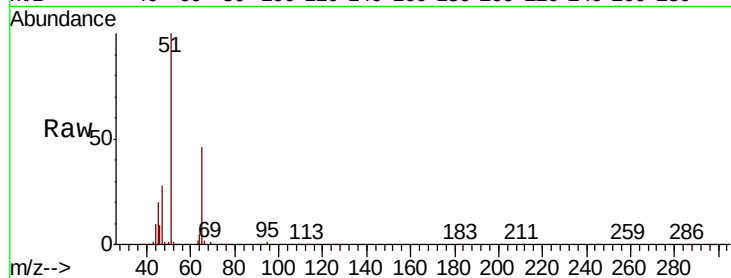

Abundance Ion 51.00 (50.70 to 51.70): VL0

Ion 67.00 (66.70 to 67.70): VL0

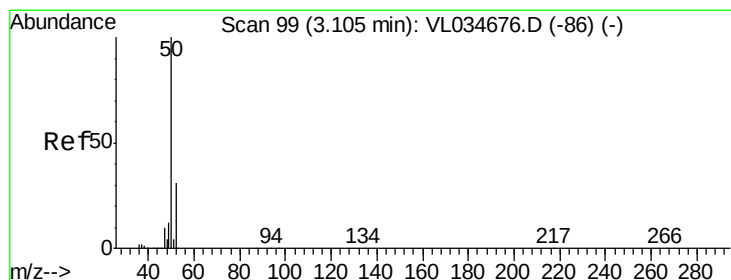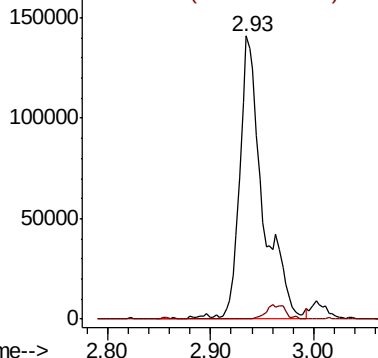

#4

Chloromethane

Concen: 0.853 ppbv

RT: 3.11 min Scan# 102

Delta R.T. 0.01 min

Lab File: VL034764.D


Acq: 3 Mar 2020 15:10

Tgt Ion: 50 Resp: 46066

Ion Ratio Lower Upper



50 100


52 31.7 25.0 37.4

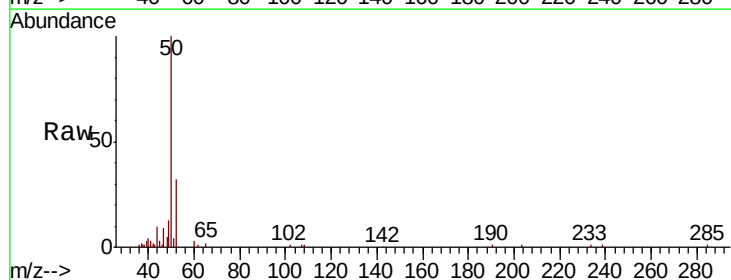

Abundance Ion 50.10 (49.80 to 50.80): VL0

Ion 52.10 (51.80 to 52.80): VL0

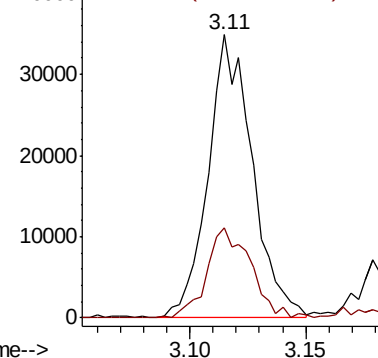



#7

Chloroethane

Concen: 0.029 ppbv

RT: 3.54 min Scan# 234

Delta R.T. 0.01 min

Lab File: VL034764.D

Acq: 3 Mar 2020 15:10

Instrument :

MSVOA_L


ClientSampleId :

Tot Ion: 64 Resp: 562

Ion Ratio Lower Upper




64 100

66 93.7 26.7 40.1#

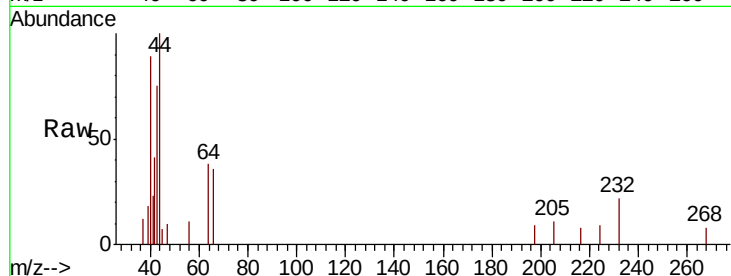

Abundance Ion 64.10 (63.80 to 64.80): VL0

Ion 66.10 (65.80 to 66.80): VL0

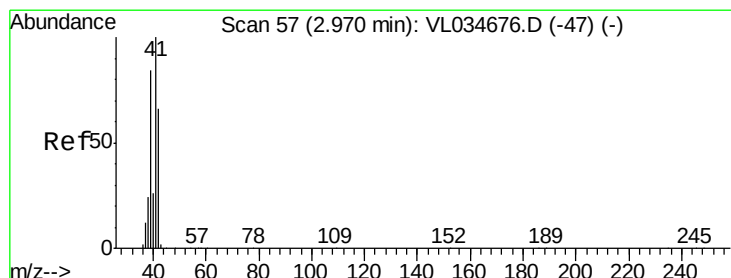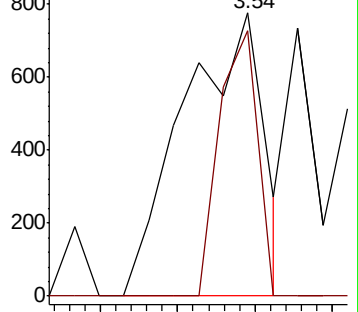

#9

Propene

Concen: 7.181 ppbv

RT: 3.18 min Scan# 123

Delta R.T. 0.21 min

Lab File: VL034764.D


Acq: 3 Mar 2020 15:10

Tgt Ion: 41 Resp: 289710

Ion Ratio Lower Upper



41 100


42 70.4 54.9 82.3

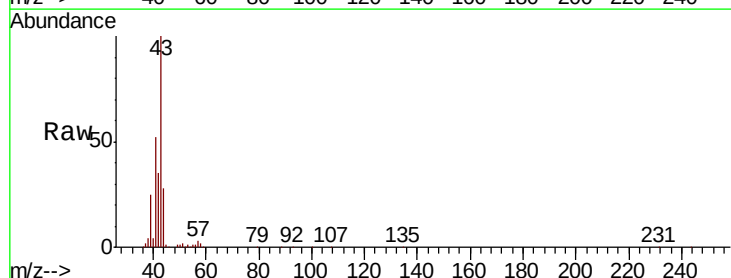

Abundance Ion 41.10 (40.80 to 41.80): VL0

Ion 42.10 (41.80 to 42.80): VL0




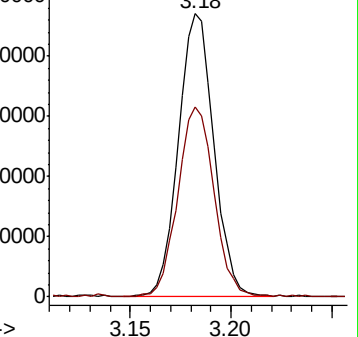


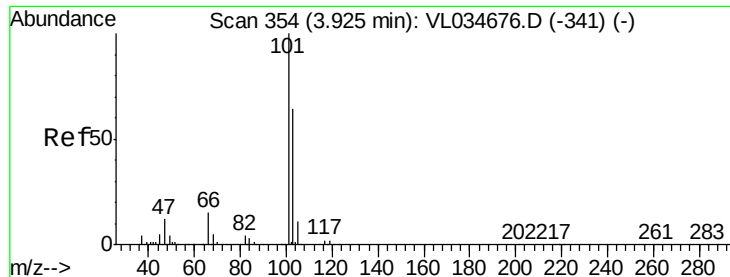

#11
 Trichlorofluoromethane
 Concen: 0.152 ppbv
 RT: 3.94 min Scan# 359
 Delta R.T. 0.02 min
 Lab File: VL034764.D
 Acq: 3 Mar 2020 15:10




Instrument :
 MSVOA_L
 ClientSampleId :


Tot Ion:101 Resp: 18799
 Ion Ratio Lower Upper
 101 100
 103 65.3 51.2 76.8

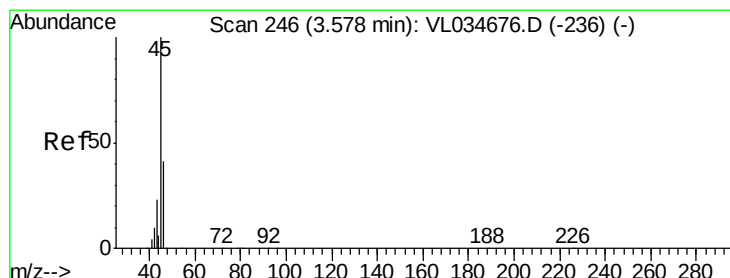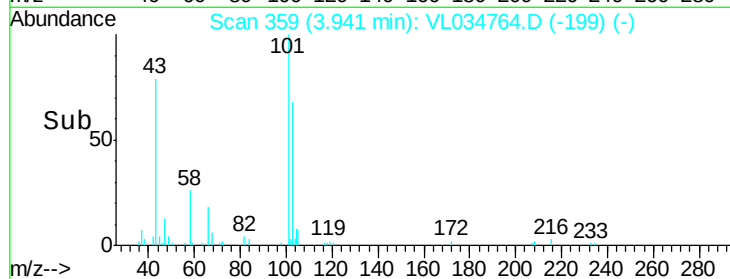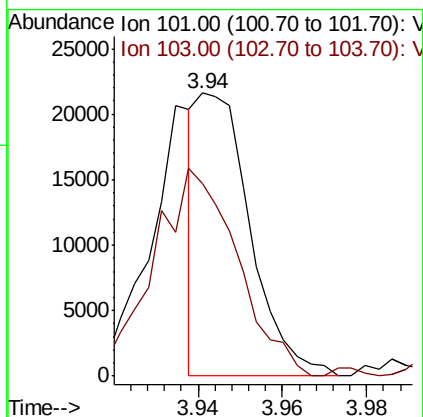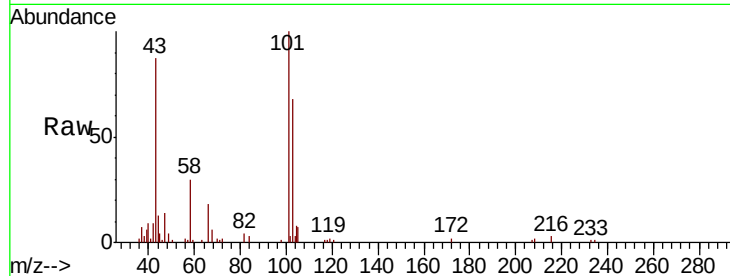

#13
 Ethanol
 Concen: 32.139 ppbv
 RT: 3.59 min Scan# 251
 Delta R.T. 0.02 min
 Lab File: VL034764.D
 Acq: 3 Mar 2020 15:10

Tgt Ion: 45 Resp: 409606
 Ion Ratio Lower Upper
 45 100
 46 37.4 15.4 61.4

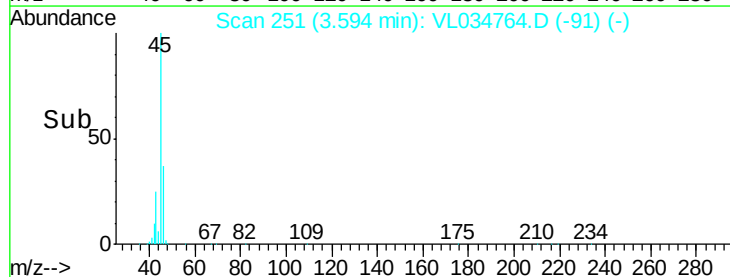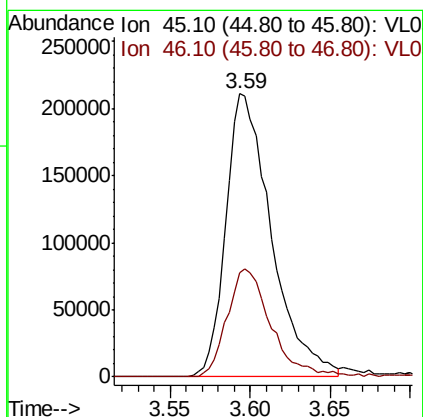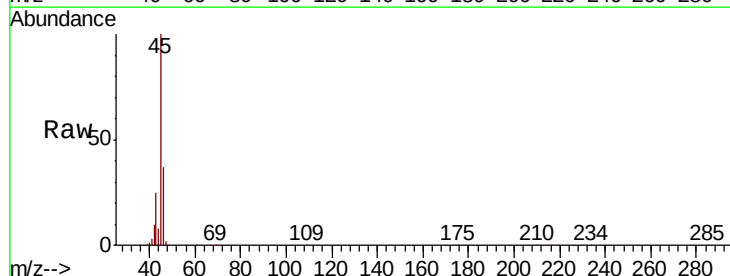



#15

Acetone

Concen: 95.983 ppbv

RT: 3.83 min Scan# 326

Delta R.T. 0.01 min

Lab File: VL034764.D

Acq: 3 Mar 2020 15:10

Instrument :

MSVOA_L





ClientSampleId :

Tot Ion: 43 Resp: 9781398

Ion Ratio Lower Upper

43 100

58 42.5 21.4 32.0#

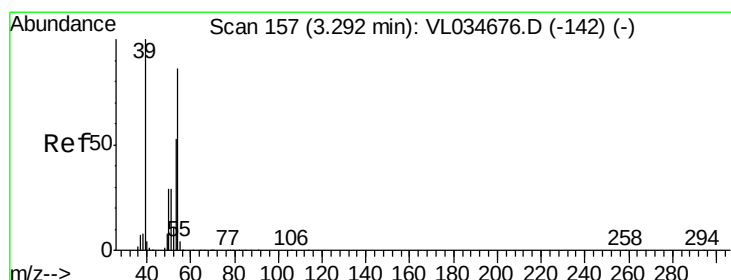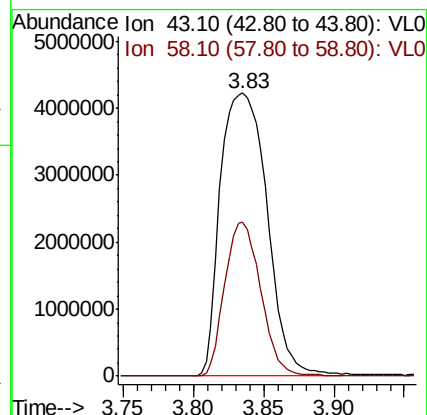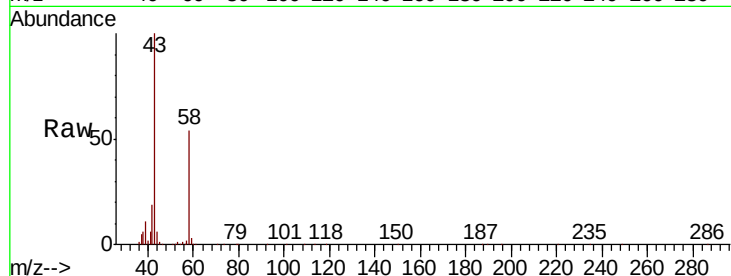

#16

1,3-Butadiene

Concen: 0.960 ppbv

RT: 3.29 min Scan# 156

Delta R.T. -0.00 min

Lab File: VL034764.D




Acq: 3 Mar 2020 15:10


Tgt Ion: 39 Resp: 45288

Ion Ratio Lower Upper

39 100

54 4.5 67.0 100.6#

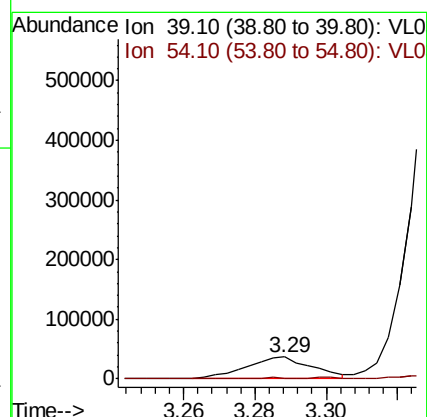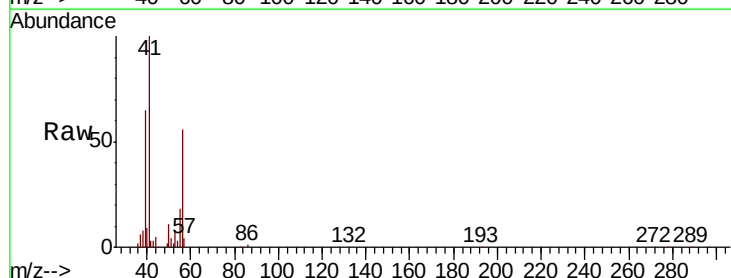

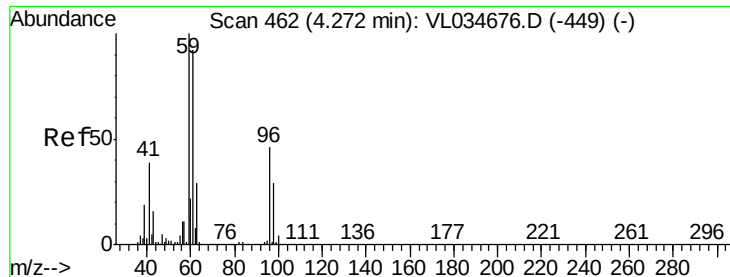

#17

tert-Butyl alcohol

Concen: 0.026 ppbv

RT: 4.32 min Scan# 477

Delta R.T. 0.05 min

Lab File: VL034764.D

Acq: 3 Mar 2020 15:10

Instrument :

MSVOA_L





ClientSampleId :

Tot Ion: 59 Resp: 2045

Ion Ratio Lower Upper

59 100

57 434.1 8.8 13.2#

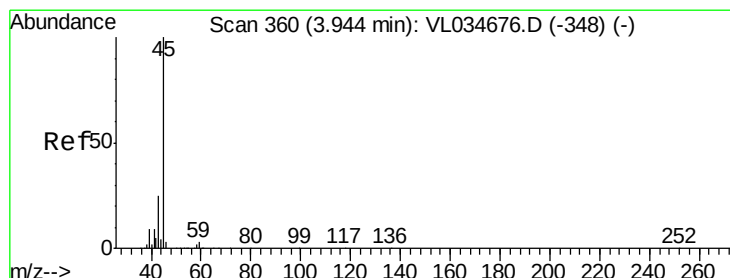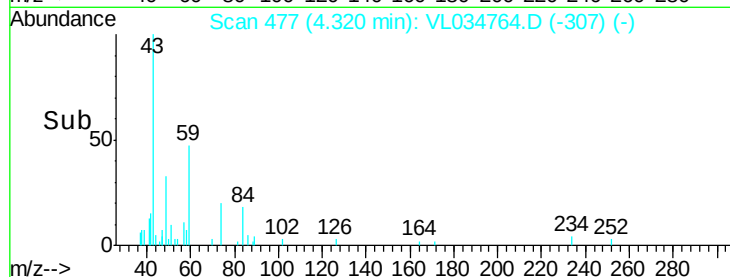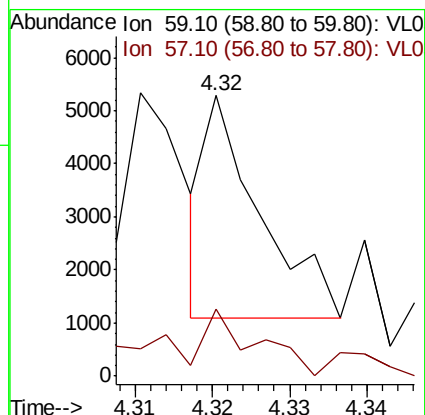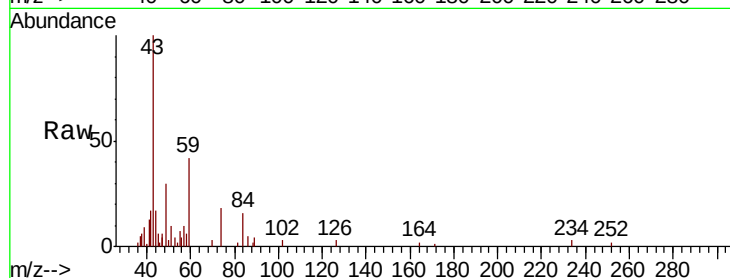

#19

Isopropyl Alcohol

Concen: 0.308 ppbv

RT: 3.97 min Scan# 369

Delta R.T. 0.03 min

Lab File: VL034764.D




Acq: 3 Mar 2020 15:10


Tgt Ion: 45 Resp: 18713

Ion Ratio Lower Upper

45 100

58 0.0 1.8 2.6#


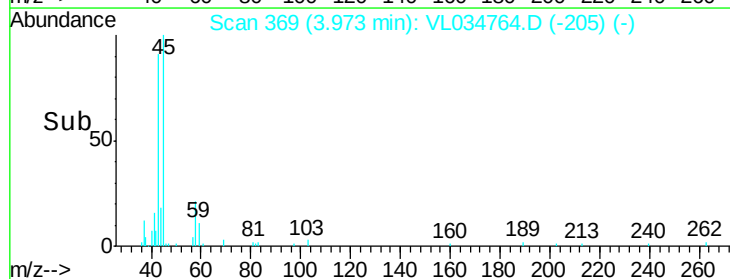
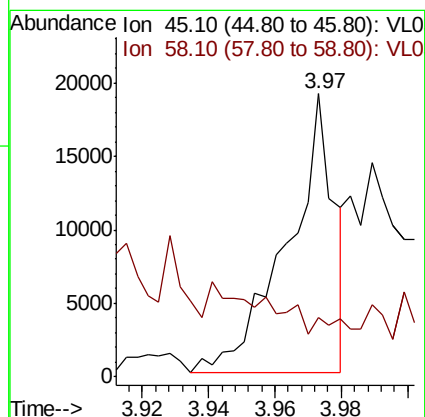
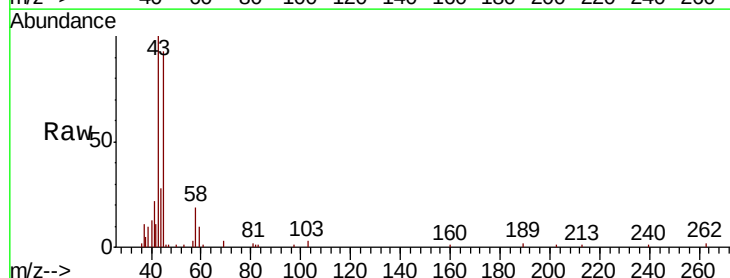




#20
Methylene Chloride
Concen: 1.826 ppbv
RT: 4.34 min Scan# 484
Delta R.T. 0.02 min
Lab File: VL034764.D
Acq: 3 Mar 2020 15:10




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion: 84 Resp: 69217
Ion Ratio Lower Upper
84 100
49 159.7 122.8 184.2
51 48.9 38.6 58.0
86 68.1 47.7 71.5

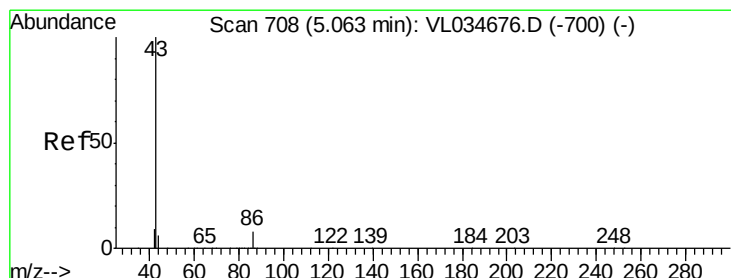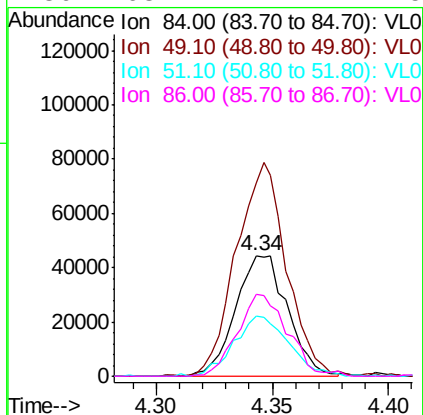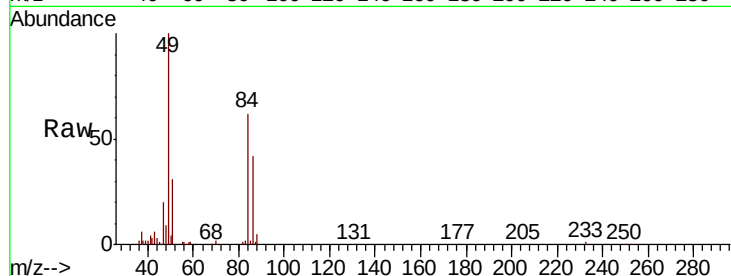

#23
Vinyl Acetate
Concen: 0.728 ppbv
RT: 5.08 min Scan# 714
Delta R.T. 0.02 min
Lab File: VL034764.D
Acq: 3 Mar 2020 15:10

Tgt Ion: 43 Resp: 100864
Ion Ratio Lower Upper
43 100
86 6.1 6.0 9.0
42 8.5 8.0 12.0
44 10.7 4.5 6.7#



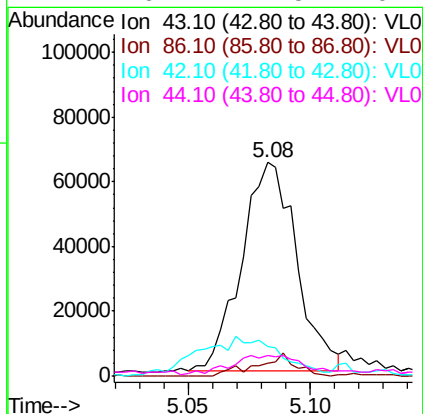
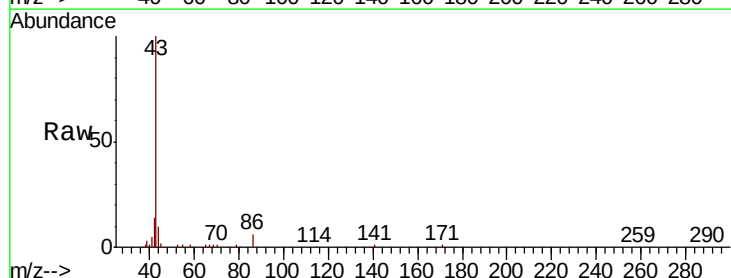




#25
Ethyl Acetate
Concen: 0.032 ppbv
RT: 5.69 min Scan# 903
Delta R.T. 0.02 min
Lab File: VL034764.D
Acq: 3 Mar 2020 15:10




Instrument :
MSVOA_L
ClientSampled :


Tot Ion	43	Resp:	5738
Ion	Ratio	Lower	Upper
43	100		
45	37.0	8.2	12.4#
61	15.5	7.8	11.6#
70	0.0	6.1	9.1#

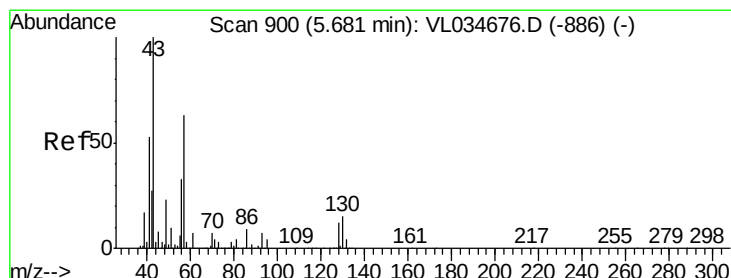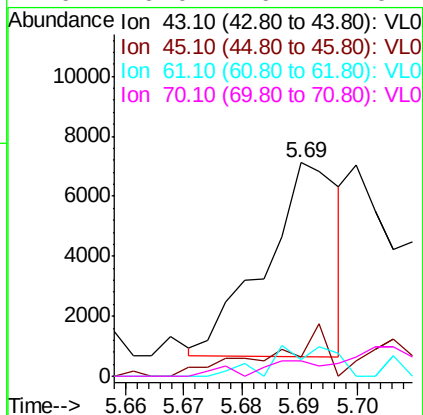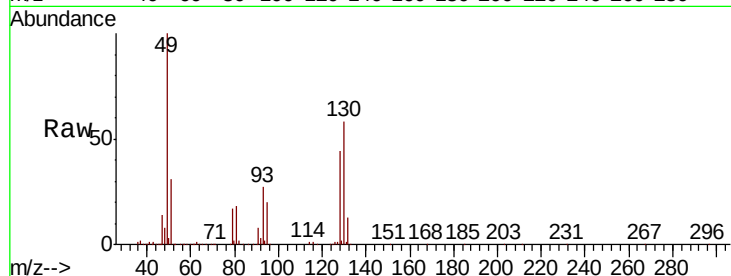

#26
Hexane
Concen: 0.066 ppbv
RT: 5.69 min Scan# 904
Delta R.T. 0.01 min
Lab File: VL034764.D
Acq: 3 Mar 2020 15:10

Tgt Ion	57	Resp:	5507
Ion	Ratio	Lower	Upper
57	100		
41	140.4	70.3	105.5#
43	272.5	177.0	265.4#
56	92.7	42.6	64.0#



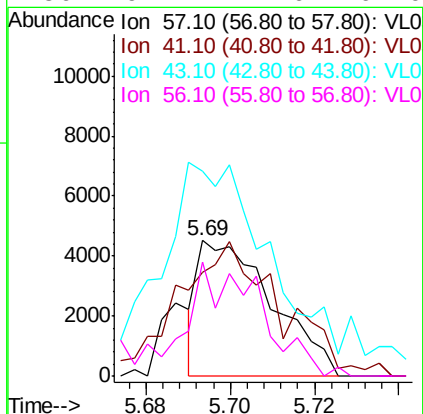
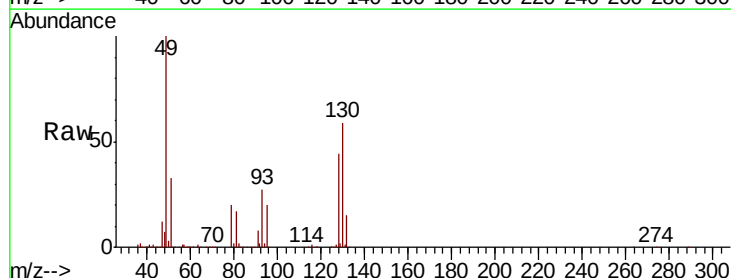


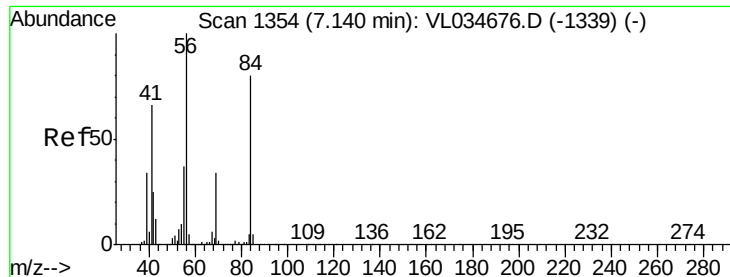

#30
Cyclohexane
Concen: 0.059 ppbv
RT: 7.16 min Scan# 1361
Delta R.T. 0.02 min
Lab File: VL034764.D
Acq: 3 Mar 2020 15:10




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion: 84 Resp: 3830
Ion Ratio Lower Upper
84 100
56 216.2 113.4 170.2#
41 0.0 68.2 102.4#

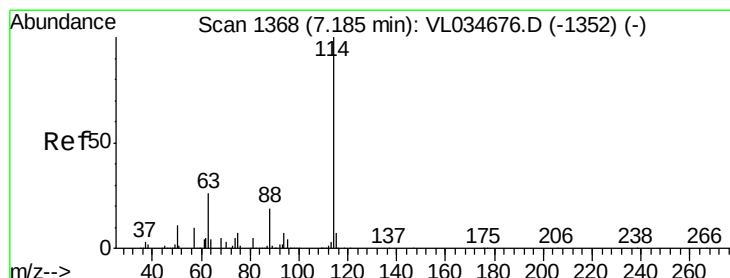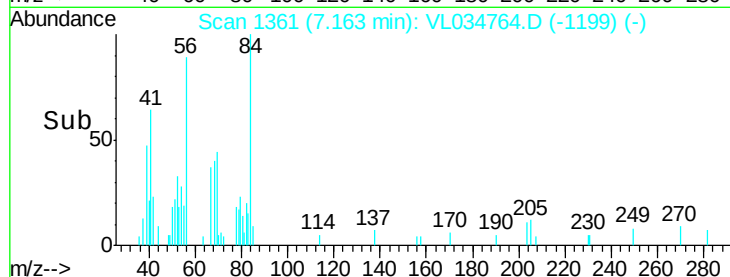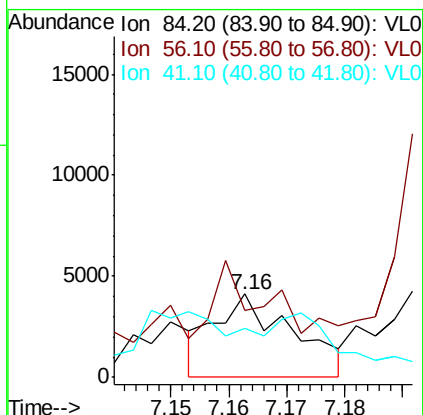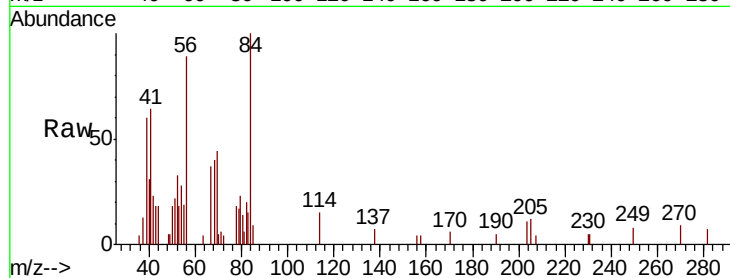

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.21 min Scan# 1375
Delta R.T. 0.02 min
Lab File: VL034764.D
Acq: 3 Mar 2020 15:10

Tgt Ion: 114 Resp: 1860443
Ion Ratio Lower Upper
114 100
63 29.7 22.9 34.3
88 19.7 15.8 23.6


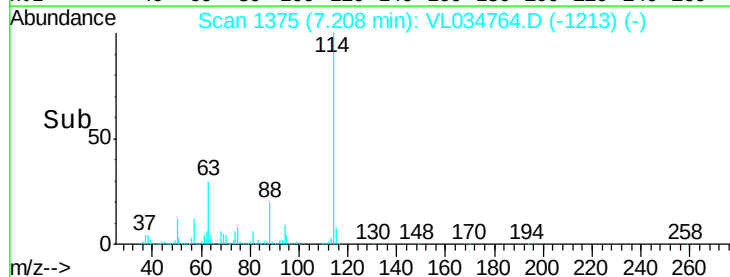
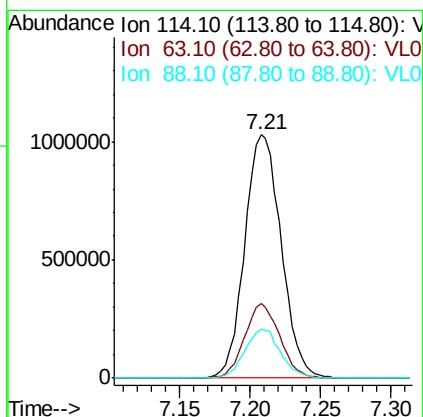
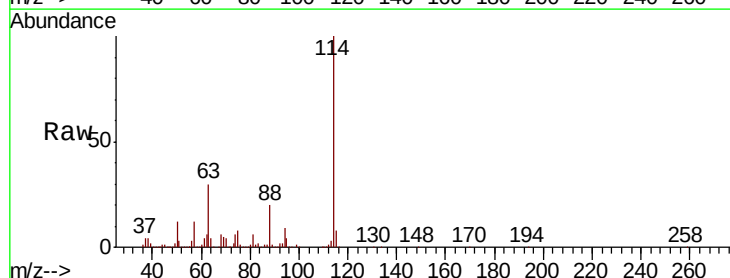


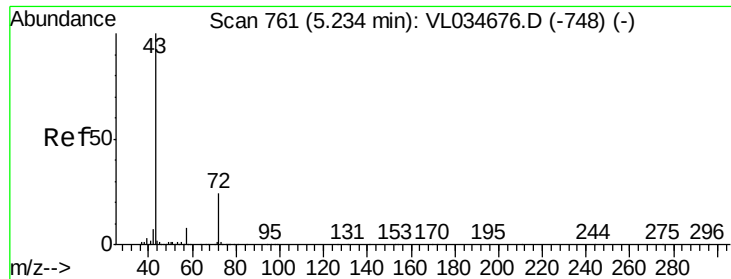

#34
2-Butanone
Concen: 0.083 ppbv
RT: 5.26 min Scan# 769
Delta R.T. 0.03 min
Lab File: VL034764.D
Acq: 3 Mar 2020 15:10




Instrument :
MSVOA_L
ClientSampled :


Tot Ion: 43 Resp: 9749
Ion Ratio Lower Upper
43 100
72 36.4 18.2 27.2#

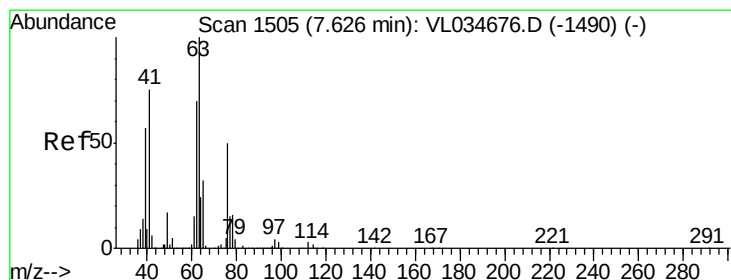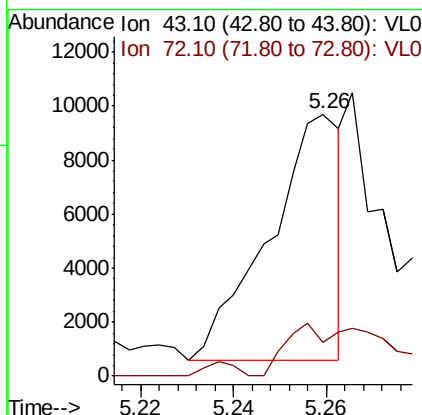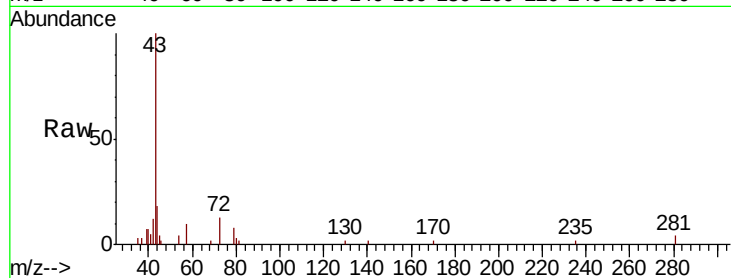

#39
1,2-Dichloropropane
Concen: 8.581 ppbv
RT: 7.21 min Scan# 1375
Delta R.T. -0.42 min
Lab File: VL034764.D
Acq: 3 Mar 2020 15:10

Tgt Ion: 63 Resp: 548549
Ion Ratio Lower Upper
63 100
41 0.0 60.2 90.4#
62 18.3 56.3 84.5#

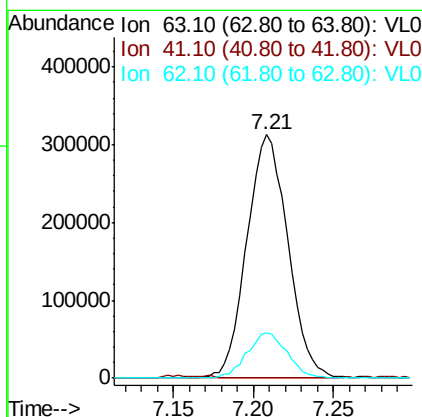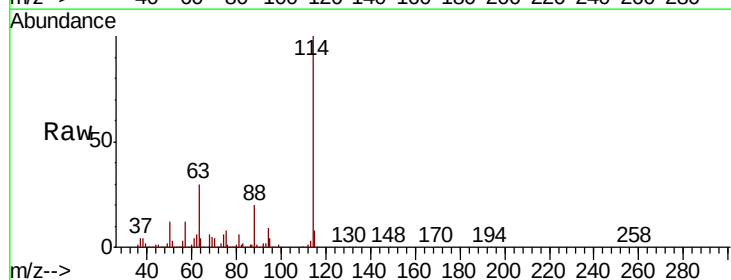

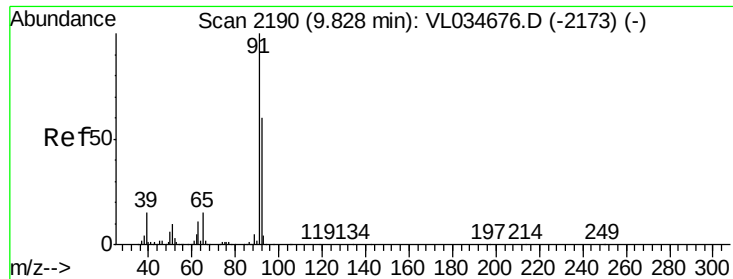

#53

Toluene

Concen: 0.030 ppbv

RT: 9.85 min Scan# 2198

Delta R.T. 0.03 min

Lab File: VL034764.D

Acq: 3 Mar 2020 15:10

Instrument :

MSVOA_L





ClientSampleId :

Tot Ion: 91 Resp: 5189

Ion Ratio Lower Upper

91 100

92 165.0 48.5 72.7#

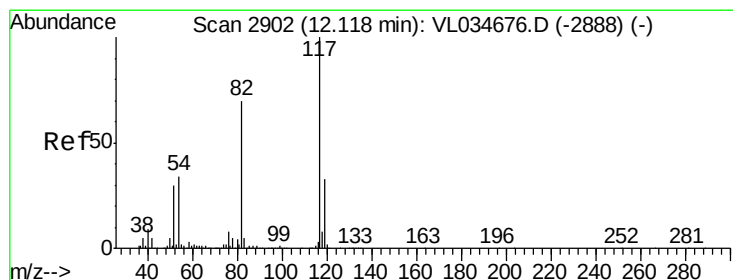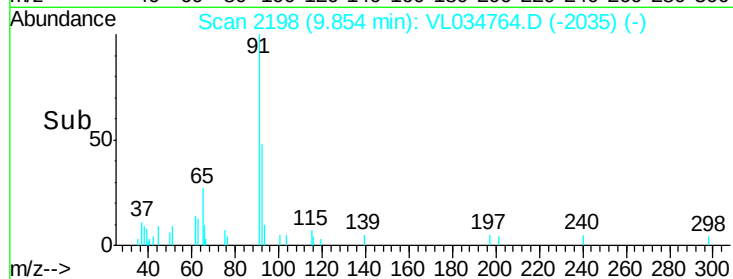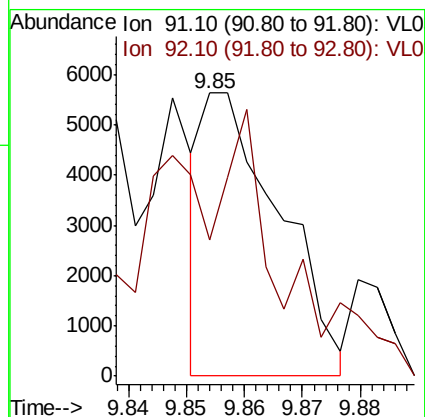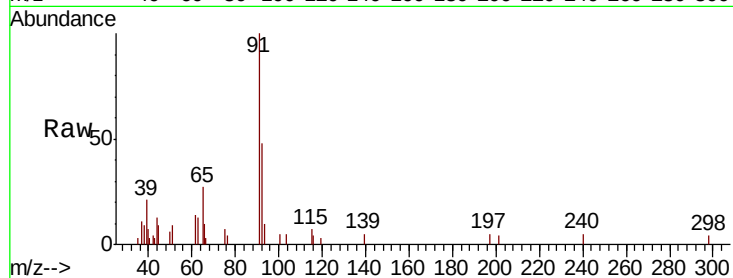

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.14 min Scan# 2910

Delta R.T. 0.03 min

Lab File: VL034764.D

Acq: 3 Mar 2020 15:10




Tgt Ion: 117 Resp: 1768812


Ion Ratio Lower Upper

117 100

82 71.5 54.1 81.1

119 33.2 27.6 41.4

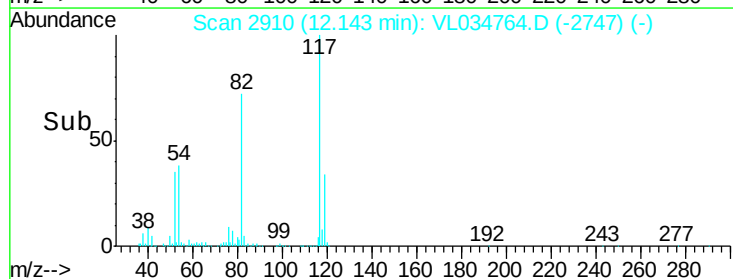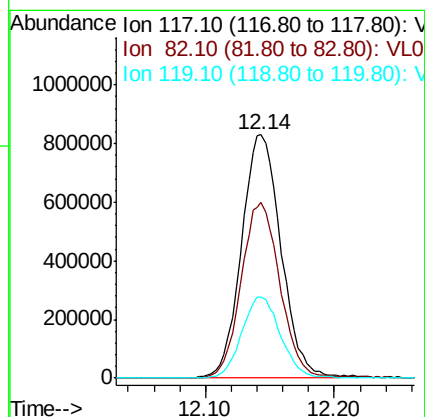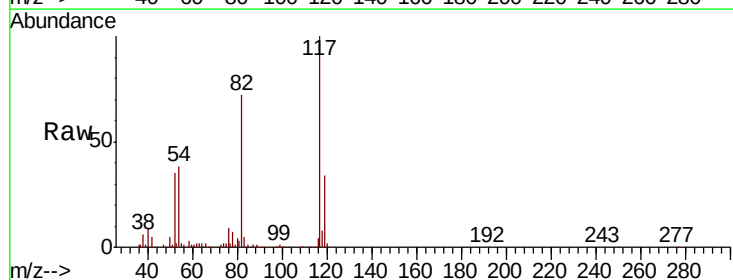

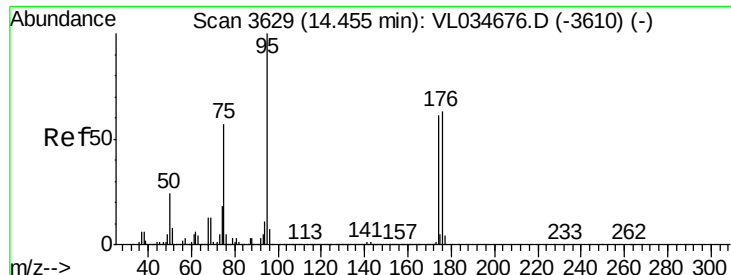

#68

1-Bromo-4-Fluorobenzene

Concen: 10.567 ppbv

RT: 14.48 min Scan# 3638

Delta R.T. 0.03 min

Lab File: VL034764.D

Acq: 3 Mar 2020 15:10

Instrument :

MSVOA_L

ClientSampleId :

Tot Ion: 95 Resp: 1532543

Ion Ratio Lower Upper

95 100

174 65.0 50.7 76.1

175 4.5 3.9 5.9

