


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL030320\
 Data File : VL034757.D
 Acq On : 3 Mar 2020 9:05
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL022620AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Feb 28 01:15:02 2020
 Last Update : Fri Feb 28 01:15:02 2020

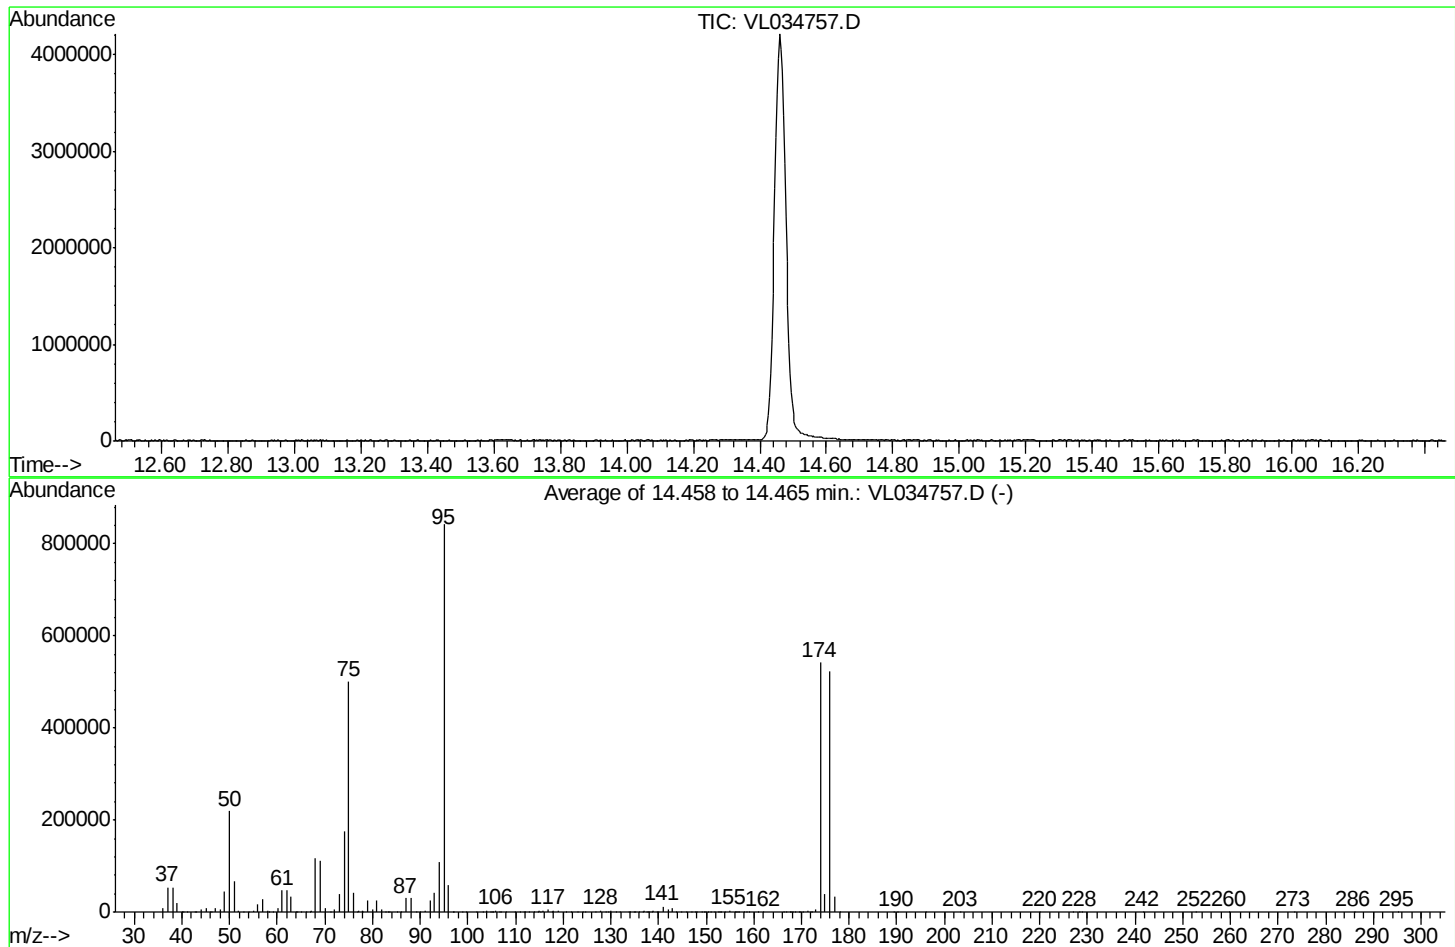

AutoFind: Scans 3630, 3631, 3632; Background Corrected with Scan 3606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.0	219336	PASS
75	95	30	66	59.3	499791	PASS
95	95	100	100	100.0	842517	PASS
96	95	5	9	7.1	59813	PASS
173	174	0.00	2	0.9	5126	PASS
174	95	50	120	64.4	542250	PASS
175	174	4	9	7.2	39312	PASS
176	174	93	101	96.2	521856	PASS
177	176	5	9	6.2	32210	PASS