

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL030325\
 Data File : VL042090.D
 Acq On : 03 Mar 2025 22:02
 Operator : SY/MD
 Sample : QC022625 CAN 10746
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC022625 CAN 10746

Quant Time: Mar 04 00:24:43 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL022525AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Wed Feb 26 01:08:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.787	49	146067	10.000	ppbv	-0.01
33) 1,4-Difluorobenzene	3.959	114	315381	10.000	ppbv	-0.02
55) Chlorobenzene-d5	8.882	117	272704	10.000	ppbv	-0.02

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.374	95	202629	9.658	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	96.600%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL030325\
Data File : VL042090.D
Acq On : 03 Mar 2025 22:02
Operator : SY/MD
Sample : QC022625 CAN 10746
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC022625 CAN 10746

Quant Time: Mar 04 00:24:43 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL022525AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Wed Feb 26 01:08:36 2025
Response via : Initial Calibration




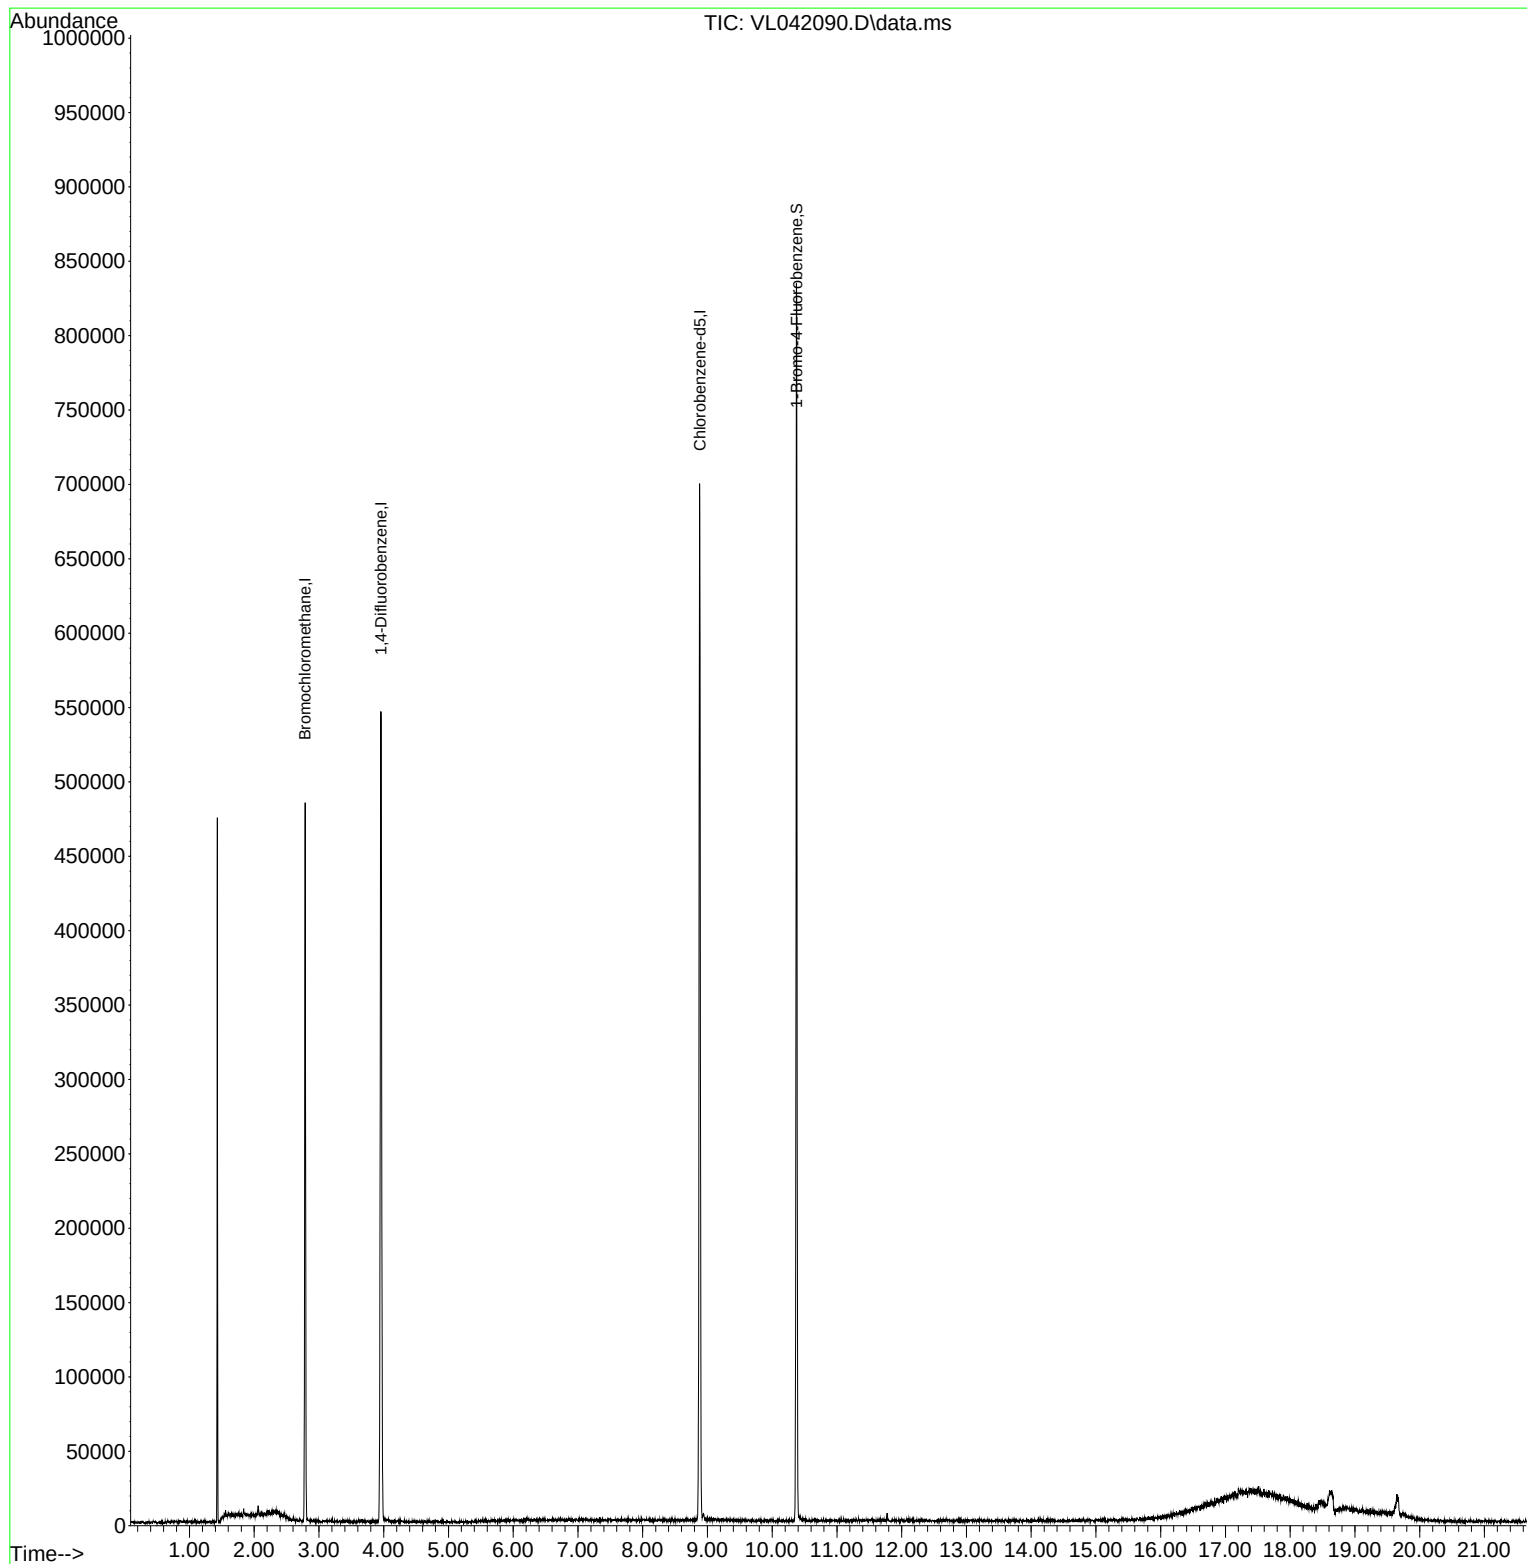


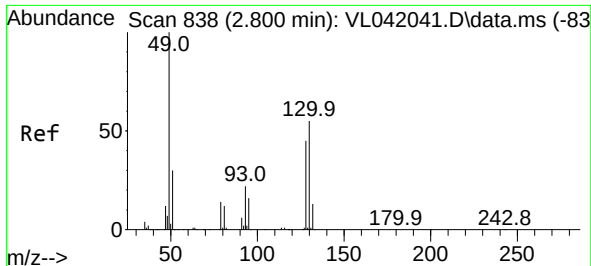

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 2.787 min Scan# 81
Delta R.T. -0.013 min
Lab File: VL042090.D
Acq: 03 Mar 2025 22:02




Instrument :
MSVOA_L
ClientSampleId :
QC022625 CAN 10746


Tgt Ion: 49 Resp: 146067
Ion Ratio Lower Upper
49 100
128 40.4 21.6 64.8
130 50.9 27.8 83.4

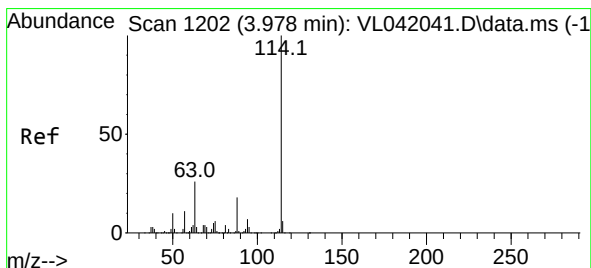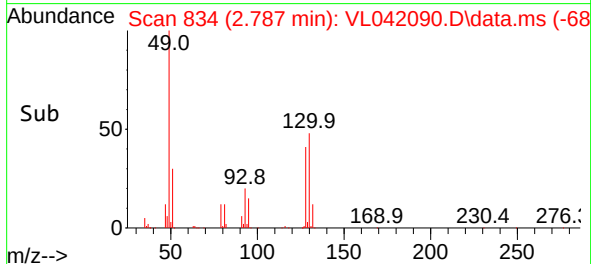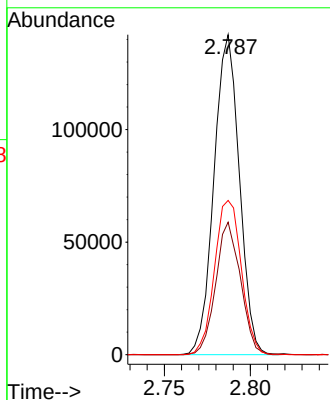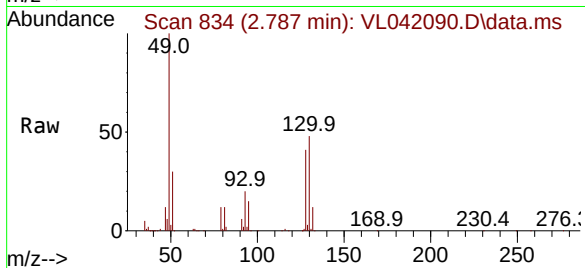

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 3.959 min Scan# 1196
Delta R.T. -0.020 min
Lab File: VL042090.D
Acq: 03 Mar 2025 22:02

Tgt Ion: 114 Resp: 315381
Ion Ratio Lower Upper
114 100
63 26.2 20.1 30.1
88 18.2 14.3 21.5


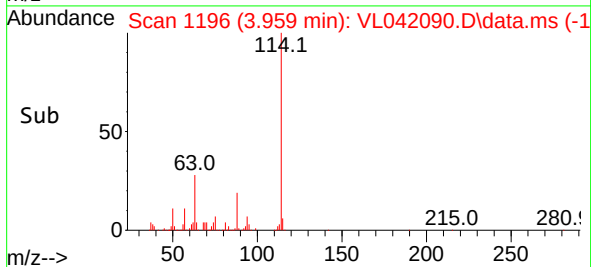
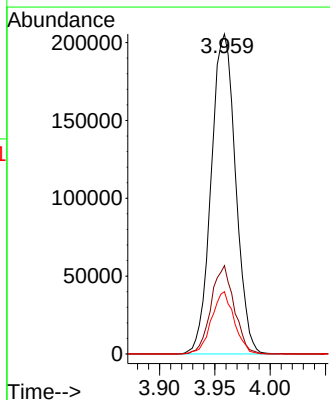
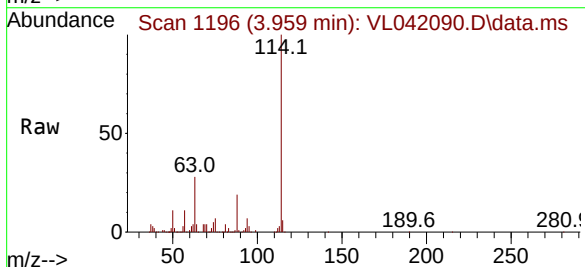


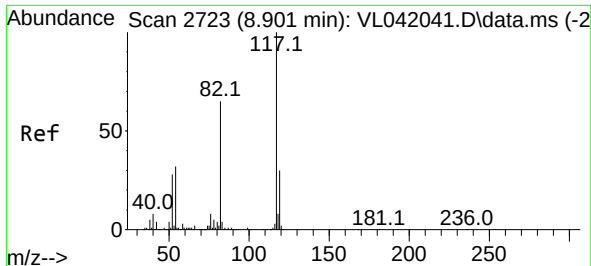

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 8.882 min Scan# 211
Delta R.T. -0.020 min
Lab File: VL042090.D
Acq: 03 Mar 2025 22:02

Instrument :
MSVOA_L
ClientSampleId :
QC022625 CAN 10746

Tgt Ion:117 Resp: 272704
Ion Ratio Lower Upper
117 100
82 66.9 55.0 82.6
119 32.2 25.9 38.9

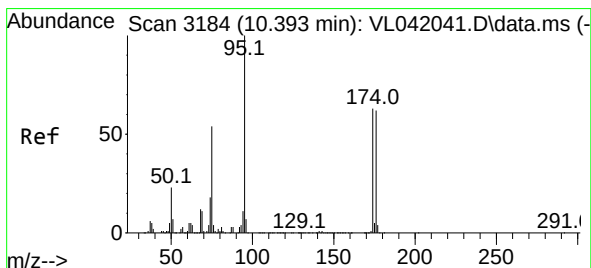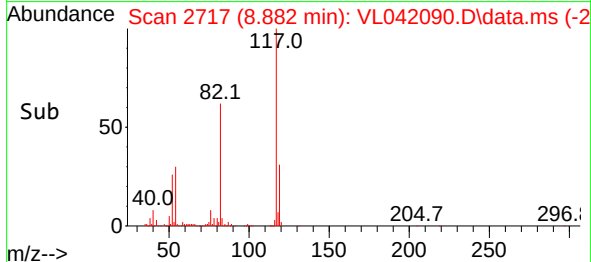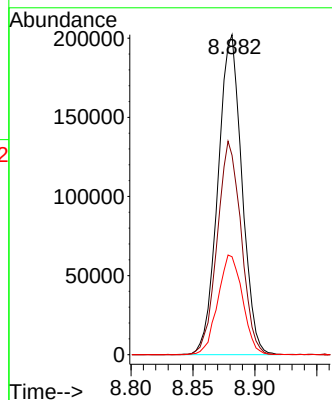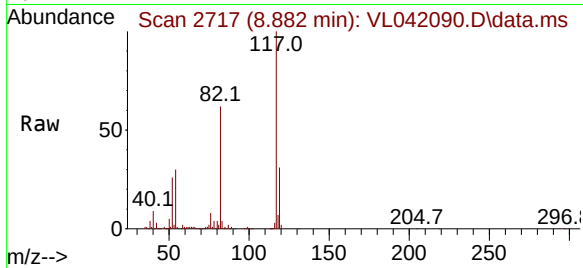

#68
1-Bromo-4-Fluorobenzene
Concen: 9.658 ppbv
RT: 10.374 min Scan# 3178
Delta R.T. -0.020 min
Lab File: VL042090.D
Acq: 03 Mar 2025 22:02

Tgt Ion: 95 Resp: 202629
Ion Ratio Lower Upper
95 100
174 62.7 51.8 77.6
175 4.3 3.9 5.9

