
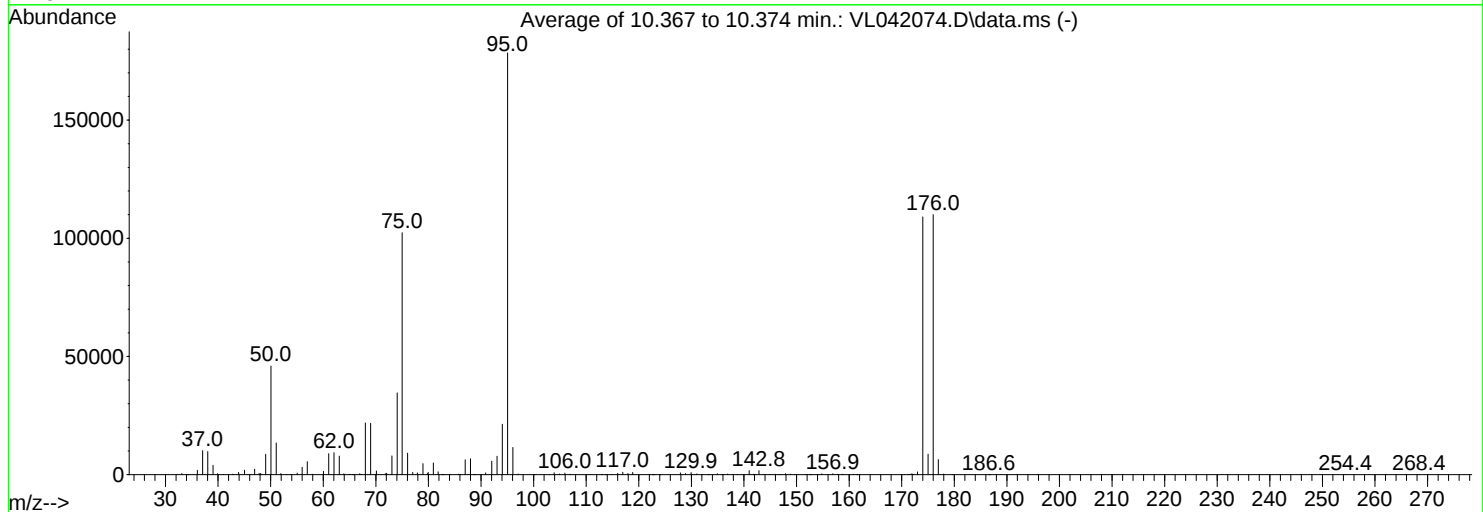


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL030325\
Data File : VL042074.D
Acq On : 03 Mar 2025 11:45
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL022525AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Feb 26 01:08:36 2025

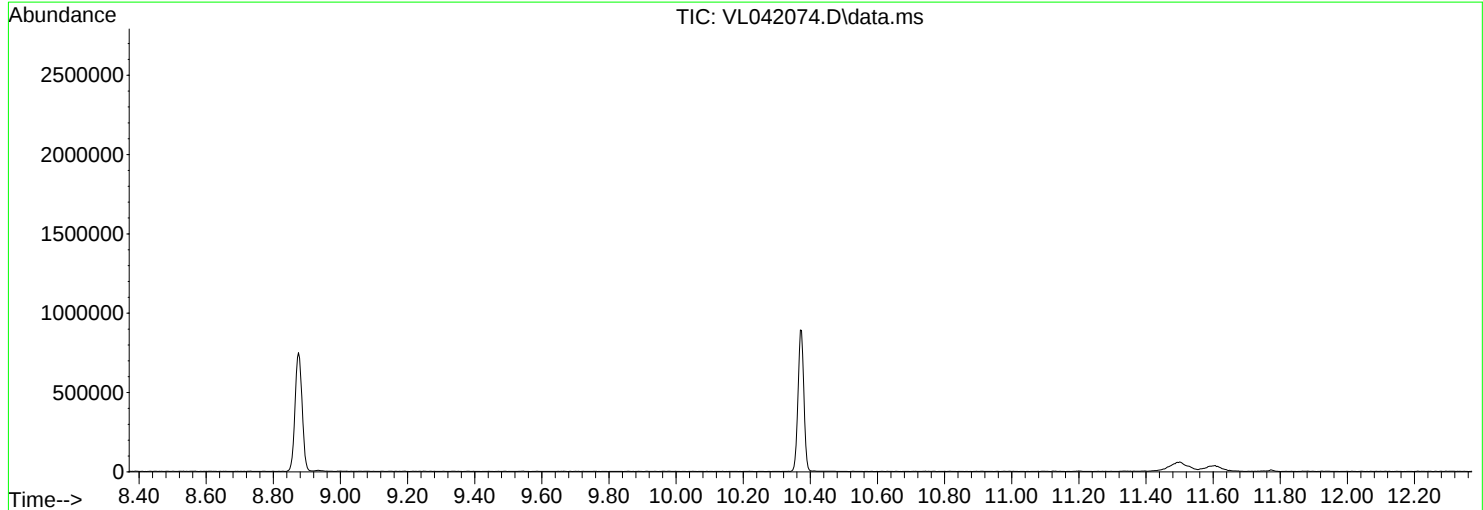

AutoFind: Scans 3176, 3177, 3178; Background Corrected with Scan 3162

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.8	45971	PASS
75	95	30	66	57.4	102347	PASS
95	95	100	100	100.0	178453	PASS
96	95	5	9	6.5	11542	PASS
173	174	0.00	2	1.0	1135	PASS
174	95	50	120	61.1	109091	PASS
175	174	4	9	7.9	8641	PASS
176	174	93	101	100.9	110029	PASS
177	176	5	9	5.8	6386	PASS

Average of 10.367 to 10.374 min.: VL042074.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	499	45.95	123	56.00	3141	65.10	141
34.20	24	46.95	2324	56.95	5518	65.60	31
36.05	1847	47.80	581	57.90	195	66.00	9
37.05	10159	48.10	557	58.10	87	66.95	39
38.05	9726	49.05	8595	60.05	1431	67.20	111
39.05	3956	50.05	45971	61.05	8845	68.00	21867
39.90	401	51.05	13381	62.05	9305	69.00	21725
41.05	77	51.95	458	63.05	7854	70.10	1543
42.80	217	53.05	71	63.90	365	71.00	68
43.90	939	53.80	86	64.10	192	71.80	400
45.05	1864	55.05	665	64.90	127	72.05	639

Average of 10.367 to 10.374 min.: VL042074.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.05	7939	82.60	20	94.05	21349	110.80	88
74.05	34621	82.90	64	95.05	178453	111.95	81
75.00	102347	83.20	93	96.05	11542	112.90	33
76.05	9040	85.70	222	97.05	259	113.60	17
77.00	952	86.10	141	100.00	26	114.80	166
77.90	743	87.00	6274	103.00	44	116.00	577
78.95	4653	88.00	6722	103.90	820	116.95	1016
79.80	502	88.70	26	104.90	260	117.95	461
79.95	968	90.90	762	105.95	657	118.85	973
80.95	4962	92.05	5671	106.95	192	120.00	59
81.85	1201	93.05	7819	110.05	129	122.60	36

Average of 10.367 to 10.374 min.: VL042074.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
122.80	19	136.90	265	147.10	57	160.85	125
123.90	26	138.80	98	147.90	435	161.50	20
124.15	78	139.80	141	148.90	225	169.80	52
127.90	771	141.00	1695	149.60	44	170.00	52
128.90	476	141.85	195	149.95	159	170.50	74
129.95	904	142.10	50	151.75	87	171.15	95
131.05	359	142.85	1716	152.60	17	171.40	93
131.90	28	143.70	106	154.80	337	171.60	130
133.20	23	144.95	78	156.90	392	171.95	416
134.95	407	145.95	210	157.85	162	172.20	124
135.90	22	146.65	52	158.80	216	173.00	1135

Average of 10.367 to 10.374 min.: VL042074.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.00	109091						
175.00	8641						
176.00	110029						
176.95	6386						
178.00	252						
179.65	41						
186.60	29						
254.40	42						
268.40	46						