

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL030422\
Data File : VL038547.D
Acq On : 4 Mar 2022 23:16
Operator : SY/AP
Sample : CAN 10271
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10271

Quant Time: Mar 05 06:28:45 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL022222AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
QLast Update : Tue Feb 22 19:45:51 2022
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.64	49	906938	10.00	ppbv	-0.01
33) 1,4-Difluorobenzene	7.14	114	2079715	10.00	ppbv	-0.02
55) Chlorobenzene-d5	12.04	117	1776718	10.00	ppbv	-0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.37	95	1406040	9.56	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	95.60%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL030422\
Data File : VL038547.D
Acq On : 4 Mar 2022 23:16
Operator : SY/AP
Sample : CAN 10271
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10271

Quant Time: Mar 05 06:28:45 2022
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL022222AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
QLast Update : Tue Feb 22 19:45:51 2022
Response via : Initial Calibration

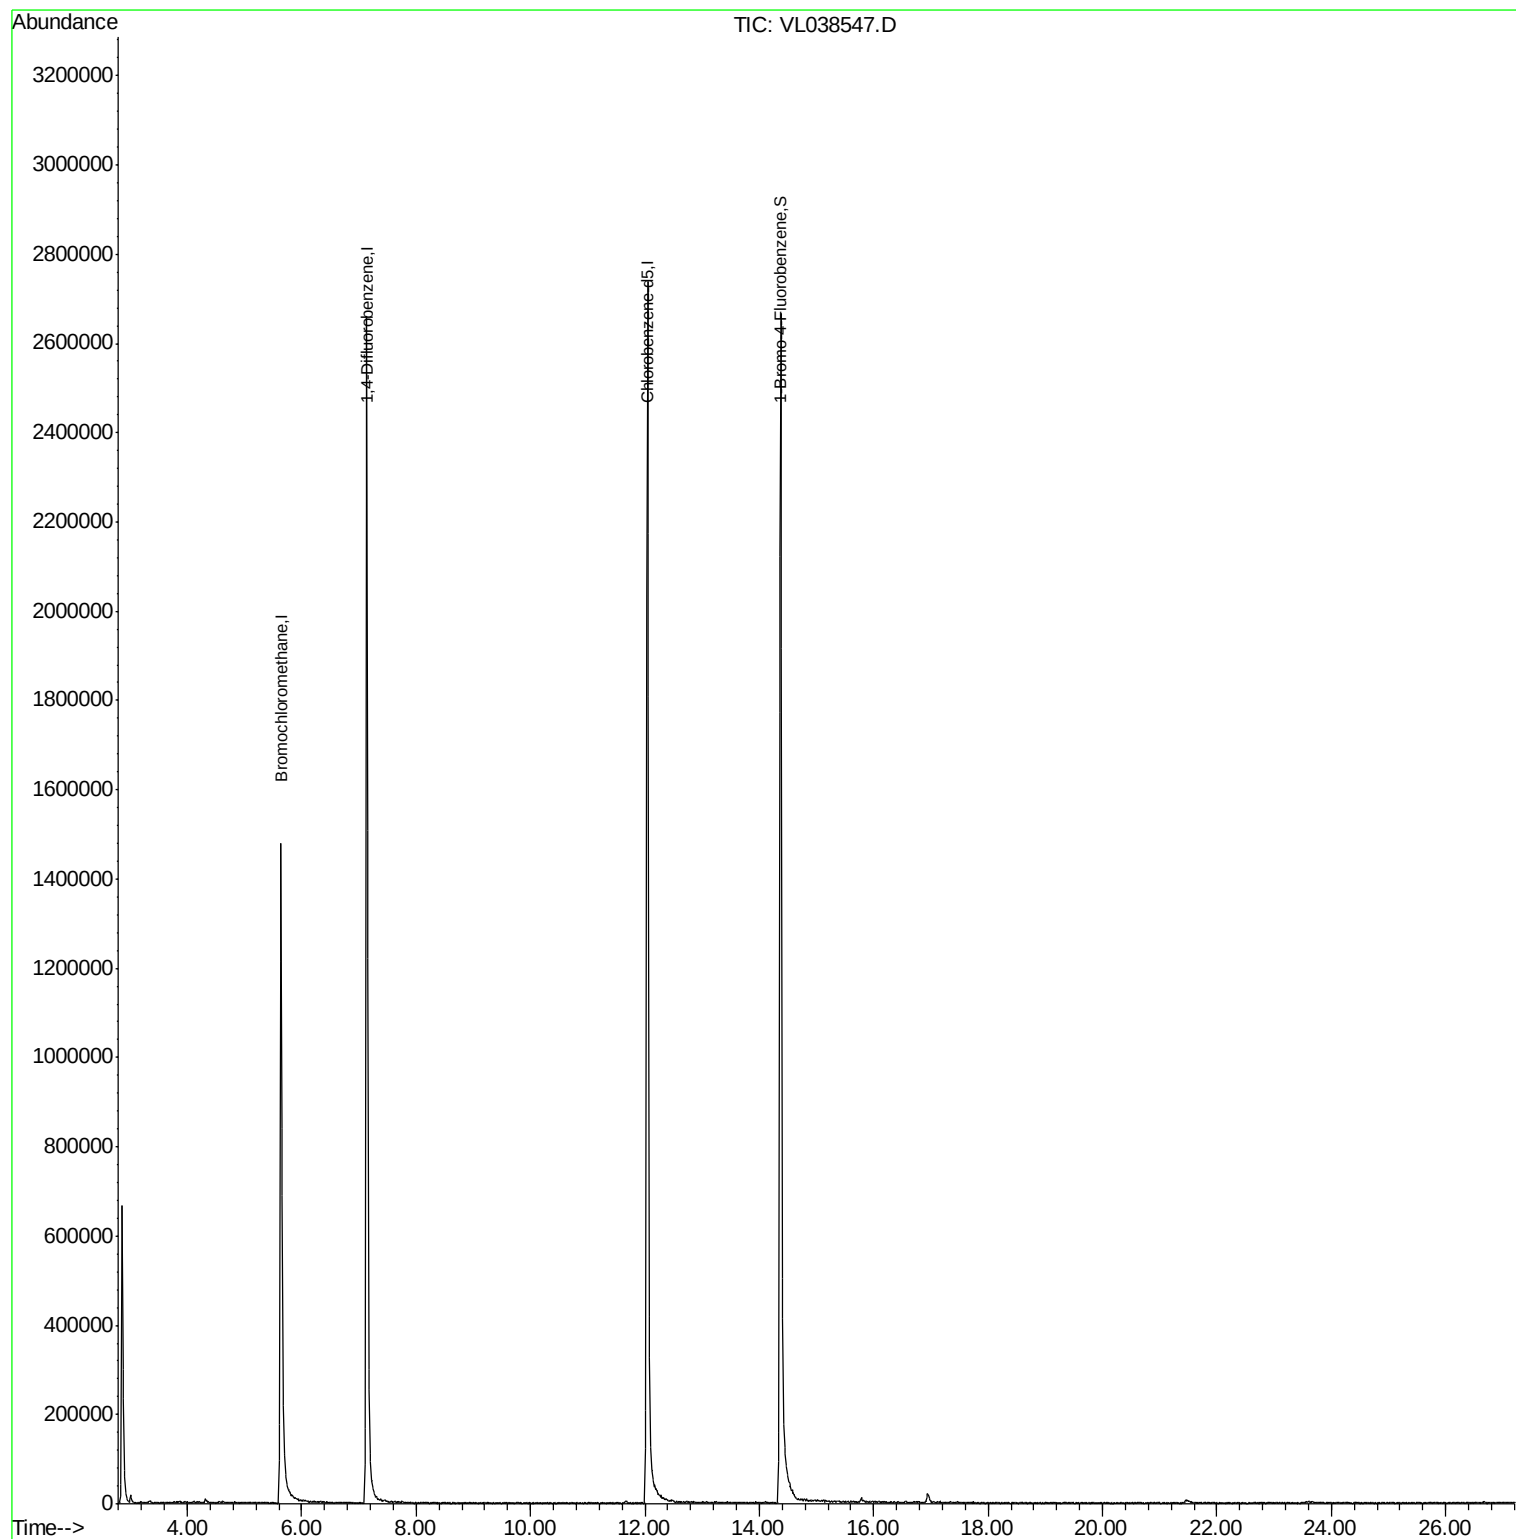

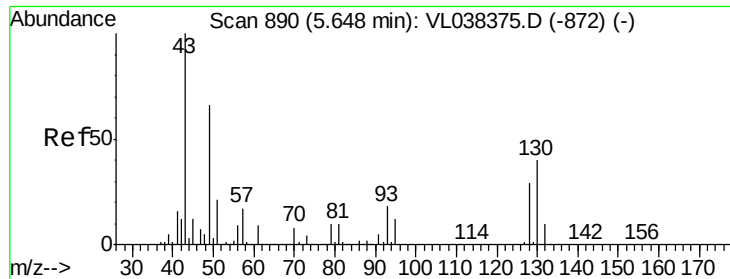

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.64 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 4 Mar 2022 23:16


Tot Ion: 49 Resp: 906938

Ion Ratio Lower Upper

49 100

128 45.3 24.3 72.9




130 57.9 30.1 90.5

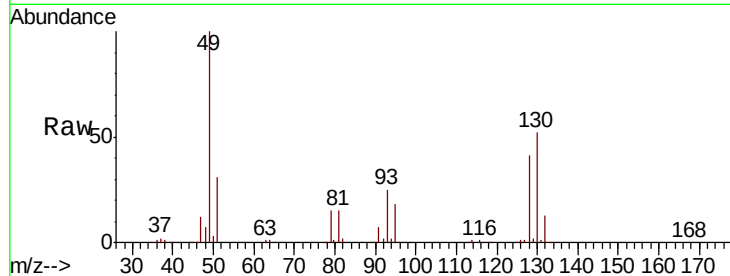

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

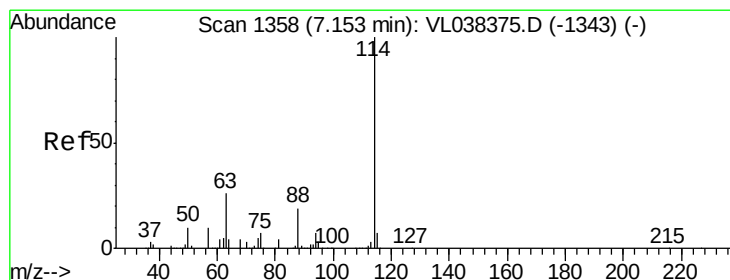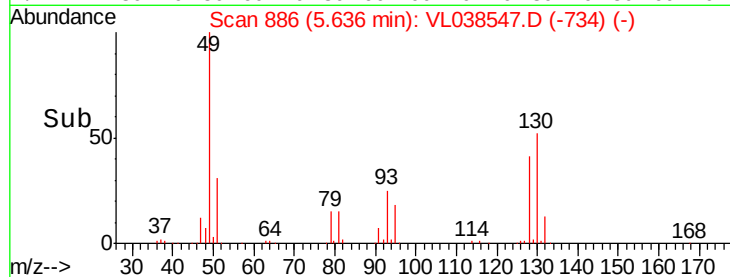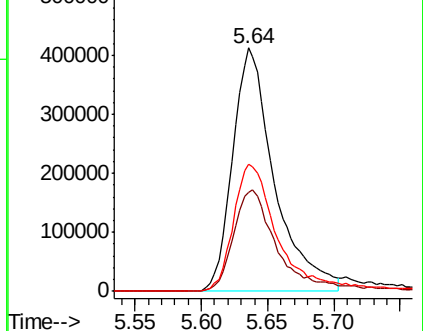

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.14 min Scan# 1353

Delta R.T. -0.02 min

Lab File: VL038547.D

Acq: 4 Mar 2022 23:16


Tgt Ion:114 Resp: 2079715

Ion Ratio Lower Upper

114 100

63 29.0 22.2 33.2



88 19.2 15.2 22.8

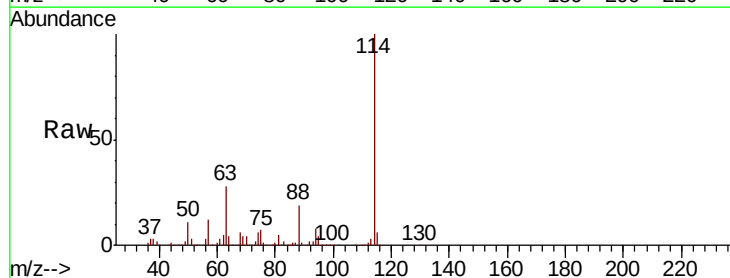


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0





Ion 88.10 (87.80 to 88.80): VL0

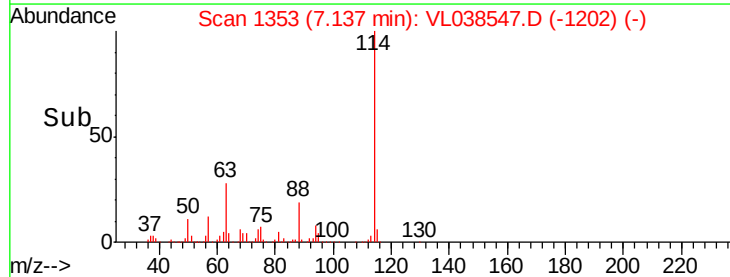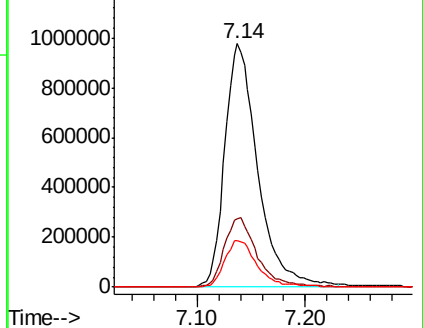

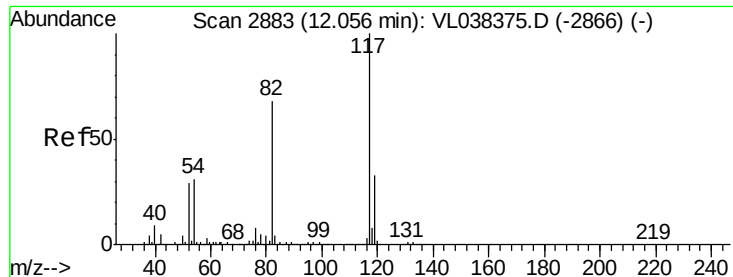

#55
 Chlorobenzene-d5
 Concen: 10.000 ppbv
 RT: 12.04 min
 Delta R.T. MSVOA_L
 Lab File: ClientSampleId :
 Acq: 4 Mar 2022 23:16

Tot Ion: 117 Resp: 1776718
 Ion Ratio Lower Upper
 117 100
 82 73.3 54.9 82.3
 119 33.2 46.1 69.1#

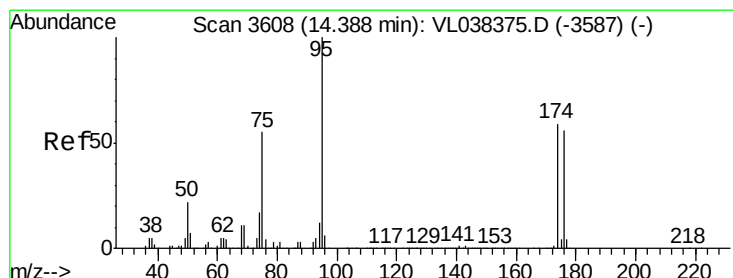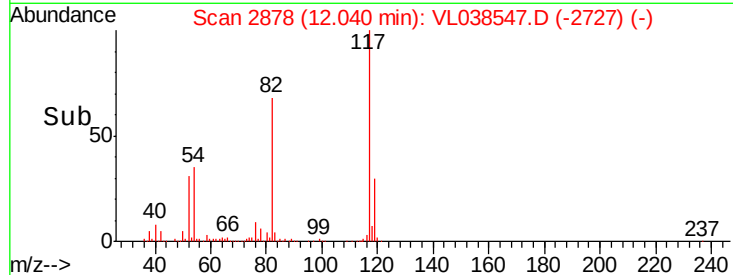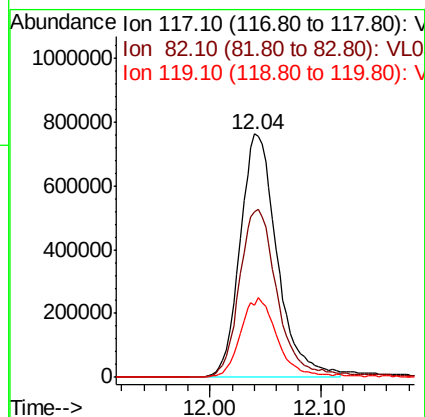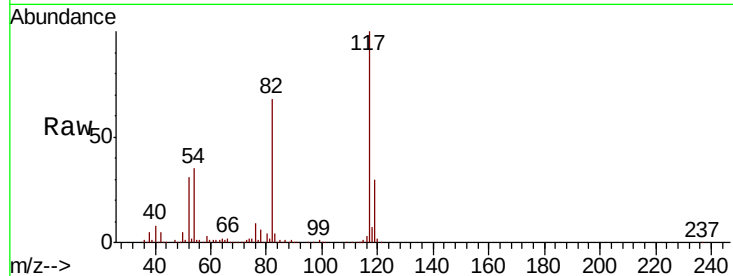

#68
 1-Bromo-4-Fluorobenzene
 Concen: 9.564 ppbv
 RT: 14.37 min Scan# 3603
 Delta R.T. -0.02 min
 Lab File: VL038547.D
 Acq: 4 Mar 2022 23:16

Tgt Ion: 95 Resp: 1406040
 Ion Ratio Lower Upper
 95 100
 174 58.6 49.0 73.4
 175 4.1 3.6 5.4

