

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL030422\
Data File : VL038549.D
Acq On : 5 Mar 2022 00:30
Operator : SY/AP
Sample : CAN 10321
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10321

Quant Time: Mar 05 06:29:59 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL022222AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
QLast Update : Tue Feb 22 19:45:51 2022
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.64	49	910263	10.00	ppbv	-0.01
33) 1,4-Difluorobenzene	7.14	114	2065153	10.00	ppbv	-0.01
55) Chlorobenzene-d5	12.04	117	1738670	10.00	ppbv	-0.01

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.37	95	1342879	9.33	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	93.30%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL030422\
Data File : VL038549.D
Acq On : 5 Mar 2022 00:30
Operator : SY/AP
Sample : CAN 10321
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10321

Quant Time: Mar 05 06:29:59 2022
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL022222AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
QLast Update : Tue Feb 22 19:45:51 2022
Response via : Initial Calibration

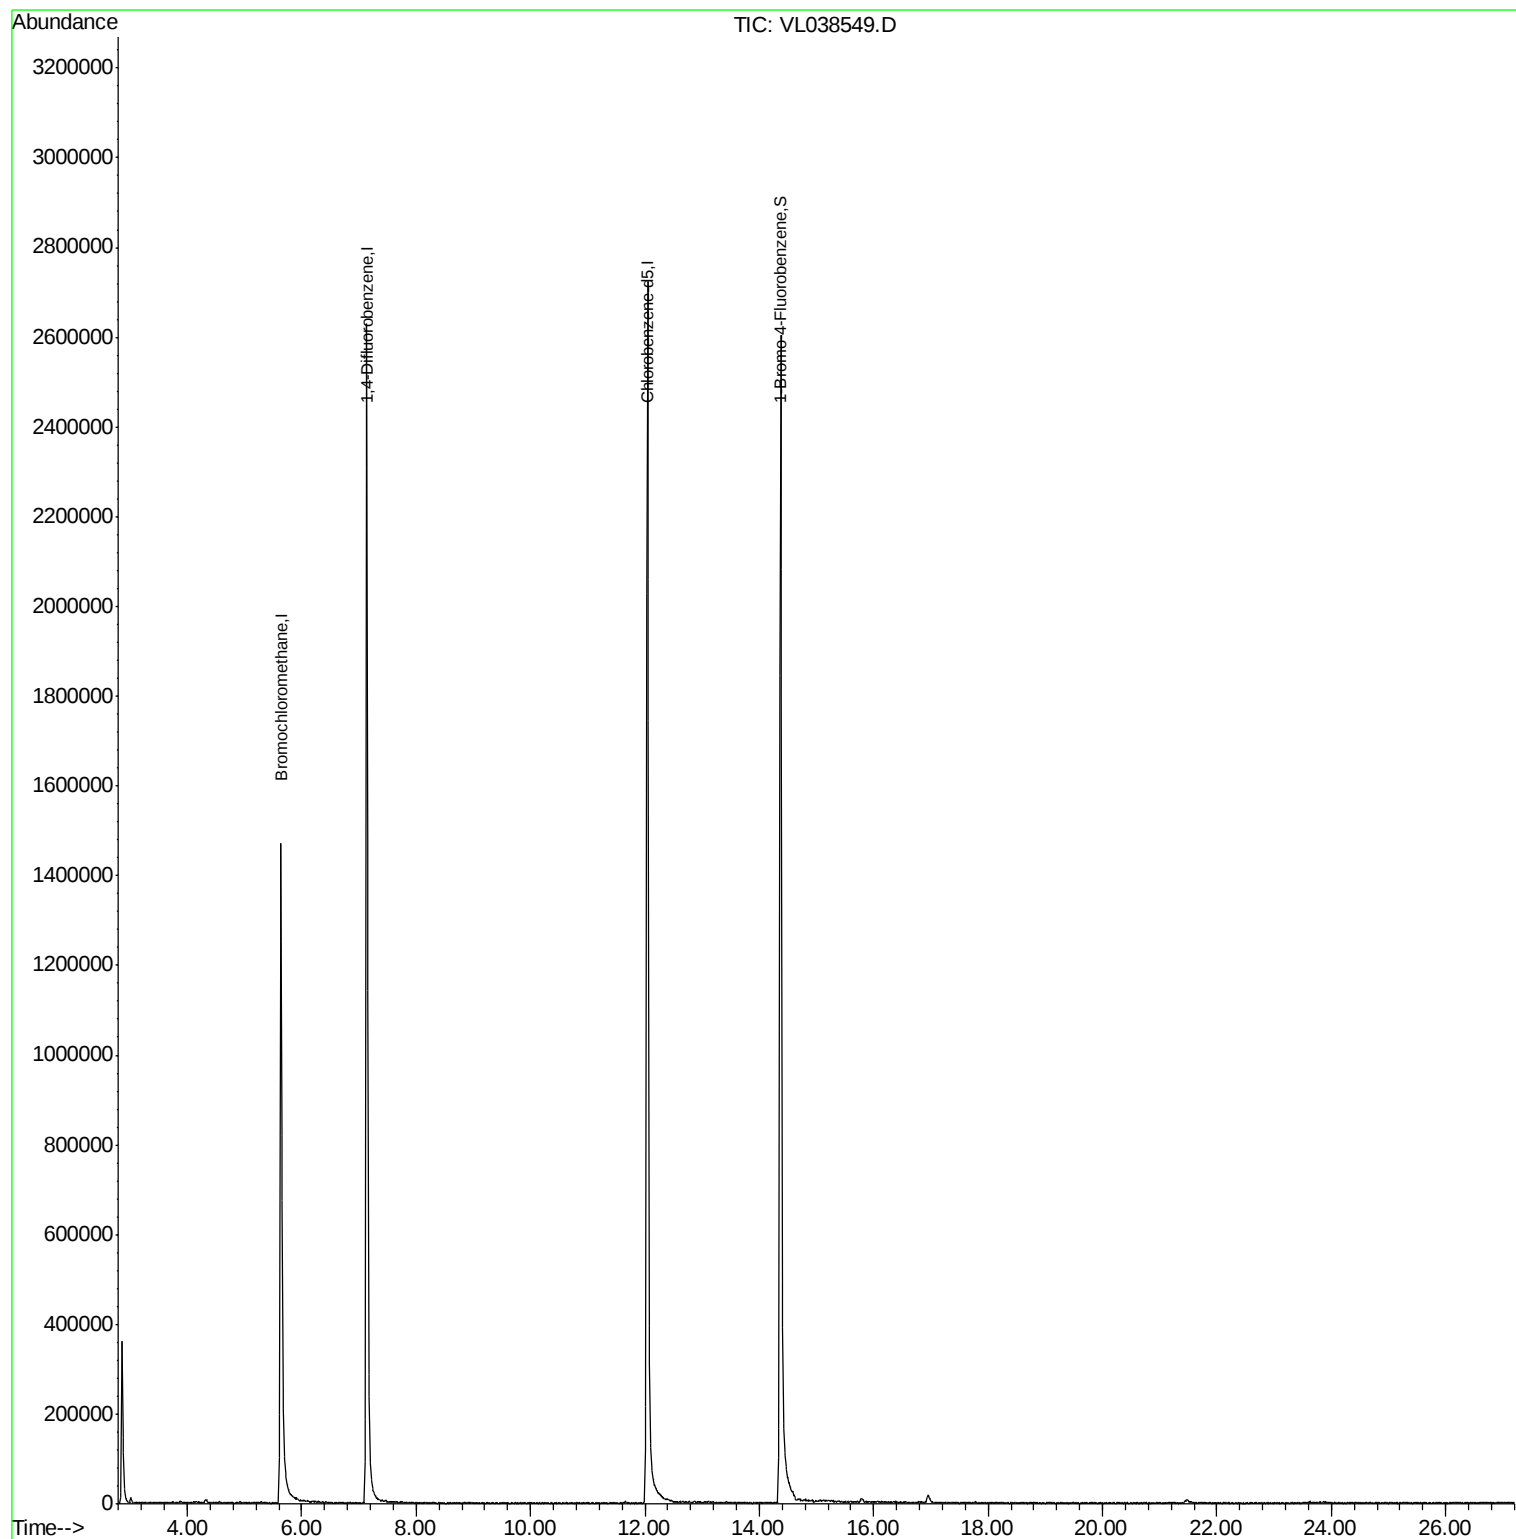

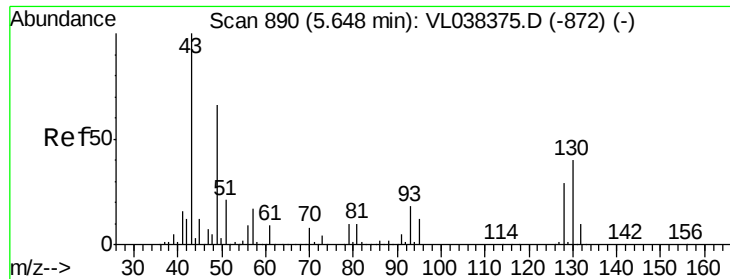

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.64 Instrument:

Delta R.T. MSVOA_L

Lab File: ClientSampleId:

Acq: 5 Mar 2022 00:30


Tot Ion: 49 Resp: 910263

Ion Ratio Lower Upper

49 100

128 44.2 24.3 72.9




130 57.2 30.1 90.5

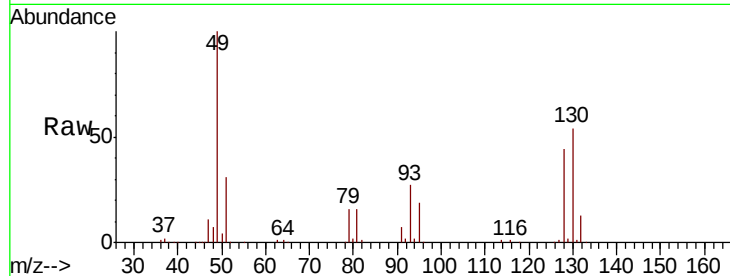

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

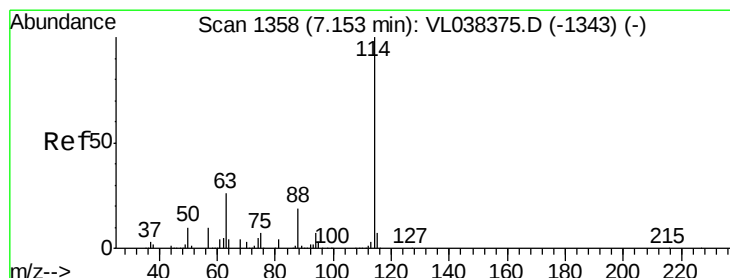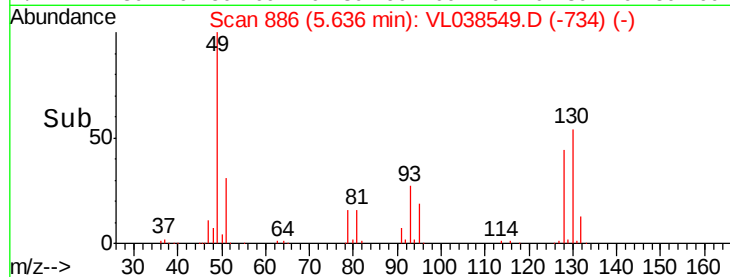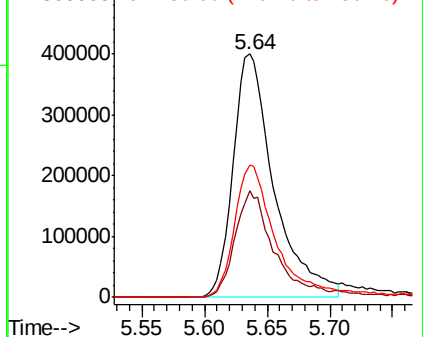

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.14 min Scan# 1354

Delta R.T. -0.01 min

Lab File: VL038549.D

Acq: 5 Mar 2022 00:30


Tgt Ion:114 Resp: 2065153

Ion Ratio Lower Upper

114 100

63 28.7 22.2 33.2



88 19.3 15.2 22.8

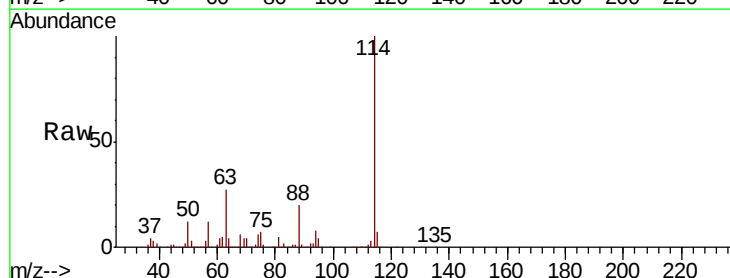


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0





Ion 88.10 (87.80 to 88.80): VL0

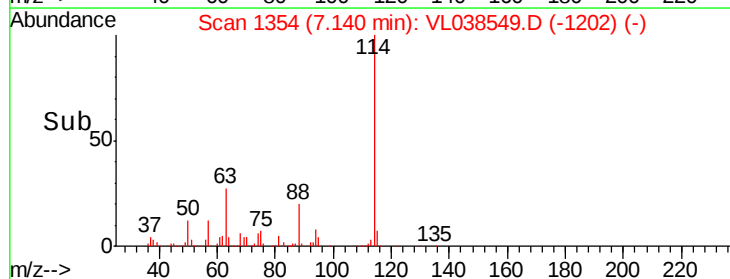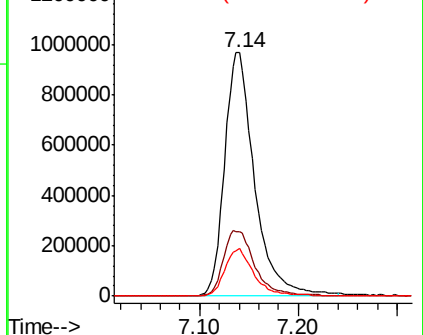

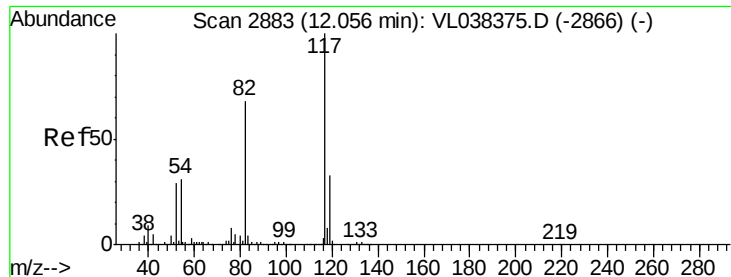

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.04 min
Instrument: MSVOA_1
Delta R.T.:
Lab File: ClientSampleId:
Acq: 5 Mar 2022 00:30

Tot Ion: 117 Resp: 1738670
Ion Ratio Lower Upper
117 100
82 74.8 54.9 82.3
119 33.8 46.1 69.1#

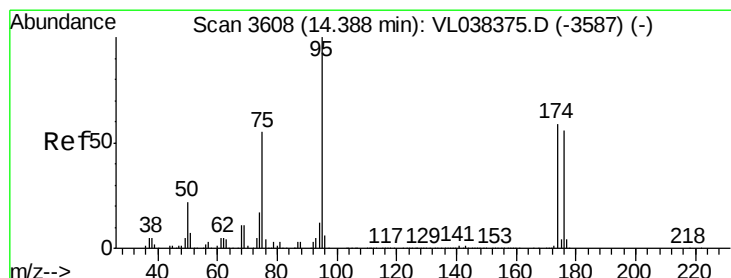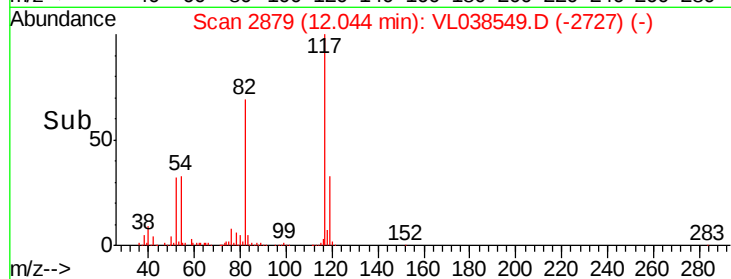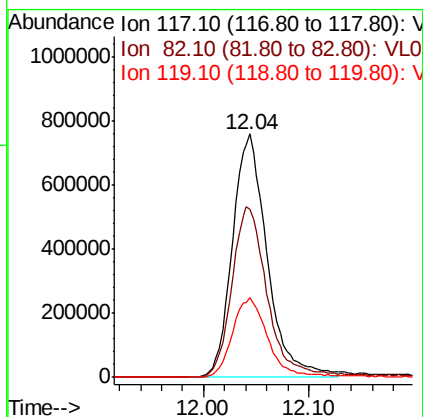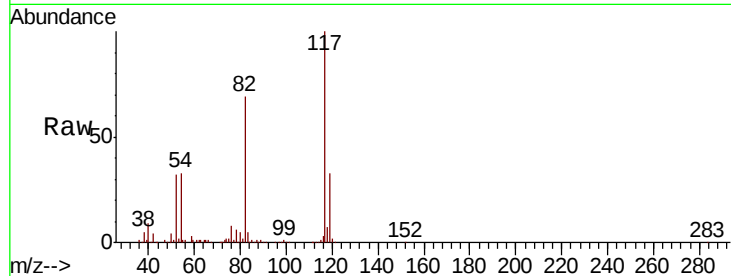

#68
1-Bromo-4-Fluorobenzene
Concen: 9.335 ppbv
RT: 14.37 min Scan# 3603
Delta R.T.: -0.02 min
Lab File: VL038549.D
Acq: 5 Mar 2022 00:30

Tgt Ion: 95 Resp: 1342879
Ion Ratio Lower Upper
95 100
174 59.9 49.0 73.4
175 4.2 3.6 5.4

