


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL030422\
Data File : VL038532.D
Acq On : 4 Mar 2022 12:44
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL022222AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Feb 22 19:45:51 2022
Last Update : Tue Feb 22 19:45:51 2022

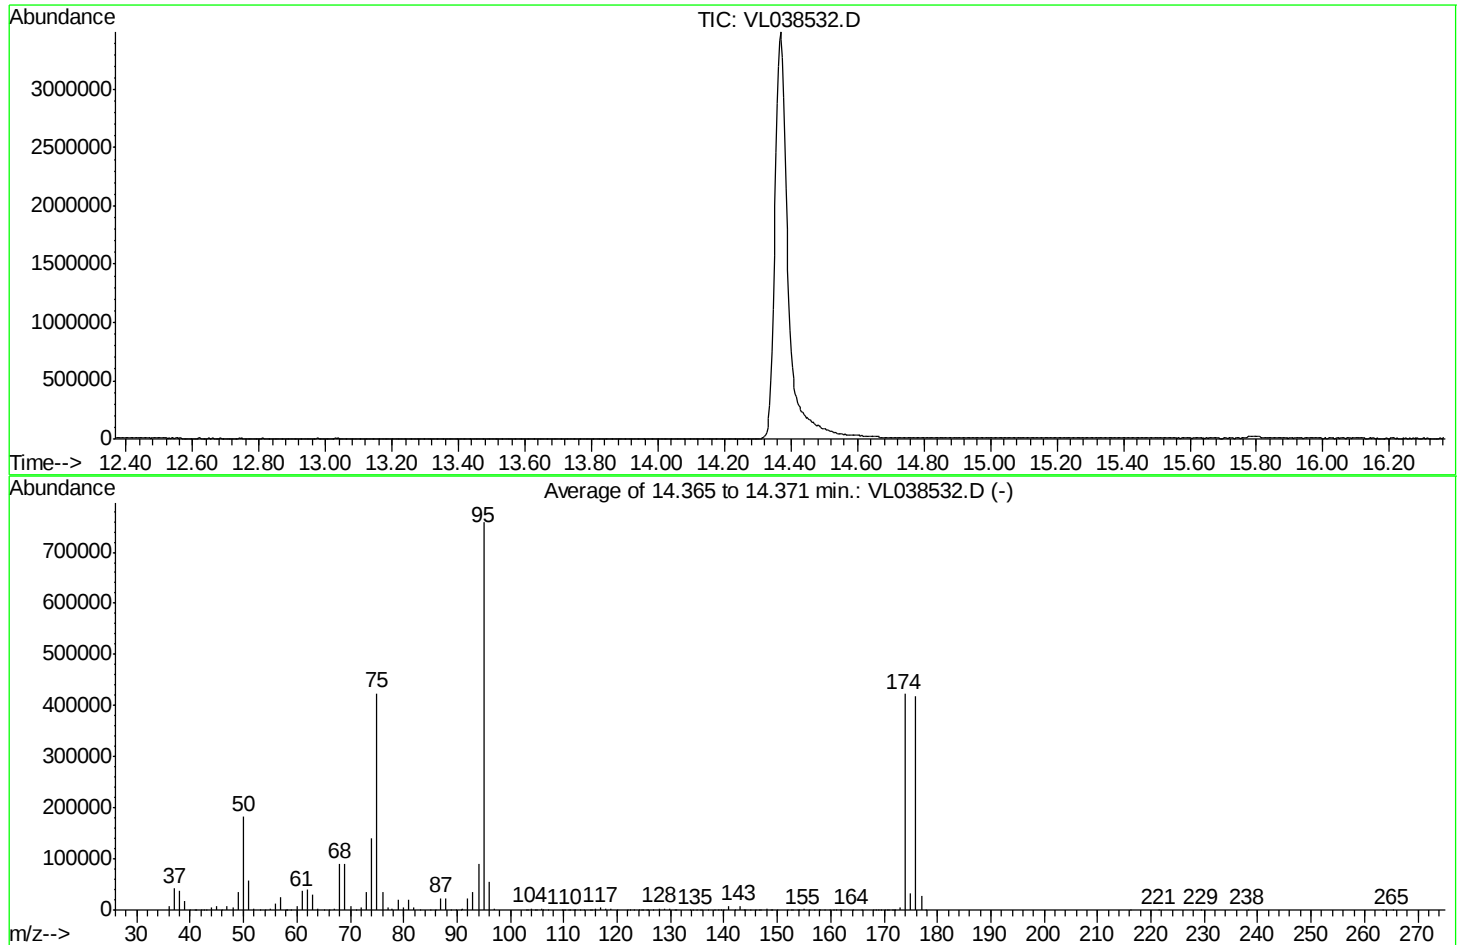

AutoFind: Scans 3601, 3602, 3603; Background Corrected with Scan 3576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.0	182208	PASS
75	95	30	66	55.9	424064	PASS
95	95	100	100	100.0	758485	PASS
96	95	5	9	7.2	54640	PASS
173	174	0.00	2	1.3	5446	PASS
174	95	50	120	55.7	422698	PASS
175	174	4	9	7.7	32498	PASS
176	174	93	101	98.8	417642	PASS
177	176	5	9	6.7	27850	PASS