


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL030525\
Data File : VL042094.D
Acq On : 05 Mar 2025 07:48
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL022525AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Feb 26 01:08:36 2025

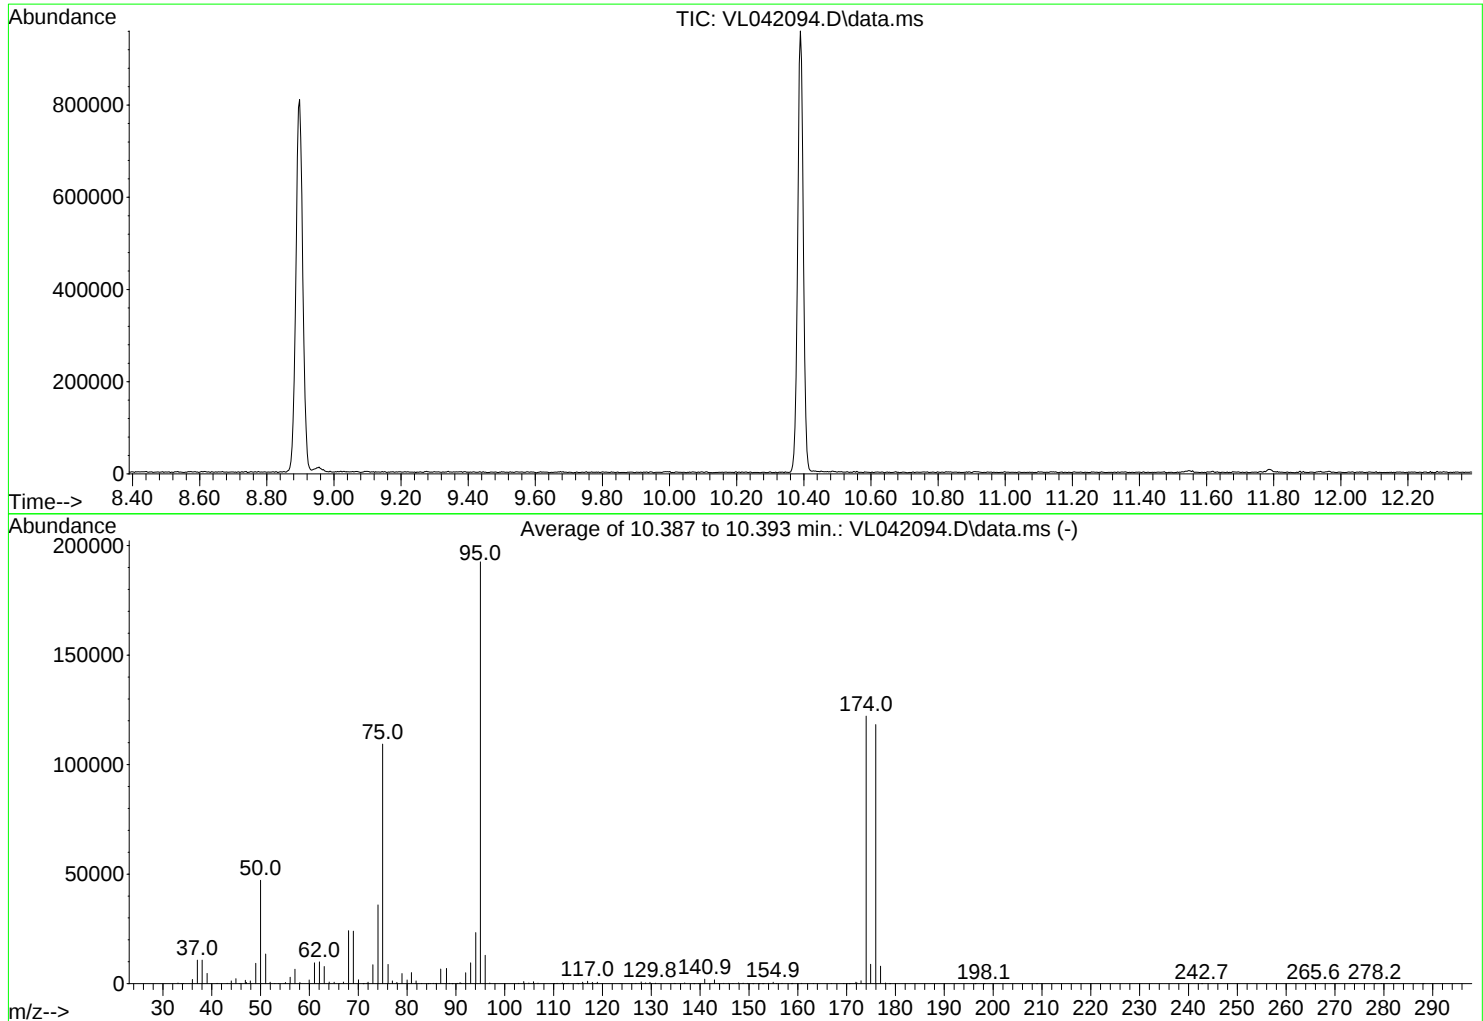

AutoFind: Scans 3182, 3183, 3184; Background Corrected with Scan 3168

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.5	47221	PASS
75	95	30	66	56.8	109403	PASS
95	95	100	100	100.0	192597	PASS
96	95	5	9	6.7	12955	PASS
173	174	0.00	2	1.1	1355	PASS
174	95	50	120	63.4	122160	PASS
175	174	4	9	7.2	8822	PASS
176	174	93	101	96.8	118272	PASS
177	176	5	9	6.8	8001	PASS

Average of 10.387 to 10.393 min.: VL042094.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	311	44.95	2292	53.70	80	65.05	691
33.75	46	45.70	53	54.80	135	66.10	91
34.20	46	45.95	170	55.10	505	66.95	711
36.05	1889	46.90	1504	56.05	2942	68.00	2418
37.05	10775	47.10	550	57.05	6564	69.00	23955
38.05	10756	47.90	1278	58.05	527	70.05	1729
39.05	4702	49.00	9251	59.95	1674	71.00	18
41.10	113	50.00	47221	61.05	9535	71.80	212
42.00	55	51.05	13512	62.05	9916	72.00	637
43.15	167	51.95	640	63.05	7808	73.00	8644
44.00	1229	52.90	75	64.05	748	74.05	35981

Average of 10.387 to 10.393 min.: VL042094.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.00	109403	85.35	119	93.00	9487	110.70	149
76.10	8743	85.80	68	94.05	23312	111.80	267
77.00	1276	86.00	154	95.00	192597	112.10	37
77.90	602	86.90	6677	96.00	12955	112.70	50
78.95	4612	88.05	6928	96.95	285	112.95	177
80.00	1664	88.70	143	102.85	137	114.80	161
80.90	5071	89.20	17	103.90	924	115.00	21
81.85	1260	90.25	129	104.95	326	115.95	695
83.00	93	90.85	537	105.90	884	116.95	1126
84.30	23	91.10	187	106.80	231	117.95	591
84.80	99	92.00	4979	110.00	18	118.70	149

Average of 10.387 to 10.393 min.: VL042094.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.95	675	135.95	46	146.75	69	156.75	191
123.65	82	136.85	350	147.90	394	158.70	37
124.00	55	138.70	21	148.80	212	158.95	134
126.05	61	139.70	87	149.75	185	160.05	63
126.85	127	140.10	126	150.80	29	160.80	157
127.95	787	140.95	2020	152.00	34	163.20	47
128.85	355	142.00	58	152.80	33	166.90	72
129.75	594	142.95	1781	153.05	60	169.40	93
130.90	247	143.80	45	154.00	156	170.10	94
134.70	185	144.85	188	154.95	640	170.50	34
134.90	70	145.85	172	155.70	51	170.85	93

Average of 10.387 to 10.393 min.: VL042094.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
171.10	64	196.30	24				
171.50	56	198.10	33				
171.90	639	208.90	19				
172.10	401	242.70	29				
172.95	1355	265.60	29				
174.00	122160	278.20	111				
174.90	8822	279.50	70				
175.95	118272	288.00	23				
176.95	8001						
177.95	308						
178.80	32						