


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL030620\
 Data File : VL034818.D
 Acq On : 6 Mar 2020 14:41
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL030420AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Mar 04 06:36:39 2020
 Last Update : Wed Mar 04 06:36:39 2020

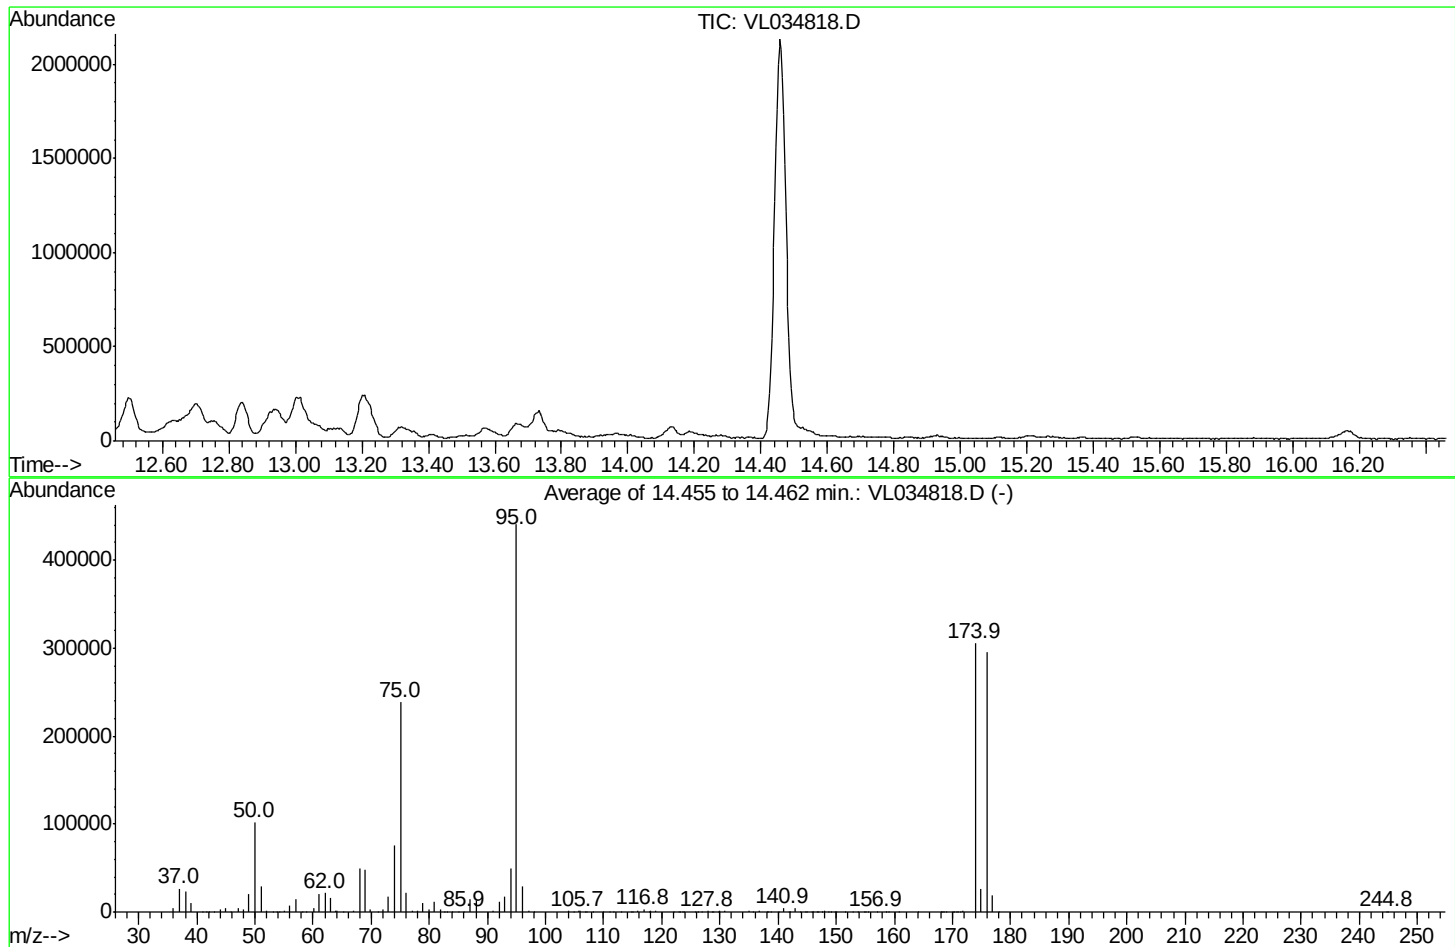

AutoFind: Scans 3629, 3630, 3631; Background Corrected with Scan 3606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.1	101773	PASS
75	95	30	66	54.0	238144	PASS
95	95	100	100	100.0	440832	PASS
96	95	5	9	6.8	29877	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.3	305578	PASS
175	174	4	9	8.8	26917	PASS
176	174	93	101	96.9	296064	PASS
177	176	5	9	6.6	19578	PASS