


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL031020\
 Data File : VL034862.D
 Acq On : 10 Mar 2020 10:08
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL030920AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Mar 09 16:42:53 2020
 Last Update : Mon Mar 09 16:42:53 2020

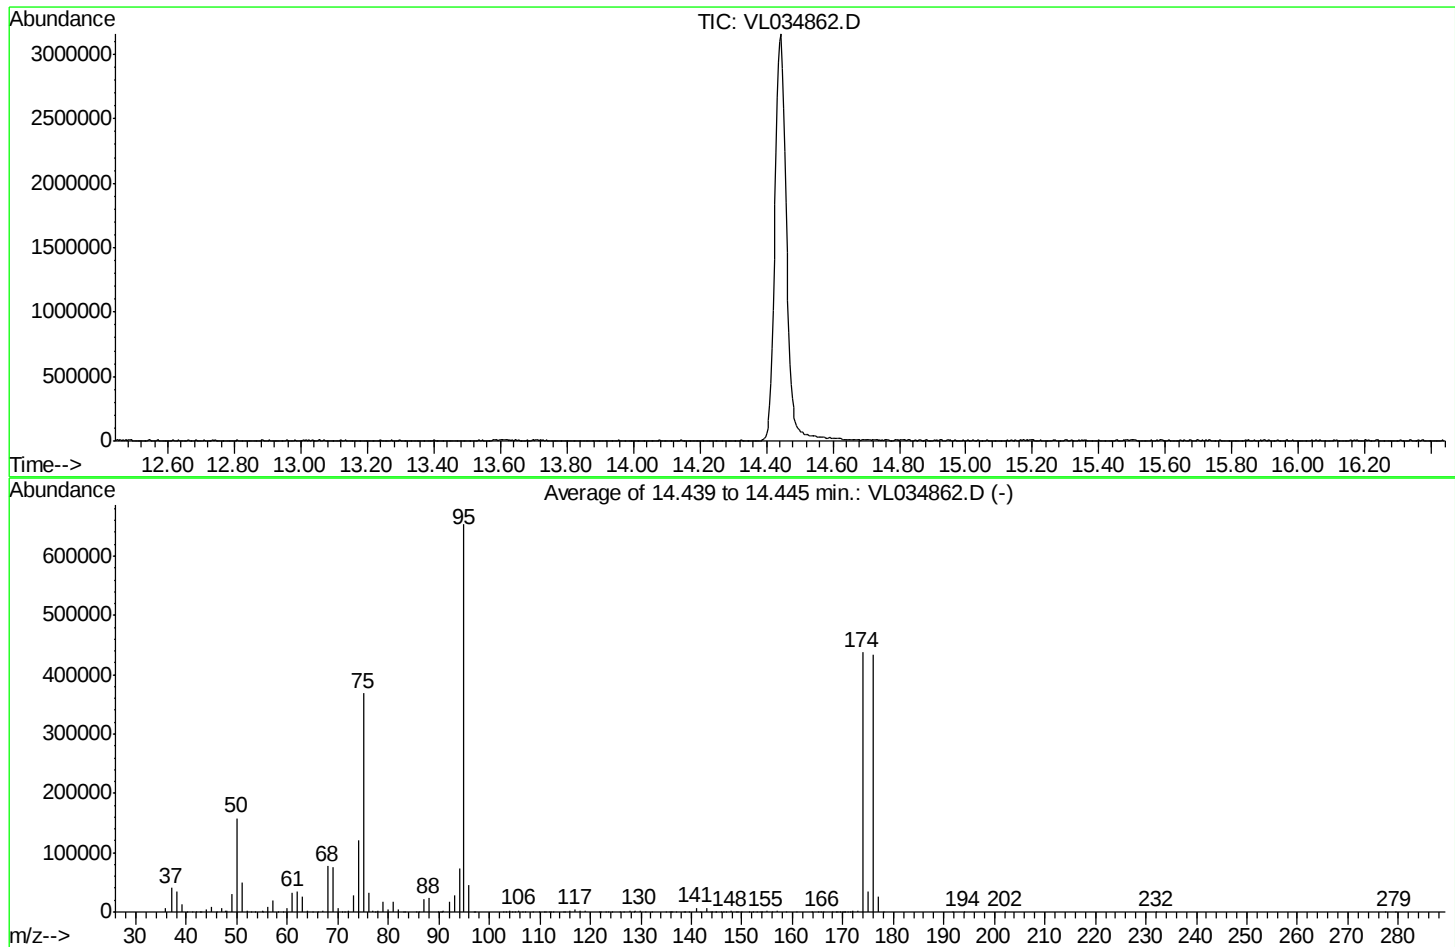

AutoFind: Scans 3624, 3625, 3626; Background Corrected with Scan 3603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.2	158357	PASS
75	95	30	66	56.4	368490	PASS
95	95	100	100	100.0	653632	PASS
96	95	5	9	7.0	45573	PASS
173	174	0.00	2	0.6	2649	PASS
174	95	50	120	67.0	437760	PASS
175	174	4	9	7.7	33768	PASS
176	174	93	101	99.1	433834	PASS
177	176	5	9	6.1	26296	PASS