


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL031224\
Data File : VL041090.D
Acq On : 12 Mar 2024 8:59
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL031124AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Mar 13 01:22:02 2024

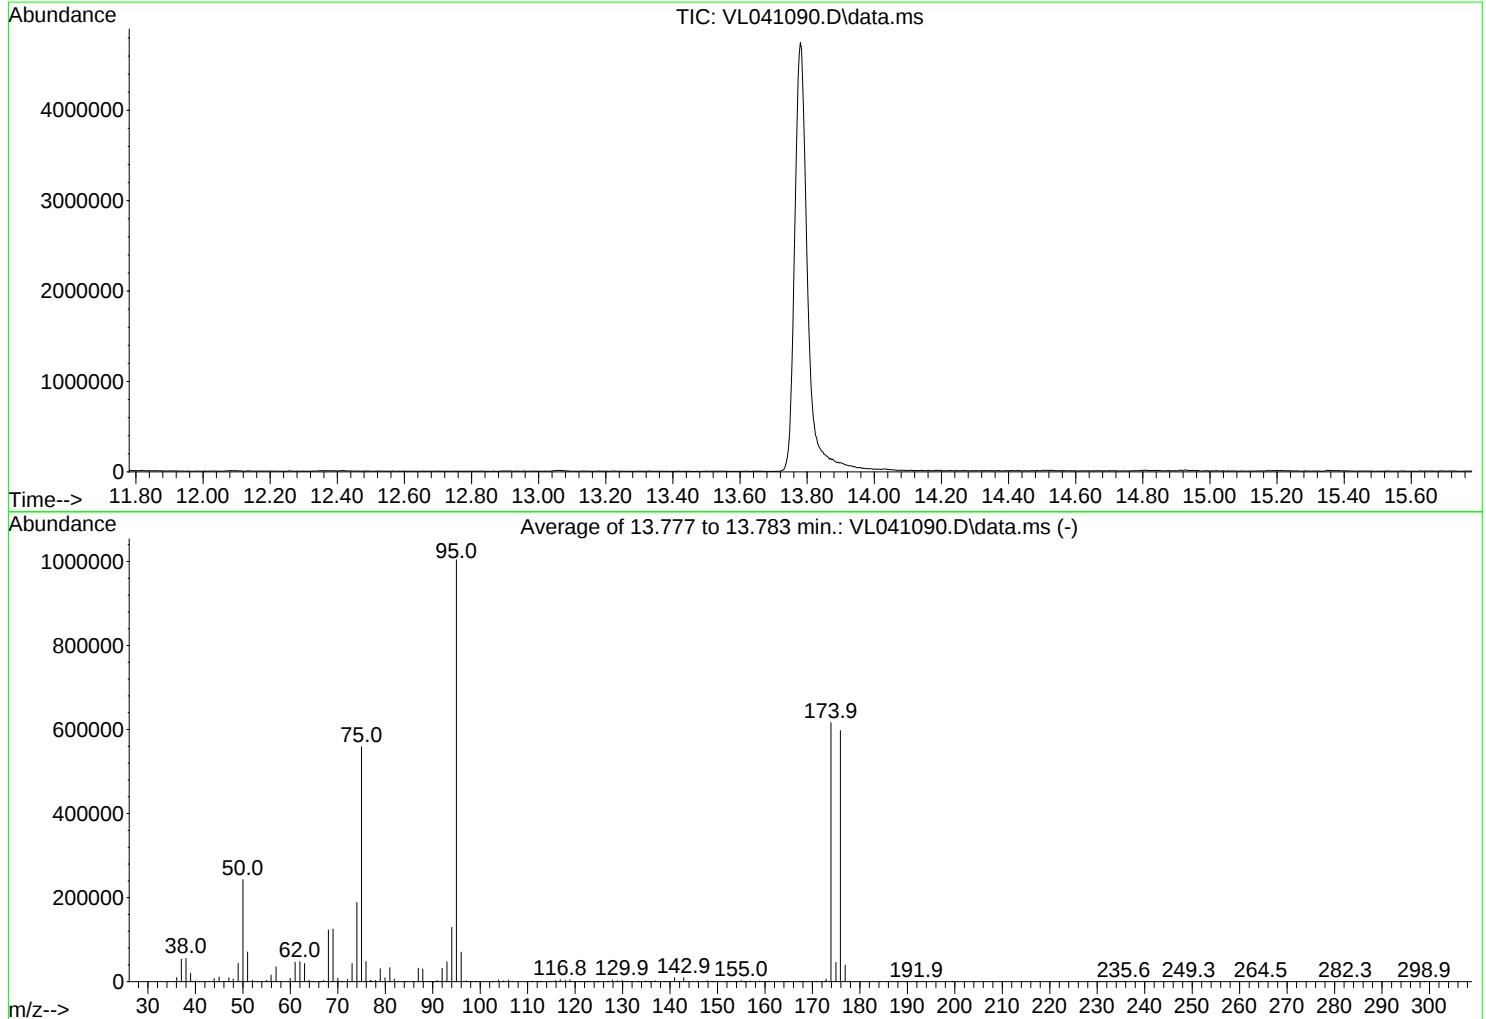

AutoFind: Scans 3475, 3476, 3477; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.2	242880	PASS
75	95	30	66	55.7	559083	PASS
95	95	100	100	100.0	1003755	PASS
96	95	5	9	7.0	70627	PASS
173	174	0.00	2	1.0	6214	PASS
174	95	50	120	61.4	616341	PASS
175	174	4	9	7.4	45776	PASS
176	174	93	101	96.9	597419	PASS
177	176	5	9	6.6	39355	PASS

Average of 13.777 to 13.783 min.: VL041090.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	9999	47.05	8979	58.05	1111	70.00	804
37.05	53373	47.95	5968	59.95	8050	70.80	15
38.00	55379	49.00	43957	61.00	46415	71.00	44
39.00	19699	50.00	242880	62.00	47528	72.05	513
40.05	1530	51.00	70283	63.00	43093	73.00	42981
41.30	398	52.05	3030	63.95	3460	74.00	188587
41.85	308	53.00	182	64.85	671	75.00	559083
42.80	545	53.85	303	66.20	180	75.95	47882
43.95	7379	55.00	3032	67.00	2502	76.85	3447
45.00	10927	55.95	15751	68.00	122856	77.10	1708
46.00	573	57.00	35539	69.00	125320	77.95	3026

Average of 13.777 to 13.783 min.: VL041090.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	31045	89.90	74	102.50	192	112.85	1260
79.95	8965	90.10	94	102.70	318	114.70	382
80.95	32976	90.90	3262	103.85	4371	114.90	462
81.90	6088	92.00	31779	104.85	1767	115.85	2916
82.70	306	93.00	47227	105.95	3803	116.85	5178
82.85	563	94.00	129253	106.80	808	117.95	3405
84.20	81	95.00	1.00376e+006	109.80	544	118.90	4794
85.85	809	96.00	70627	110.80	327	119.90	247
86.95	32168	97.05	2383	111.05	767	121.00	57
87.90	30277	98.20	219	111.95	568	121.85	401
89.40	182	98.95	161	112.20	204	122.50	180

Average of 13.777 to 13.783 min.: VL041090.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
122.90	138	133.30	56	140.95	9416	148.90	173
123.90	878	133.80	218	141.80	496	149.95	1206
124.50	96	134.80	646	142.00	533	151.70	163
124.90	92	134.95	1562	142.90	9645	152.00	437
125.85	557	135.60	117	143.80	314	152.75	528
126.80	56	135.90	175	144.05	423	153.65	266
127.85	3653	136.90	2221	144.80	677	153.90	84
128.95	1936	138.80	206	145.80	1315	155.00	2205
129.90	3400	138.95	336	146.90	506	155.70	100
130.90	1117	139.75	416	147.85	2280	155.90	261
131.80	401	140.00	499	148.70	441	156.90	1469

Average of 13.777 to 13.783 min.: VL041090.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
158.90	1704	170.75	786	191.90	78	298.90	64
160.10	58	171.00	394	195.00	53		
160.85	1107	171.90	959	199.40	63		
163.80	100	172.60	1304	230.40	65		
164.20	200	172.90	6214	234.70	76		
164.70	106	173.90	616341	235.60	126		
165.80	53	174.95	45776	240.70	87		
167.30	88	175.90	597419	247.90	56		
168.35	431	176.90	39355	249.30	103		
169.10	379	177.90	1408	264.50	52		
169.90	758	189.70	70	282.30	67		