


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL031319\
 Data File : VL033298.D
 Acq On : 13 Mar 2019 15:53
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL031319AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Mar 13 07:17:55 2019
 Last Update : Wed Mar 13 07:17:55 2019

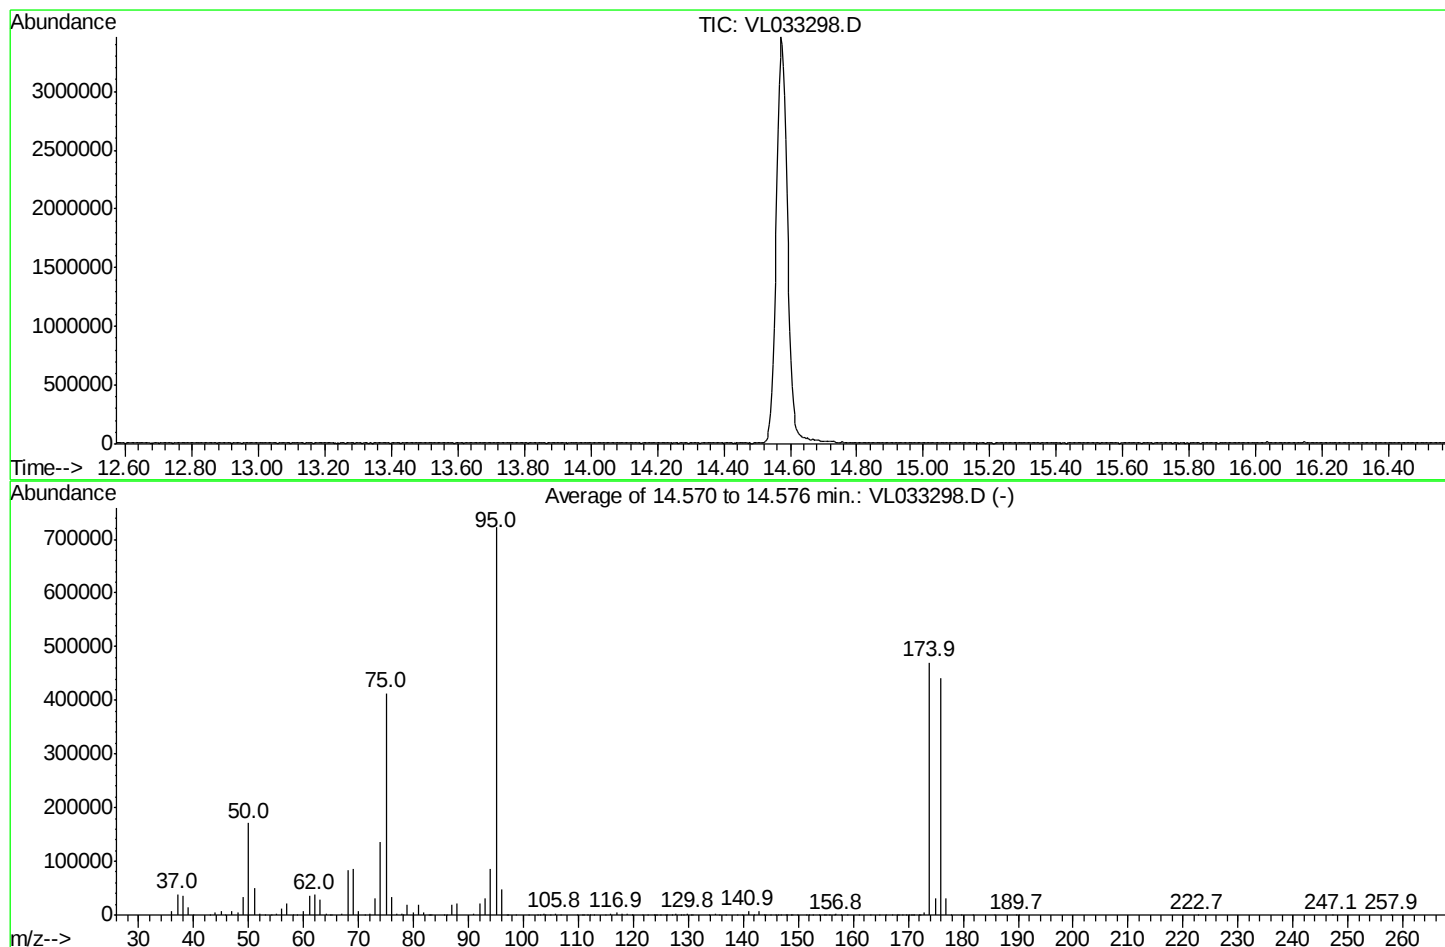

AutoFind: Scans 3618, 3619, 3620; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.6	170645	PASS
75	95	30	66	57.1	412736	PASS
95	95	100	100	100.0	722304	PASS
96	95	5	9	6.5	46837	PASS
173	174	0.00	2	0.8	3994	PASS
174	95	50	120	65.2	470741	PASS
175	174	4	9	6.8	32194	PASS
176	174	93	101	94.0	442325	PASS
177	176	5	9	6.8	30282	PASS