


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL031424\
Data File : VL041103.D
Acq On : 14 Mar 2024 10:05
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL031124AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 15 02:44:43 2024

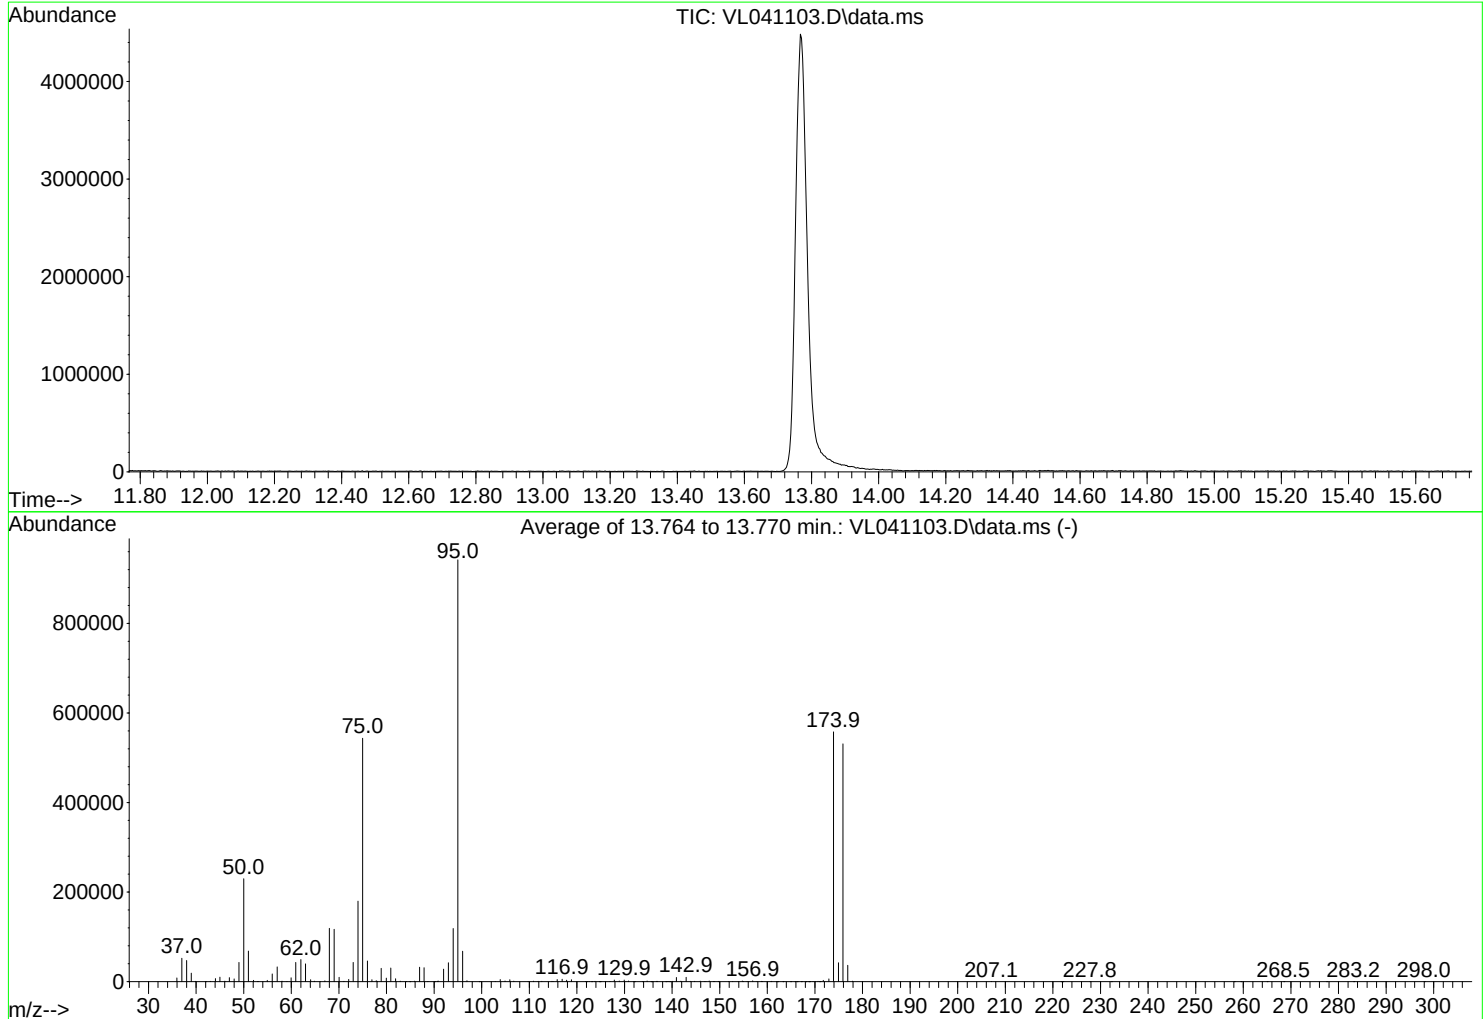

AutoFind: Scans 3471, 3472, 3473; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	229717	PASS
75	95	30	66	57.7	543616	PASS
95	95	100	100	100.0	941909	PASS
96	95	5	9	7.2	67880	PASS
173	174	0.00	2	1.1	6200	PASS
174	95	50	120	59.2	557717	PASS
175	174	4	9	7.6	42189	PASS
176	174	93	101	95.2	530944	PASS
177	176	5	9	6.9	36395	PASS

Average of 13.764 to 13.770 min.: VL041103.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	8209	48.00	5960	59.10	228	70.05	978
37.00	52053	49.00	42787	59.95	8422	71.05	68
38.00	47059	50.00	229717	60.95	42792	72.05	517
39.00	19118	51.00	68243	62.00	49424	73.00	4295
39.85	629	52.05	2856	63.00	39555	74.00	179733
41.95	143	52.90	239	64.05	4161	75.00	543616
43.00	747	53.15	209	64.85	1167	76.00	45984
44.05	6897	54.95	2800	66.10	267	76.95	4325
45.00	10189	56.00	17094	67.05	1770	77.85	2005
46.05	1139	57.05	32757	68.00	118896	78.10	916
47.00	9118	58.05	1273	69.00	116709	78.90	29523

Average of 13.764 to 13.770 min.: VL041103.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.95	7863	90.70	814	104.90	1479	117.85	3291
80.90	30549	90.85	1539	105.90	4279	118.85	4397
81.90	6581	92.00	27939	106.75	1207	121.80	365
82.90	1128	93.00	42360	109.75	573	122.00	115
84.20	334	94.00	118771	110.90	1029	122.60	327
84.90	91	95.00	941909	111.85	700	123.10	163
85.90	1187	96.00	67880	112.65	860	123.80	685
86.95	32040	96.90	2011	114.75	737	124.70	133
87.90	31024	99.50	60	115.00	357	124.90	149
88.70	345	102.85	282	115.85	4513	126.00	373
90.10	67	103.90	4545	116.90	5394	126.95	322

Average of 13.764 to 13.770 min.: VL041103.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
127.85	3479	136.90	661	145.90	1083	154.75	1410
128.90	1612	138.70	173	146.75	411	155.00	497
129.95	3716	139.00	201	147.10	235	155.75	226
130.85	1562	139.30	201	147.80	1561	156.10	303
131.90	53	139.50	76	148.70	204	156.95	1686
132.10	55	140.05	584	148.95	402	157.85	310
133.80	95	140.90	9286	149.70	238	158.80	597
134.75	1621	141.85	1242	149.85	613	159.00	279
135.60	113	142.95	9762	151.90	539	160.80	295
135.80	119	143.90	728	152.75	431	160.95	841
136.70	835	144.75	922	153.90	438	161.90	166

Average of 13.764 to 13.770 min.: VL041103.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
162.20	119	170.65	780	221.70	92		
163.30	51	171.00	184	222.10	55		
164.90	51	171.30	454	227.80	182		
165.85	167	171.75	2866	232.30	59		
166.30	98	172.95	6200	258.10	64		
167.15	183	173.90	557717	259.50	66		
168.15	190	174.95	42189	265.00	64		
168.70	83	175.90	530944	268.50	104		
168.90	143	176.90	36395	277.50	57		
169.60	519	177.90	1128	283.20	71		
170.10	255	207.10	220	298.00	58		