

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL031819\
Data File : VL033383.D
Acq On : 19 Mar 2019 9:08
Operator : SY/AP
Sample : VIBLK
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Quant Time: Mar 20 01:35:22 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL031519AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Mar 15 14:52:14 2019
QLast Update : Fri Mar 15 14:52:14 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.76	49	722633	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.29	114	1642281	10.00	ppbv	-0.01
55) Chlorobenzene-d5	12.24	117	1615289	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.57	95	1214162	10.14	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	101.40%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL031819\
Data File : VL033383.D
Acq On : 19 Mar 2019 9:08
Operator : SY/AP
Sample : VIBLK
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Quant Time: Mar 20 01:35:22 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL031519AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Mar 15 14:52:14 2019
QLast Update : Fri Mar 15 14:52:14 2019
Response via : Initial Calibration

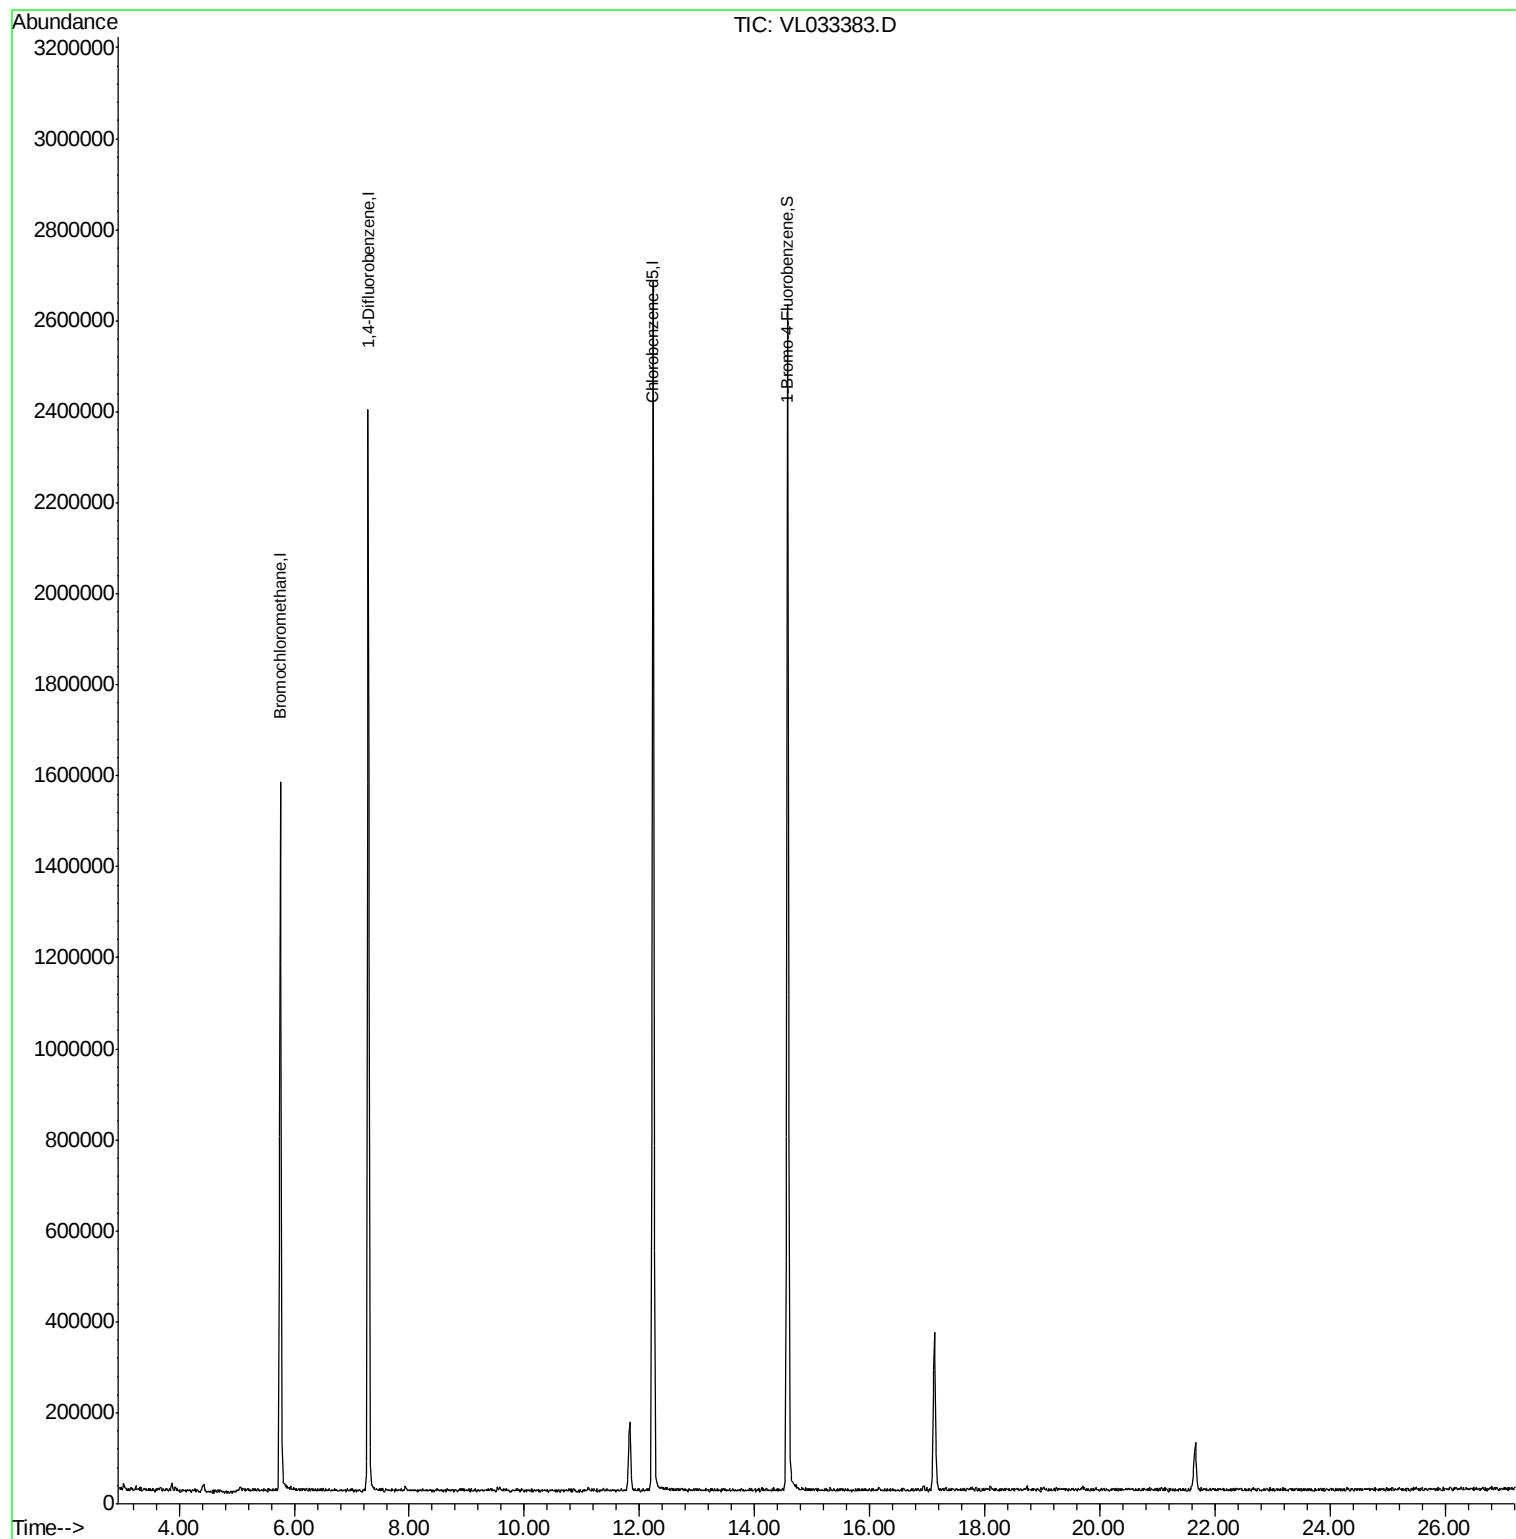

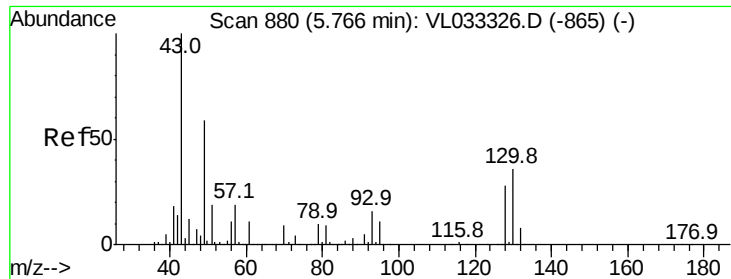

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.76 min Scan# 877

Delta R.T. -0.01 min

Lab File: VL033383.D

Acq: 19 Mar 2019 9:08

Instrument :

MSVOA_L

ClientSampleId :

VIBLK


Tot Ion: 49 Resp: 722633

Ion Ratio Lower Upper

49 100

128 48.3 23.5 70.6




130 62.1 30.1 90.3

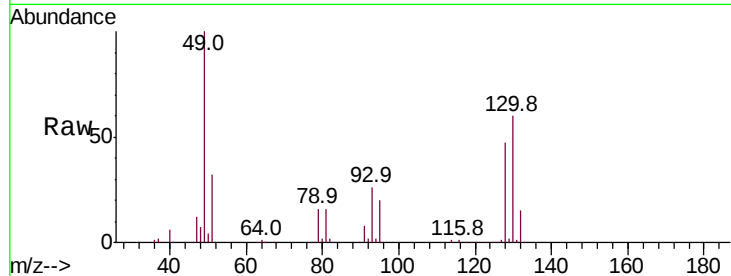

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

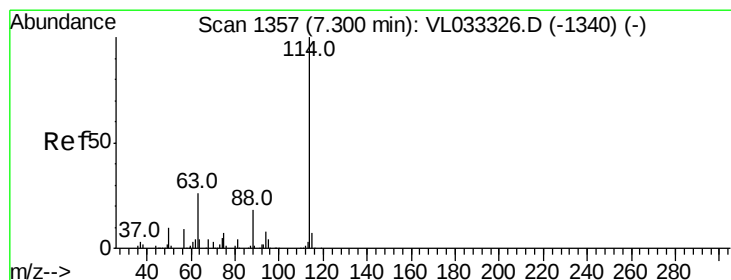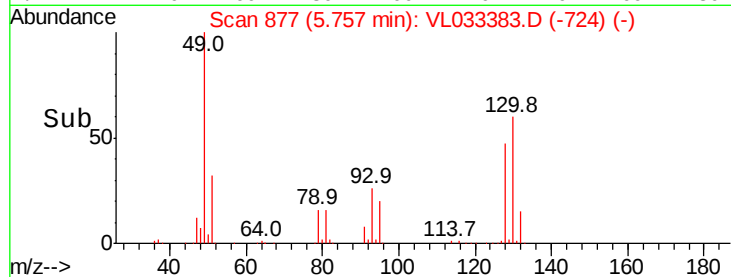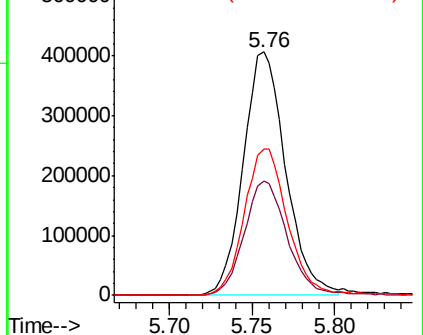

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.29 min Scan# 1353

Delta R.T. -0.01 min

Lab File: VL033383.D

Acq: 19 Mar 2019 9:08


Tgt Ion: 114 Resp: 1642281

Ion Ratio Lower Upper

114 100

63 26.7 21.4 32.2



88 18.1 14.5 21.7

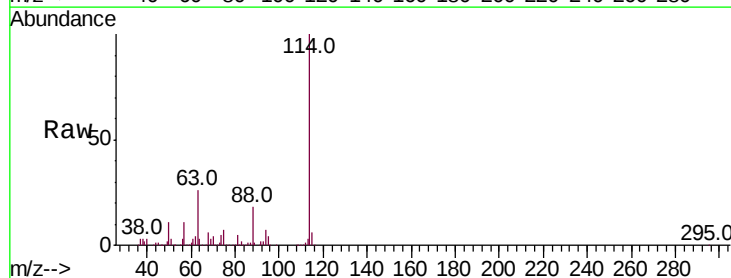


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0



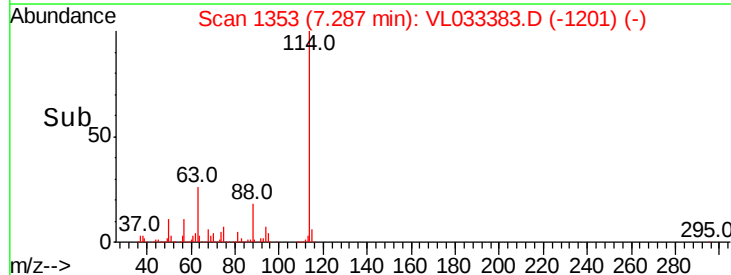
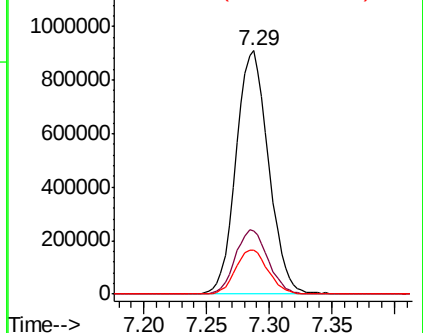


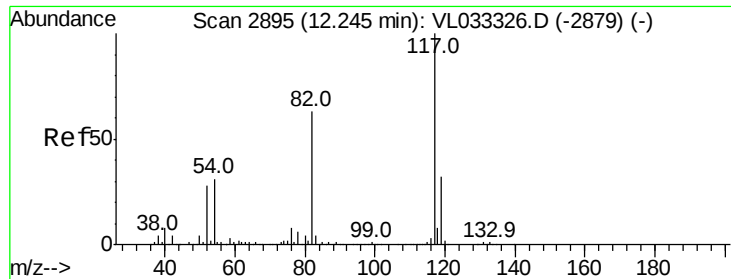

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.24 min Scan# 2892
Delta R.T. -0.01 min
Lab File: VL033383.D
Acq: 19 Mar 2019 9:08

Instrument :
MSVOA_L
ClientSampleId :
VIBLK

Tot Ion:117 Resp: 1615289
Ion Ratio Lower Upper
117 100
82 67.1 53.4 80.2
119 32.1 27.3 40.9

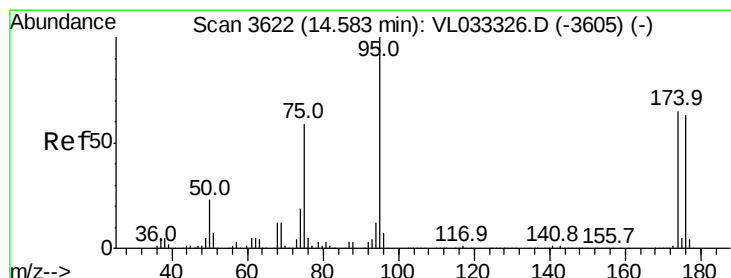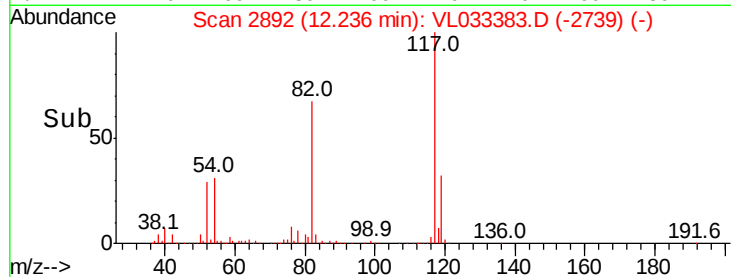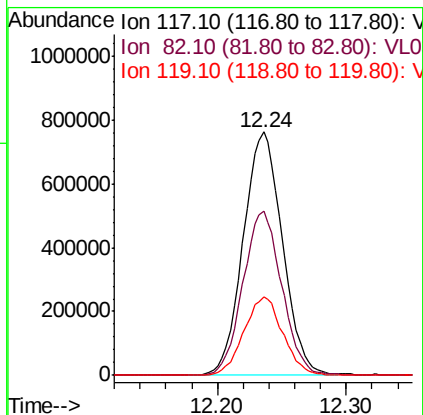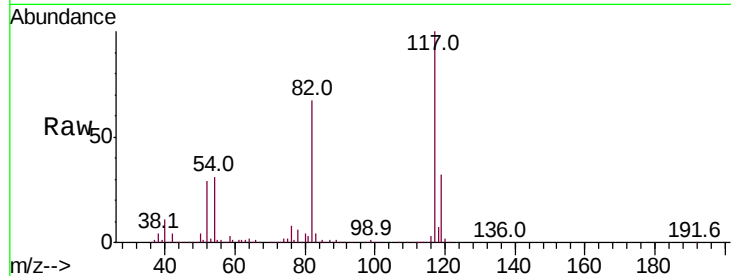

#68
1-Bromo-4-Fluorobenzene
Concen: 10.144 ppbv
RT: 14.57 min Scan# 3619
Delta R.T. -0.01 min
Lab File: VL033383.D
Acq: 19 Mar 2019 9:08

Tgt Ion: 95 Resp: 1214162
Ion Ratio Lower Upper
95 100
174 64.7 51.5 77.3
175 4.8 3.8 5.6

