


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL031819\
 Data File : VL033358.D
 Acq On : 18 Mar 2019 14:12
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL031519AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Mar 15 14:52:14 2019
 Last Update : Fri Mar 15 14:52:14 2019

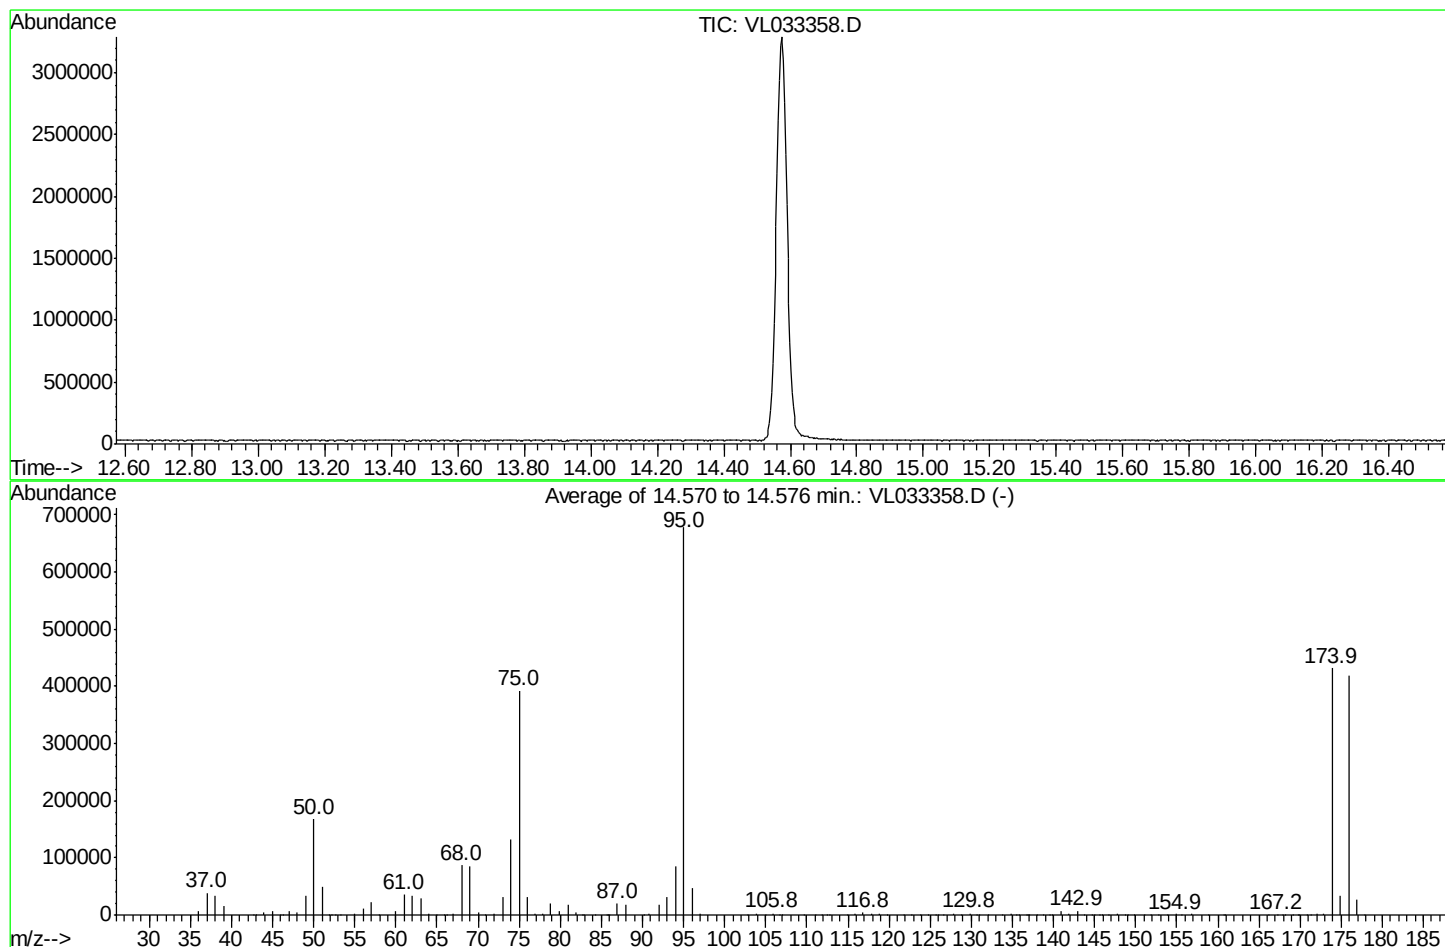

AutoFind: Scans 3618, 3619, 3620; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.6	167040	PASS
75	95	30	66	57.9	393013	PASS
95	95	100	100	100.0	678336	PASS
96	95	5	9	6.9	46928	PASS
173	174	0.00	2	0.8	3324	PASS
174	95	50	120	63.7	431786	PASS
175	174	4	9	7.9	33965	PASS
176	174	93	101	97.2	419840	PASS
177	176	5	9	6.7	28045	PASS