


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL032119\
 Data File : VL033420.D
 Acq On : 21 Mar 2019 16:12
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL031519AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Mar 15 14:52:14 2019
 Last Update : Fri Mar 15 14:52:14 2019

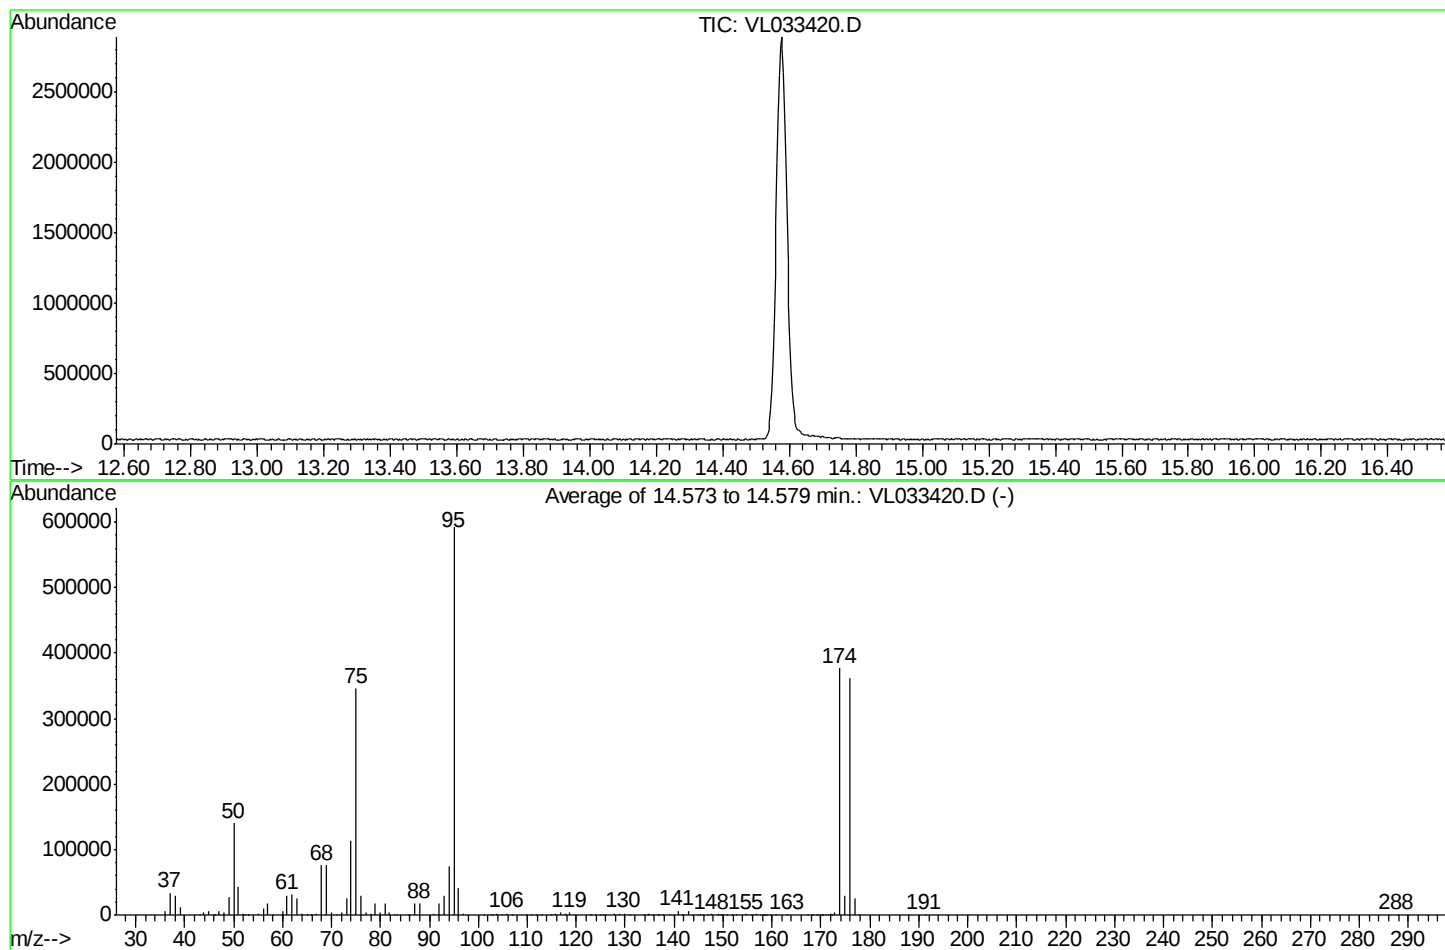

AutoFind: Scans 3619, 3620, 3621; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.6	139882	PASS
75	95	30	66	58.3	345344	PASS
95	95	100	100	100.0	592128	PASS
96	95	5	9	6.8	40472	PASS
173	174	0.00	2	0.9	3368	PASS
174	95	50	120	63.6	376554	PASS
175	174	4	9	7.6	28688	PASS
176	174	93	101	96.0	361578	PASS
177	176	5	9	7.0	25362	PASS