


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032122\
 Data File : VL038647.D
 Acq On : 21 Mar 2022 11:58
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL032122AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Mar 21 17:09:26 2022
 Last Update : Mon Mar 21 17:09:26 2022

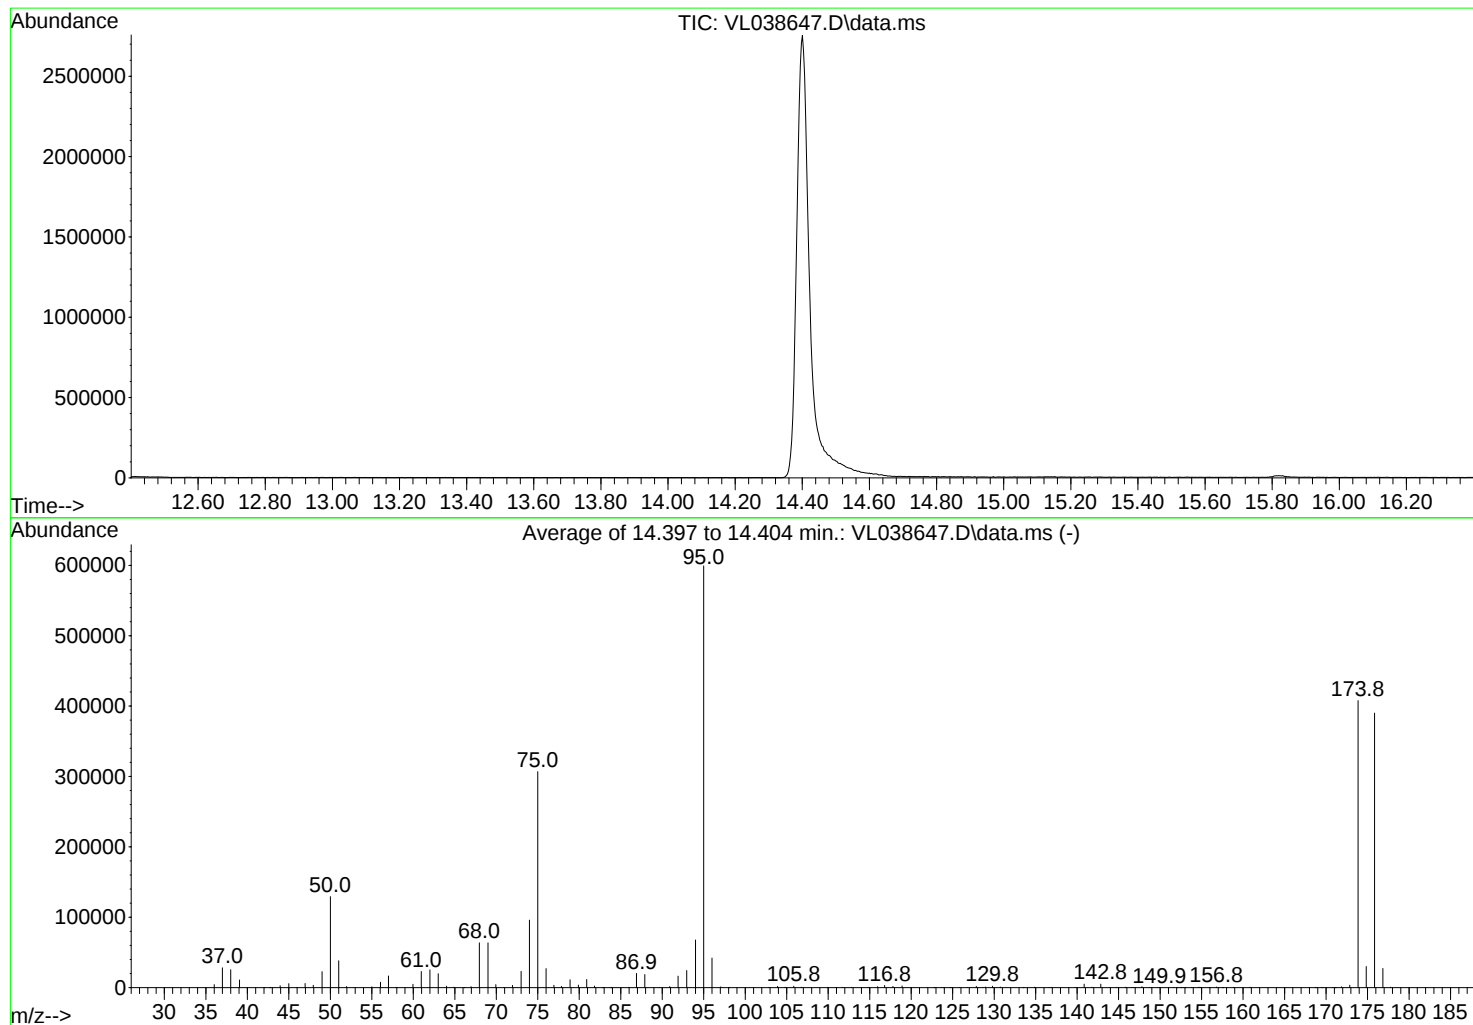

AutoFind: Scans 3611, 3612, 3613; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.6	129344	PASS
75	95	30	66	51.2	306923	PASS
95	95	100	100	100.0	599296	PASS
96	95	5	9	7.0	41957	PASS
173	174	0.00	2	0.9	3546	PASS
174	95	50	120	68.0	407744	PASS
175	174	4	9	7.4	30037	PASS
176	174	93	101	95.7	390059	PASS
177	176	5	9	7.0	27288	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	4375	46.95	5957	58.05	404	69.95	437
37.00	28195	47.95	3464	59.95	4810	70.90	20
38.00	25387	49.00	22859	60.95	22896	71.95	312
39.05	10989	50.00	129344	62.00	25211	73.00	2330
40.00	282	51.00	38315	63.00	19893	74.00	95925
42.00	52	51.95	1650	64.00	2086	75.00	306923
42.70	109	52.85	208	64.90	792	76.00	27187
43.00	152	55.00	1252	66.10	100	76.95	3347
43.95	2770	56.05	7707	66.95	1359	77.85	1850
45.00	5686	57.00	16559	67.95	63709	78.90	11252
45.95	321	57.90	237	69.00	63760	79.90	3646

Average of 14.397 to 14.404 min.: VL038647.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.90	11636	92.95	24427	109.95	410	123.60	172
81.85	2338	94.00	67672	110.95	299	123.90	83
82.80	96	95.00	599296	111.75	409	124.70	123
83.05	332	96.00	41957	112.80	370	125.85	283
83.80	94	97.05	1235	114.80	567	126.75	261
85.95	493	98.00	50	115.95	1498	127.85	1787
86.90	20227	102.85	333	116.80	3107	128.65	451
87.90	18691	103.90	1830	117.80	1892	128.95	838
89.65	132	104.80	646	118.90	2602	129.80	1959
90.90	1518	105.85	2123	119.95	195	130.75	849
91.90	16362	106.75	669	122.75	120	133.50	113

Average of 14.397 to 14.404 min.: VL038647.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
134.85	790	146.60	165	152.80	277	169.50	75
136.60	196	146.80	179	153.00	73	170.00	287
136.85	522	147.00	132	153.85	197	170.80	203
139.85	359	147.80	1400	154.70	779	171.10	106
140.85	4898	148.70	229	154.90	431	171.85	1104
141.80	734	148.90	114	155.90	91	172.85	3546
142.85	4951	149.70	144	156.80	945	173.85	407744
143.95	258	149.95	325	157.50	61	174.85	30037
144.70	395	151.65	337	158.85	514	175.85	390059
145.80	606	152.00	82	160.85	790	176.85	27288
146.00	280	152.50	67	168.70	70	177.80	610