


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032222\
 Data File : VL038681.D
 Acq On : 22 Mar 2022 11:51
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL032122AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Mar 21 17:09:26 2022
 Last Update : Mon Mar 21 17:09:26 2022

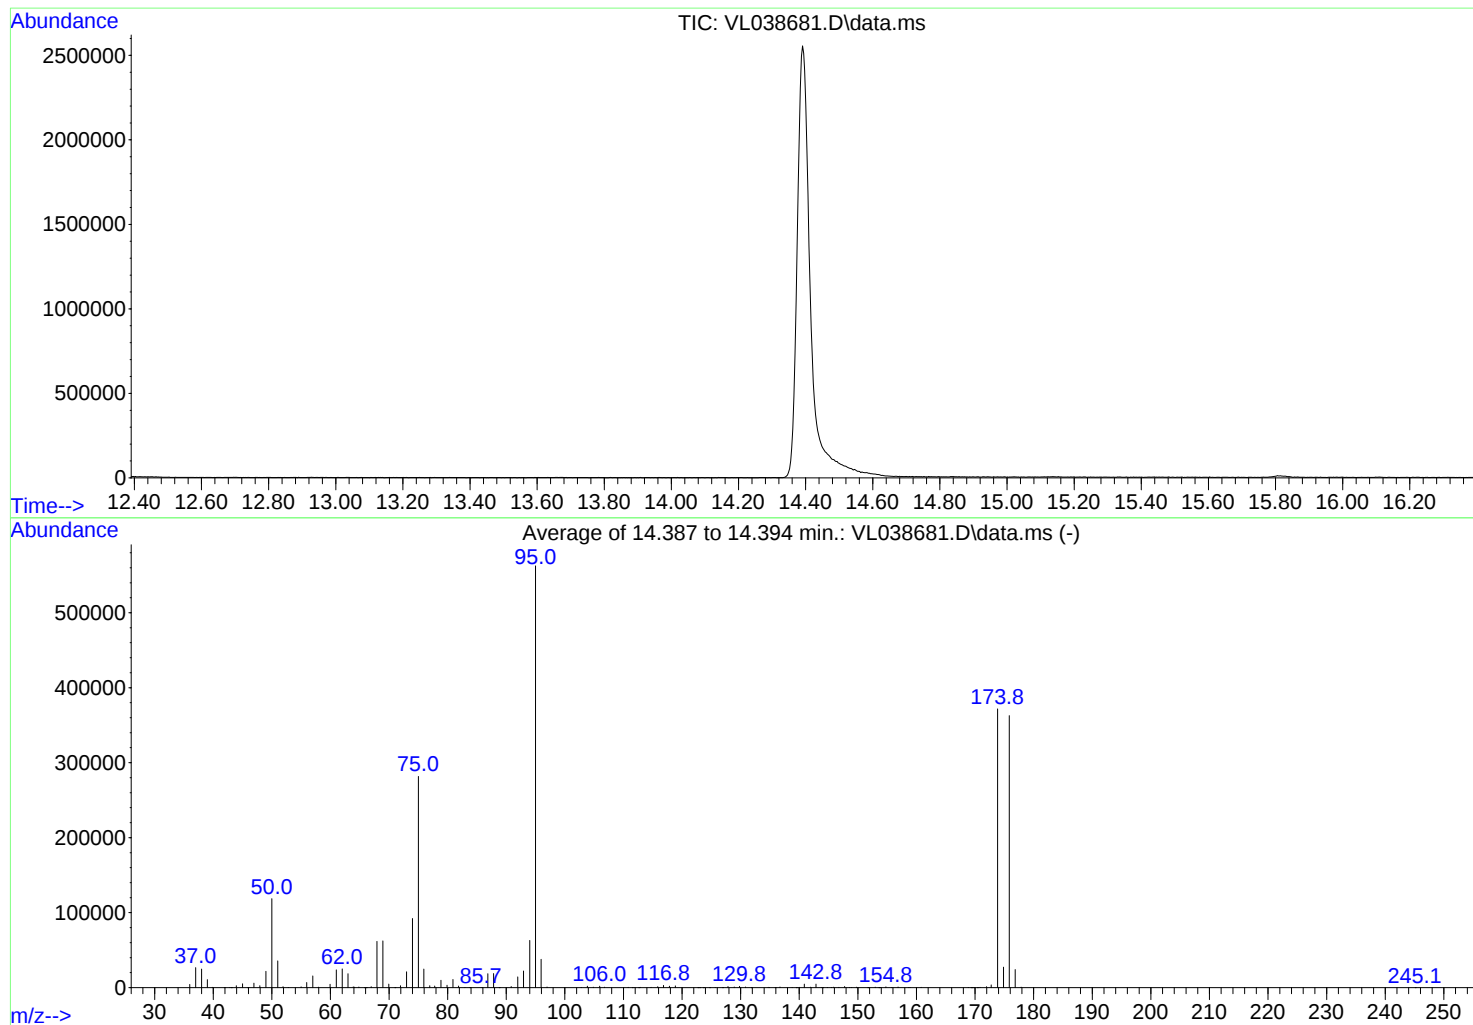

AutoFind: Scans 3608, 3609, 3610; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.1	118776	PASS
75	95	30	66	50.1	281749	PASS
95	95	100	100	100.0	562581	PASS
96	95	5	9	6.7	37744	PASS
173	174	0.00	2	1.0	3682	PASS
174	95	50	120	66.1	371691	PASS
175	174	4	9	7.3	27288	PASS
176	174	93	101	97.6	362731	PASS
177	176	5	9	6.7	24157	PASS

Average of 14.387 to 14.394 min.: VL038681.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	4376	46.05	210	57.95	711	67.95	6162
37.00	26603	46.95	6052	59.95	4405	68.95	6239
38.00	24819	47.95	2619	61.00	23648	69.95	477
39.00	10665	49.00	21840	62.00	24931	71.00	9
39.85	418	50.00	118776	63.00	18531	71.95	2635
41.90	62	51.00	35699	63.90	1127	73.00	21077
42.85	158	51.90	1287	64.10	641	74.00	92315
43.10	63	52.80	271	64.85	965	75.00	281749
43.95	2676	55.00	1132	65.80	84	75.95	24851
45.00	5123	55.95	6778	66.10	72	76.95	2586
45.90	112	57.00	15709	66.95	1239	77.80	2078

Average of 14.387 to 14.394 min.: VL038681.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.85	9907	90.85	1501	106.75	550	118.85	2303
79.90	3142	91.95	14253	110.05	155	122.70	80
80.90	10990	92.95	22184	110.80	363	123.00	101
81.85	2083	94.00	63011	111.50	62	123.60	96
82.95	292	95.00	562581	111.95	333	123.80	158
83.80	53	95.95	37744	112.60	110	124.70	79
85.70	173	96.95	965	112.85	355	125.65	231
85.95	346	102.80	179	114.70	355	126.90	86
86.85	18624	103.85	1841	115.85	1350	127.85	1491
87.85	18723	104.85	748	116.85	3086	128.90	941
88.80	101	105.95	1972	117.85	1947	129.80	1772

Average of 14.387 to 14.394 min.: VL038681.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
130.85	900	142.85	4694	151.70	59	168.85	166
131.80	81	143.75	189	151.85	232	169.30	63
134.70	352	144.00	93	152.95	544	169.50	99
134.90	342	144.80	332	153.60	100	169.80	96
135.90	74	145.50	134	153.85	191	170.40	106
136.70	810	145.90	602	154.80	1169	170.85	407
138.80	154	146.75	378	155.80	157	171.95	1272
139.50	99	147.75	1431	156.85	987	172.75	3682
140.00	391	148.60	223	158.70	307	173.85	371691
140.85	4658	148.95	226	158.90	234	174.85	27288
141.95	578	149.80	590	160.80	439	175.85	362731

Average of 14.387 to 14.394 min.: VL038681.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.85	24157						
177.85	652						
245.10	75						