
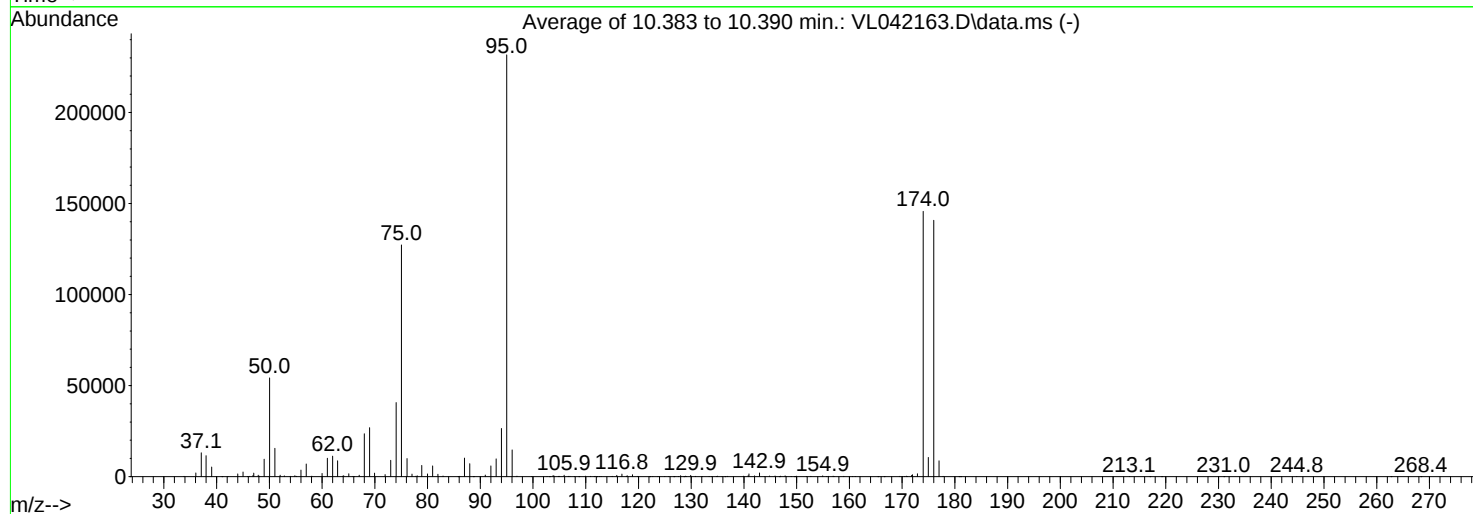


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032525\
Data File : VL042163.D
Acq On : 25 Mar 2025 08:15
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032525AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed Mar 26 02:13:42 2025

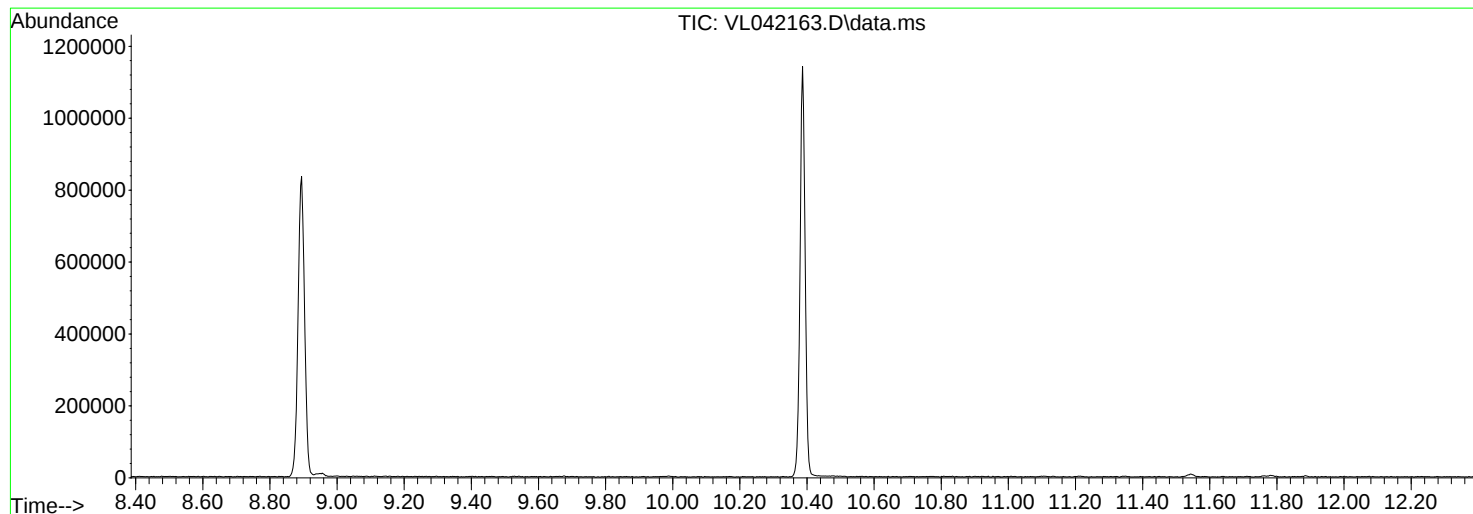

AutoFind: Scans 3181, 3182, 3183; Background Corrected with Scan 3168

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.4	54264	PASS
75	95	30	66	54.9	127272	PASS
95	95	100	100	100.0	231659	PASS
96	95	5	9	6.3	14669	PASS
173	174	0.00	2	1.1	1597	PASS
174	95	50	120	62.9	145720	PASS
175	174	4	9	7.2	10551	PASS
176	174	93	101	96.6	140749	PASS
177	176	5	9	6.2	8742	PASS

Average of 10.383 to 10.390 min.: VL042163.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.80	220	46.90	659	55.10	146	65.85	221
36.05	2047	47.05	1958	56.00	3614	66.10	81
37.10	13105	47.90	754	57.00	6926	67.05	83
38.00	11530	48.10	256	58.05	240	68.00	2358
39.05	5315	49.00	9594	60.00	1756	69.00	26861
41.00	44	50.05	54264	61.00	10101	69.95	1911
42.15	88	51.05	15524	62.00	11259	71.95	1124
44.00	1501	52.05	758	62.95	8724	73.00	8936
45.00	2538	52.85	450	63.90	279	74.05	40656
45.85	133	53.95	148	64.10	549	75.05	127272
46.20	184	54.85	556	65.05	1562	76.10	9981

Average of 10.383 to 10.390 min.: VL042163.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.05	1410	88.00	7103	103.10	33	110.90	216
77.80	284	88.70	29	103.80	610	111.60	59
78.05	463	90.95	922	104.00	377	111.75	174
78.90	6188	92.00	5930	104.80	179	112.10	42
80.00	1505	93.00	9739	105.00	214	112.60	50
80.95	5895	94.00	26496	105.90	819	112.90	109
81.95	1315	95.00	231659	106.70	184	115.00	218
82.95	343	96.05	14669	107.00	163	115.90	751
85.80	46	96.95	299	107.85	99	116.85	1449
86.10	206	99.75	49	108.70	17	117.70	225
87.00	10222	102.65	84	109.95	256	117.90	434

Average of 10.383 to 10.390 min.: VL042163.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.85	1026	128.00	562	135.85	74	146.70	37
119.90	148	128.60	47	136.40	23	146.95	227
122.10	17	128.90	267	136.90	204	147.80	430
122.70	62	129.10	60	139.90	251	148.00	132
123.70	71	129.90	721	140.80	513	148.95	110
123.95	63	130.80	177	140.95	1514	149.60	28
125.00	48	132.10	60	142.00	441	149.95	254
125.75	51	133.40	49	142.95	2028	151.85	72
126.70	23	133.90	54	143.95	110	152.70	161
126.90	66	134.80	123	144.85	330	154.95	481
127.60	130	135.00	262	145.90	365	155.70	61

Average of 10.383 to 10.390 min.: VL042163.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.00	185	170.80	234	181.10	19		
156.90	225	171.00	77	213.10	57		
157.10	96	171.80	703	217.00	20		
158.95	213	171.95	1032	219.20	24		
160.60	59	172.90	1597	231.00	18		
161.10	102	174.00	145720	244.85	53		
165.40	29	174.95	10551	262.70	18		
166.60	44	176.00	140749	268.40	46		
169.55	175	177.00	8742				
170.05	121	177.75	149				
170.50	82	180.80	20				