


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL032822\
 Data File : VL038766.D
 Acq On : 28 Mar 2022 8:41
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL032122AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Mar 21 17:09:26 2022
 Last Update : Mon Mar 21 17:09:26 2022

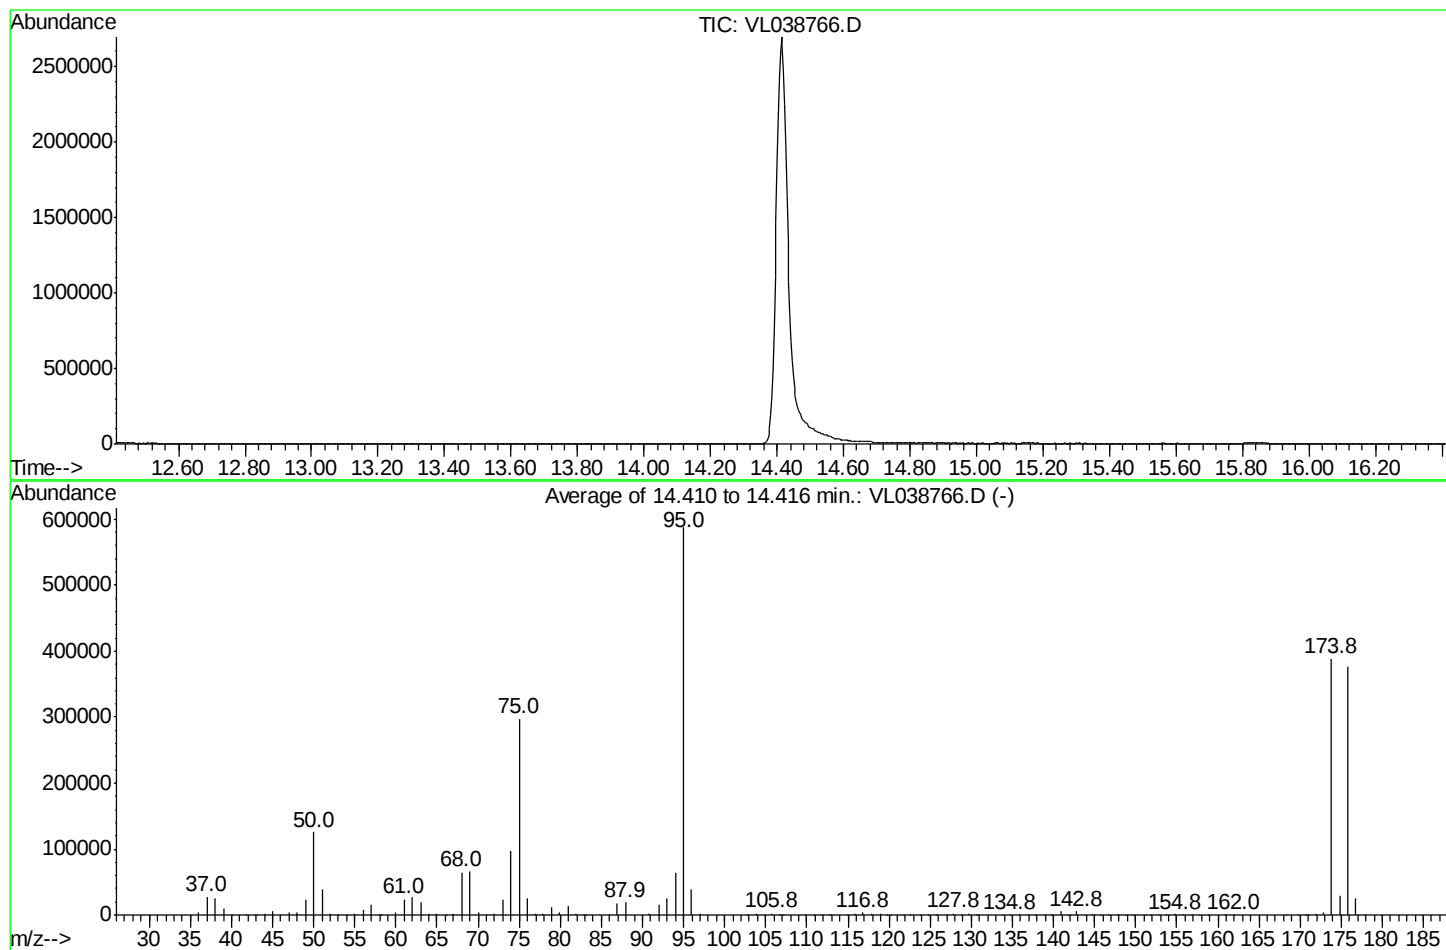

AutoFind: Scans 3615, 3616, 3617; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.4	125802	PASS
75	95	30	66	50.6	297642	PASS
95	95	100	100	100.0	587776	PASS
96	95	5	9	6.5	37981	PASS
173	174	0.00	2	0.9	3501	PASS
174	95	50	120	66.0	388202	PASS
175	174	4	9	7.4	28592	PASS
176	174	93	101	97.1	376960	PASS
177	176	5	9	6.6	24848	PASS