

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL033022\
Data File : VL038808.D
Acq On : 31 Mar 2022 9:06
Operator : SY/AP
Sample : QC033022 CAN 10320
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC033022 CAN 10320

Quant Time: Apr 01 05:16:04 2022
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL032122AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Mar 21 17:09:26 2022
QLast Update : Mon Mar 21 17:09:26 2022
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.68	49	785002	10.00	ppbv	0.02
33) 1,4-Difluorobenzene	7.19	114	2257313	10.00	ppbv	0.02
55) Chlorobenzene-d5	12.10	117	1909949	10.00	ppbv	0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.43	95	1378961	9.42	ppbv	0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	94.20%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL033022\
Data File : VL038808.D
Acq On : 31 Mar 2022 9:06
Operator : SY/AP
Sample : OC033022 CAN 10320
Misc : 400mL/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC033022 CAN 10320





Quant Time: Apr 01 05:16:04 2022
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL032122AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Mon Mar 21 17:09:26 2022
QLast Update : Mon Mar 21 17:09:26 2022
Response via : Initial Calibration

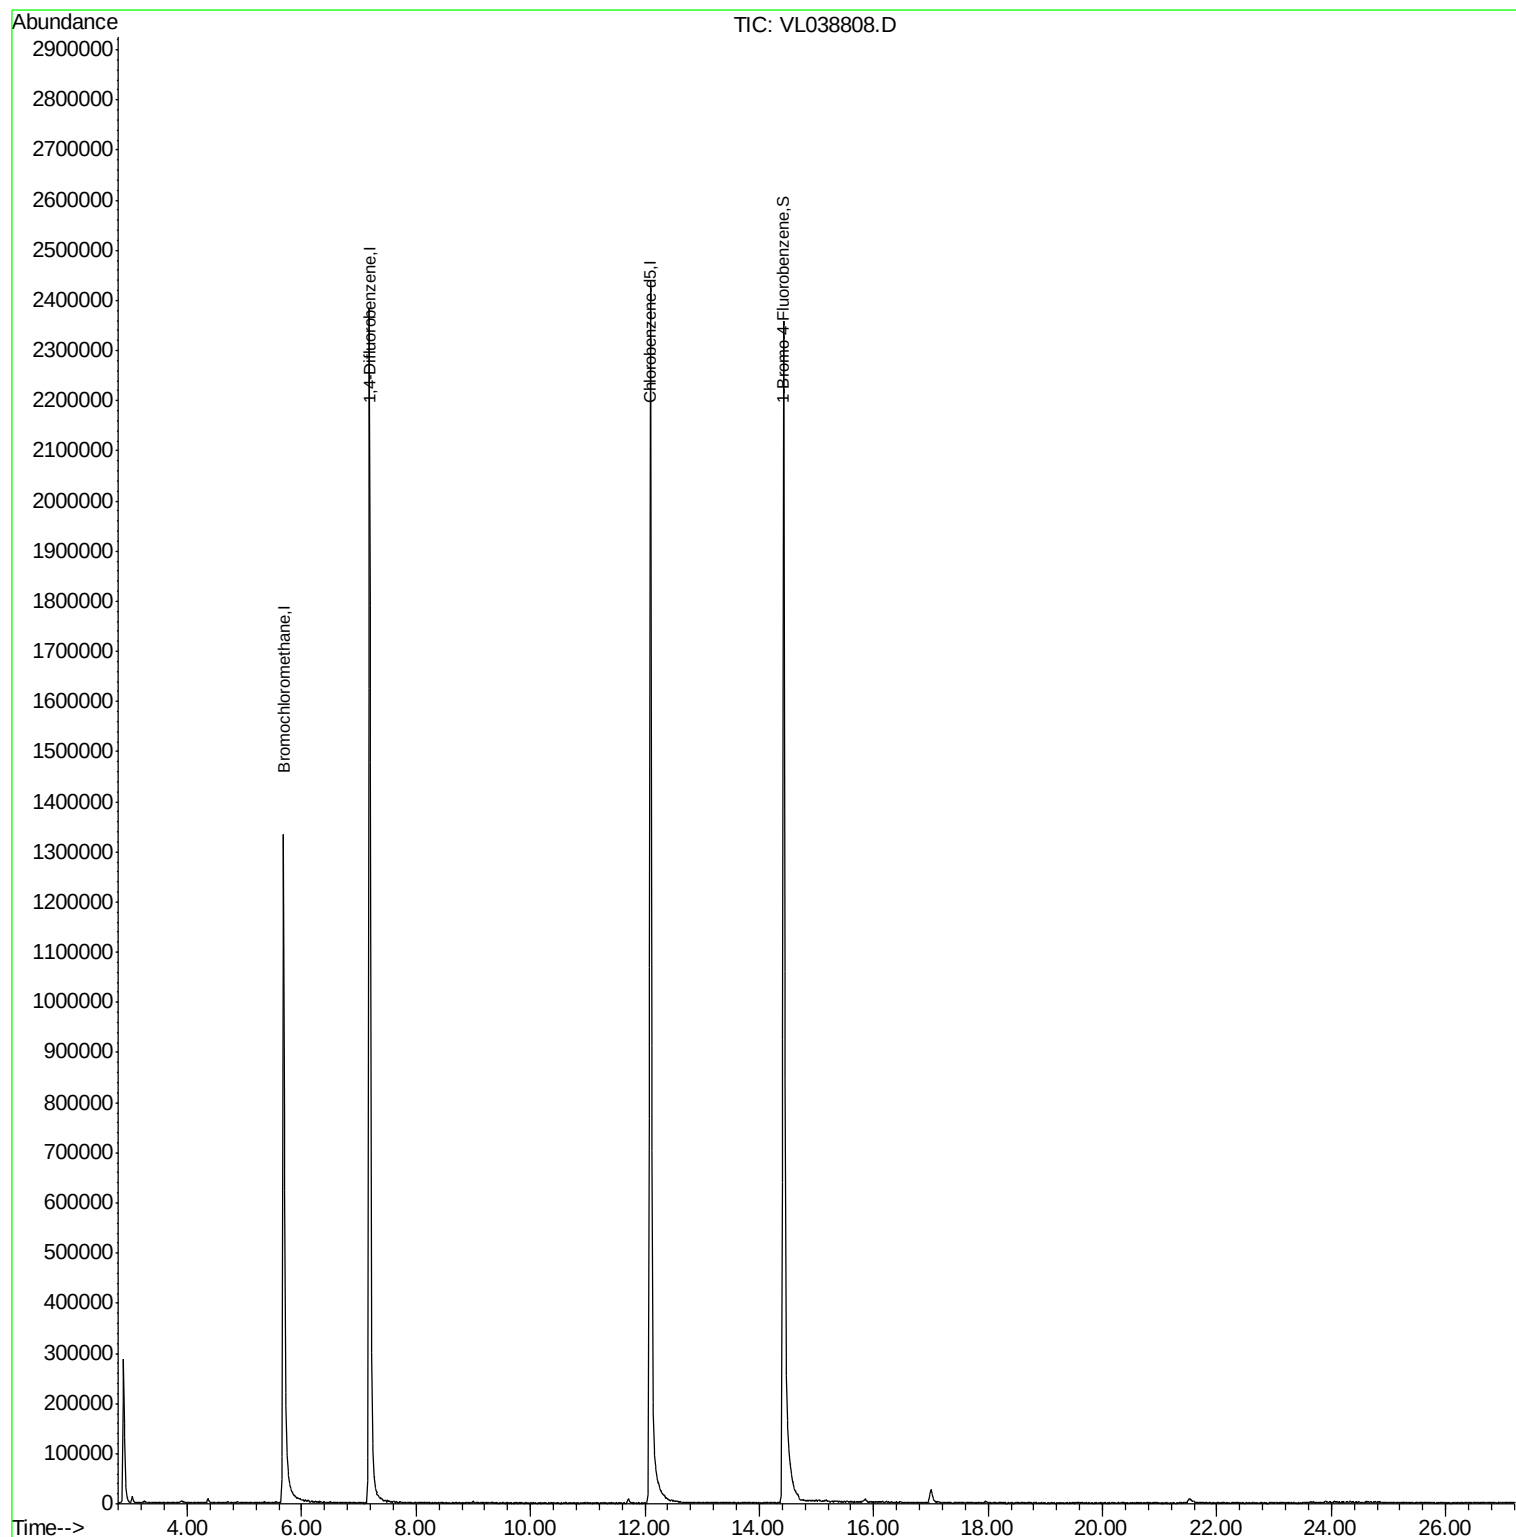

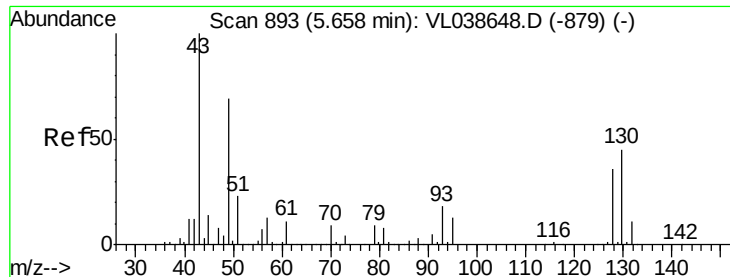




#1
 Bromochloromethane
 Concen: 10.000 ppbv
 RT: 5.68
 Instrument: MSVOA_1
 Delta R.T.:
 Lab File: ClientSampleId:
 OC033022 CAN 10320
 Acq: 31 Mar 2022 9:00


Tot Ion: 49 Resp: 785002
 Ion Ratio Lower Upper
 49 100
 128 58.6 26.2 78.6
 130 75.5 33.7 101.1

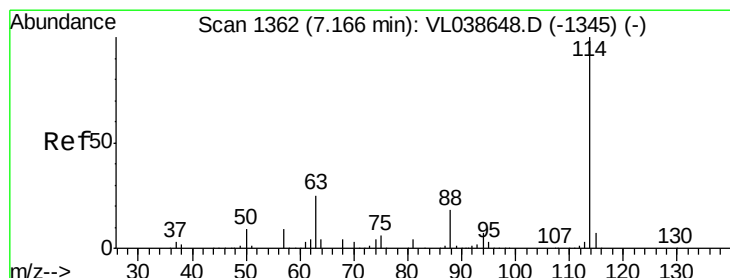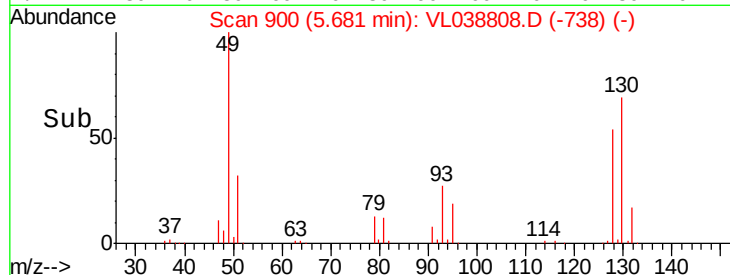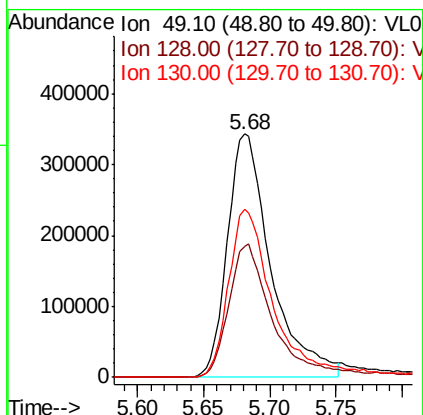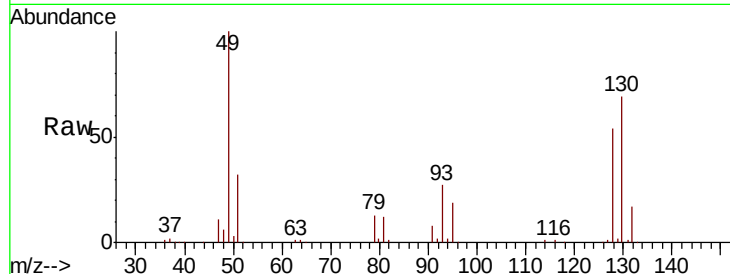

#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.19 min Scan# 1369
 Delta R.T.: 0.02 min
 Lab File: VL038808.D
 Acq: 31 Mar 2022 9:06





Tgt Ion:114 Resp: 2257313
 Ion Ratio Lower Upper
 114 100
 63 22.7 19.4 29.0
 88 16.6 13.9 20.9

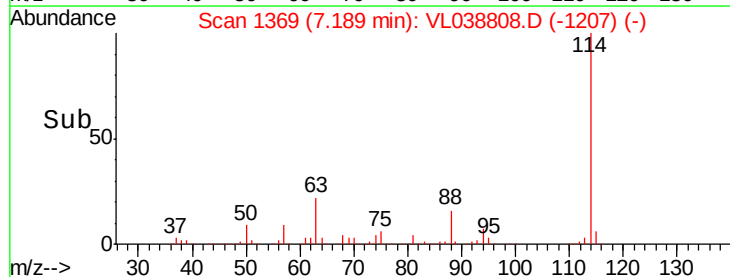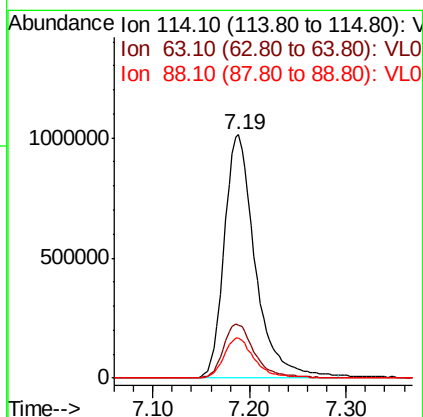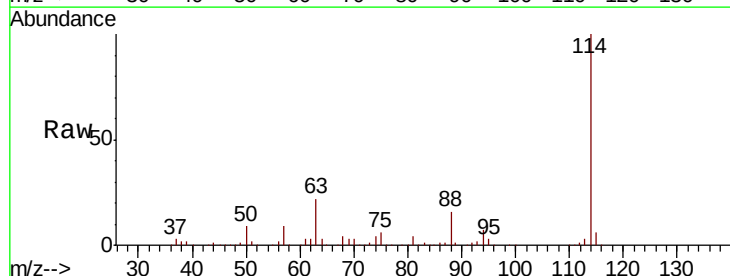

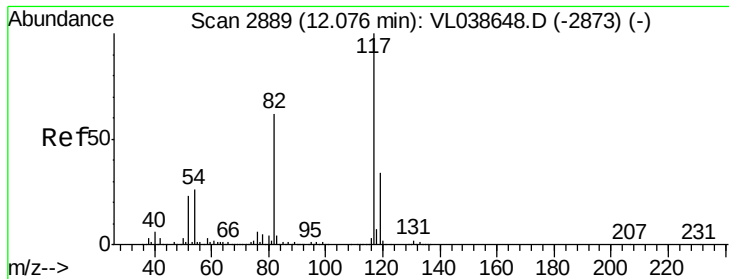

#55
 Chlorobenzene-d5
 Concen: 10.000 ppbv
 RT: 12.10 min
 Instrument: MSVOA_1
 Delta R.T.:
 Lab File: ClientSampleId :
 OC033022 CAN 10320
 Acq: 31 Mar 2022 9:00

Tot Ion:117 Resp: 1909949
 Ion Ratio Lower Upper
 117 100
 82 63.3 51.6 77.4
 119 33.8 26.9 40.3

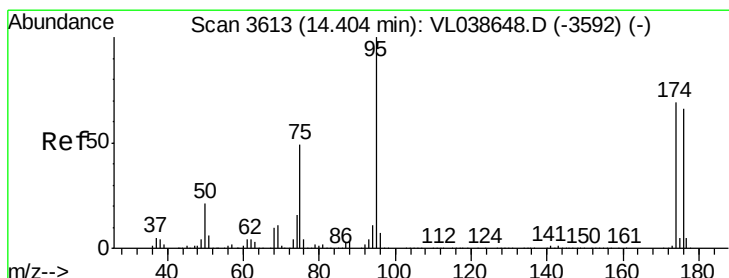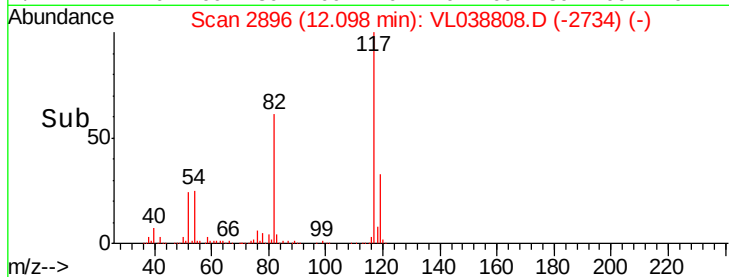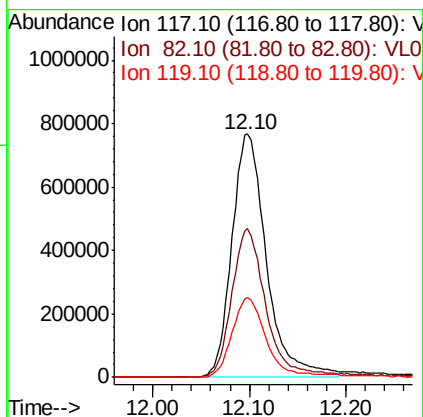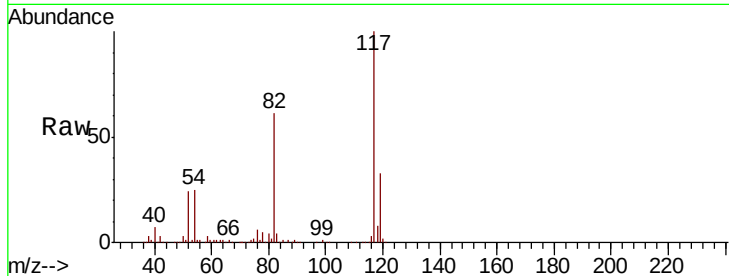

#68
 1-Bromo-4-Fluorobenzene
 Concen: 9.417 ppbv
 RT: 14.43 min Scan# 3620
 Delta R.T.: 0.02 min
 Lab File: VL038808.D
 Acq: 31 Mar 2022 9:06

Tgt Ion: 95 Resp: 1378961
 Ion Ratio Lower Upper
 95 100
 174 75.1 56.1 84.1
 175 5.4 4.2 6.2

