
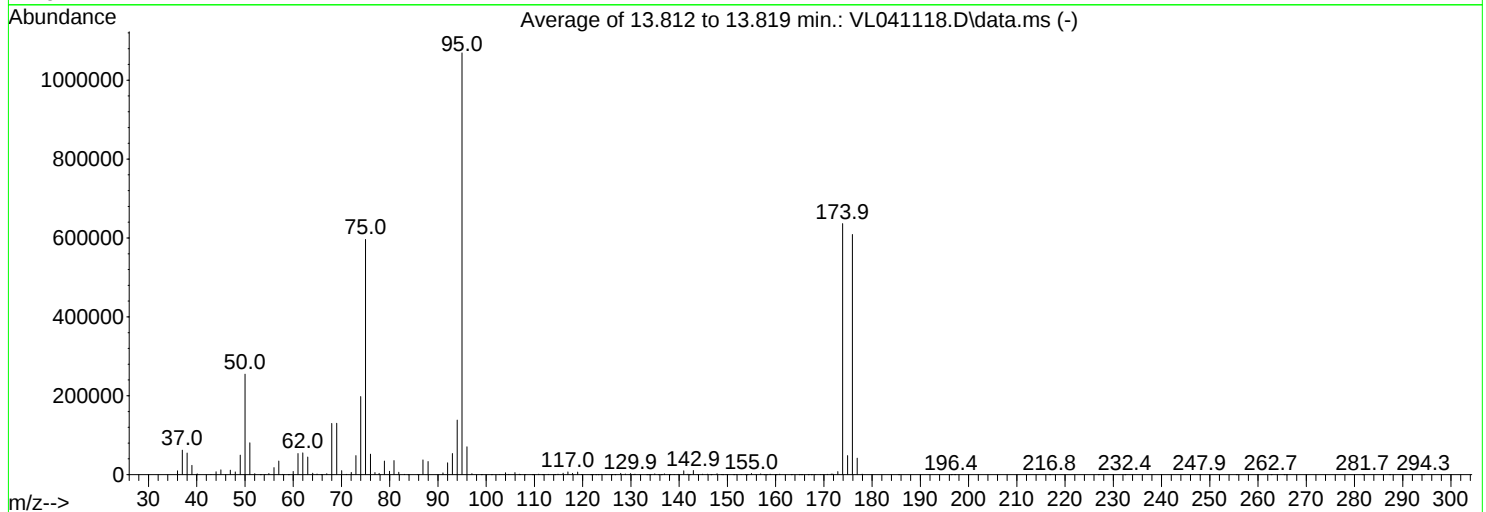


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040424\
Data File : VL041118.D
Acq On : 4 Apr 2024 8:09
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL040424AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Apr 05 04:49:46 2024

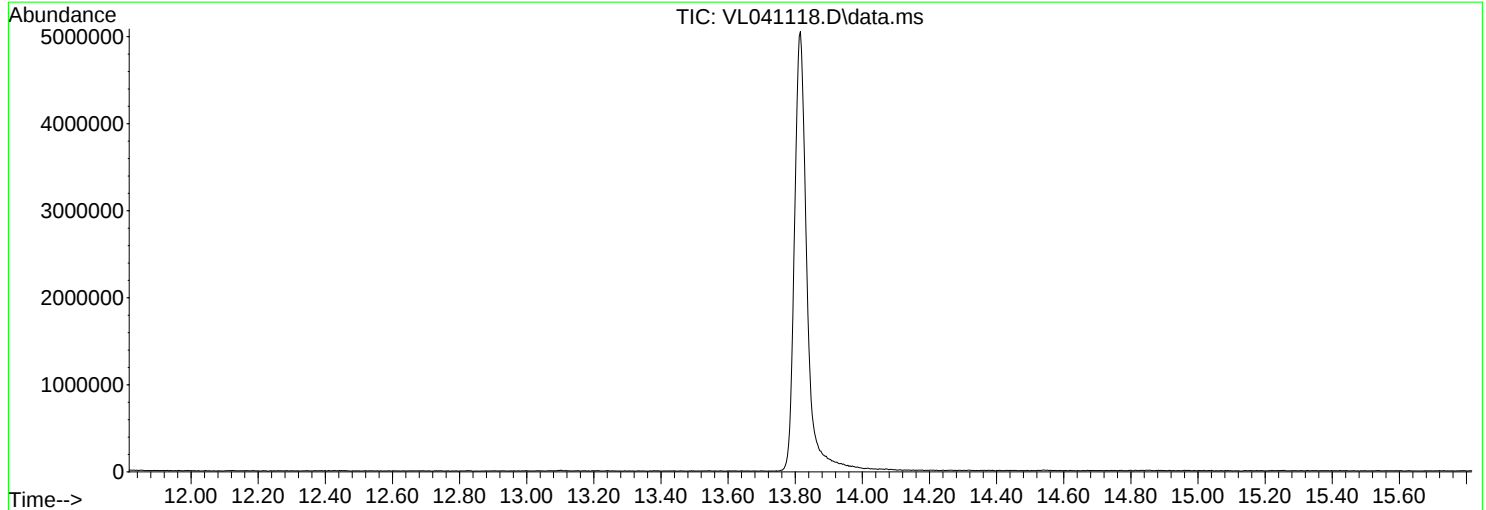

AutoFind: Scans 3486, 3487, 3488; Background Corrected with Scan 3462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.8	254912	PASS
75	95	30	66	55.8	596416	PASS
95	95	100	100	100.0	1069397	PASS
96	95	5	9	6.6	70461	PASS
173	174	0.00	2	1.2	7830	PASS
174	95	50	120	59.5	636608	PASS
175	174	4	9	7.6	48427	PASS
176	174	93	101	95.7	608981	PASS
177	176	5	9	6.8	41640	PASS

Average of 13.812 to 13.819 min.: VL041118.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	9731	48.00	6935	58.10	572	69.00	13039
37.00	62080	49.00	49571	59.00	106	70.05	1017
38.00	54960	50.00	254912	60.00	7947	71.00	70
39.00	23736	51.00	80813	61.00	53579	72.05	562
39.90	227	52.05	2668	62.00	55128	73.00	48213
40.10	1902	53.20	60	63.00	44787	74.00	197995
42.95	599	54.15	319	64.05	3875	75.00	596416
44.00	7191	54.95	3016	64.95	1530	76.00	51891
45.00	12148	56.00	17779	65.80	74	76.95	5495
45.95	454	57.00	34669	66.95	2612	77.80	3248
46.95	11395	57.85	660	68.00	130019	78.90	34437

Average of 13.812 to 13.819 min.: VL041118.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.95	8499	93.00	53456	106.85	1137	115.95	3695
80.90	35539	94.00	138411	107.10	372	116.95	6757
81.90	6305	95.00	1.0694e+006	107.95	221	117.90	3441
83.05	920	96.00	70461	109.60	156	118.95	6377
83.80	55	97.05	2358	109.90	615	119.80	364
85.80	490	99.00	64	110.90	1112	121.70	89
86.10	490	101.10	76	111.70	212	122.00	96
86.90	37499	102.75	523	112.00	453	122.70	85
87.95	33160	104.00	5110	112.85	875	123.20	69
91.05	4448	104.70	941	114.20	106	123.85	962
92.00	30003	105.95	5491	114.90	1337	124.85	470

Average of 13.812 to 13.819 min.: VL041118.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.00	106	134.00	103	142.95	10631	151.30	50
126.70	223	134.95	1935	143.90	592	151.85	418
127.90	3181	135.70	250	144.85	1311	152.85	447
128.85	1784	136.30	157	145.90	1165	153.75	543
129.80	1008	136.95	1869	146.60	118	154.10	185
129.95	2805	138.05	237	146.75	462	155.00	2923
130.60	303	138.95	261	147.85	2507	155.95	360
130.85	1315	139.80	757	148.80	316	156.90	1893
131.90	271	140.95	9943	149.00	157	157.60	88
133.30	57	141.80	1279	149.70	504	158.10	247
133.70	165	142.10	222	150.05	623	158.85	1325

Average of 13.812 to 13.819 min.: VL041118.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.10	123	171.55	1568	216.80	63	294.30	94
160.85	1390	171.85	1523	226.90	62		
163.25	113	172.90	7830	232.40	83		
164.90	61	173.90	636608	247.90	50		
165.35	115	174.90	48427	255.50	54		
166.75	111	175.90	608981	262.70	59		
167.40	60	176.90	41640	265.40	54		
168.20	326	177.95	1388	265.90	51		
169.35	314	185.50	51	281.70	61		
169.85	314	196.40	217	287.30	60		
170.75	809	197.10	70	293.80	77		