


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040522\
 Data File : VL038811.D
 Acq On : 5 Apr 2022 14:39
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL040522AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Apr 06 06:12:53 2022
 Last Update : Wed Apr 06 06:12:53 2022

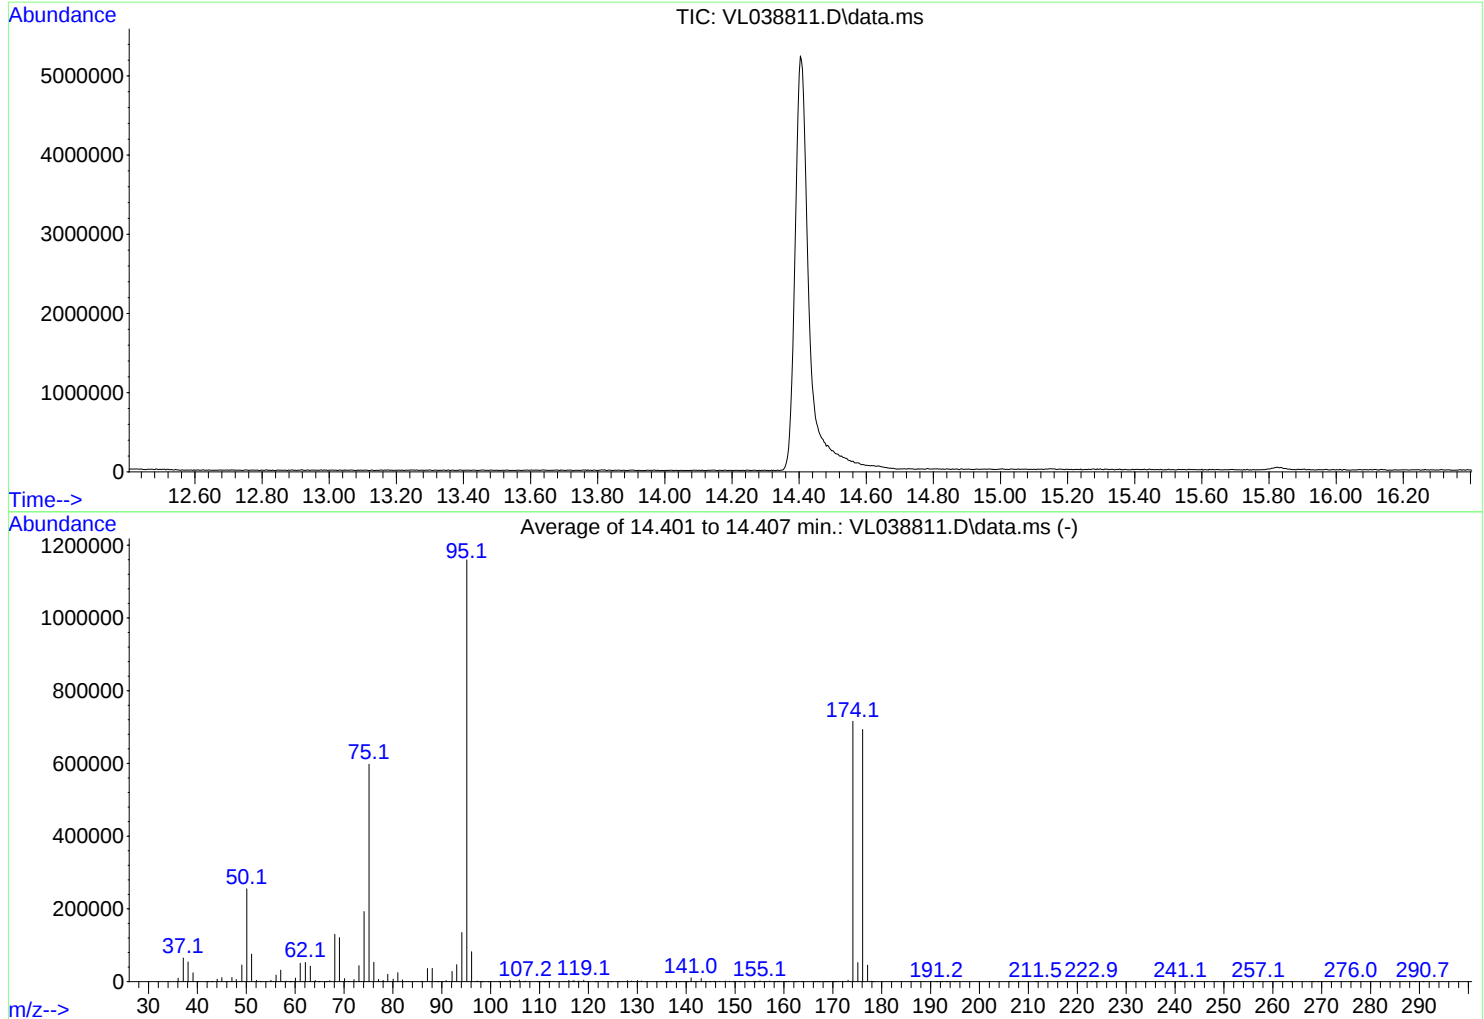

AutoFind: Scans 3612, 3613, 3614; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.0	255147	PASS
75	95	30	66	51.6	598037	PASS
95	95	100	100	100.0	1159851	PASS
96	95	5	9	7.1	82237	PASS
173	174	0.00	2	0.6	4184	PASS
174	95	50	120	61.7	715669	PASS
175	174	4	9	7.3	52448	PASS
176	174	93	101	96.9	693269	PASS
177	176	5	9	6.5	45267	PASS

Average of 14.401 to 14.407 min.: VL038811.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	9654	46.20	355	58.15	1407	67.10	270
37.10	65091	47.05	11383	58.90	252	68.10	13005
38.10	54205	47.95	5900	59.10	98	69.05	12122
39.10	24335	49.10	45781	60.05	9888	70.10	820
40.00	56	50.10	255147	61.05	50723	71.00	529
42.05	132	51.10	75651	62.10	53003	72.05	5605
42.90	12	52.10	3761	63.10	42912	73.05	44071
43.10	445	52.90	137	64.10	3133	74.10	192832
44.05	6800	55.05	3346	64.80	144	75.10	598037
45.00	11189	56.10	18120	65.05	521	76.10	53302
45.90	395	57.05	31648	66.30	170	77.05	6095

Average of 14.401 to 14.407 min.: VL038811.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.90	1786	88.80	595	97.80	133	109.70	251
78.10	2652	89.20	247	98.30	70	110.00	195
78.95	20259	90.20	488	99.50	86	110.65	310
80.05	7127	90.90	2988	101.70	58	111.00	247
81.00	24803	92.10	28405	102.90	406	111.20	205
81.95	5093	93.05	46621	103.95	3019	111.70	67
82.80	294	94.10	135211	104.75	176	111.95	263
83.25	624	95.10	1.15985e+006	105.10	638	112.20	257
85.95	1330	96.10	82237	105.85	4661	112.95	1008
87.05	36349	97.00	480	106.80	180	115.05	656
88.05	36360	97.25	2016	107.15	1185	116.00	3461

Average of 14.401 to 14.407 min.: VL038811.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.80	1669	125.05	470	135.00	658	140.20	208
117.05	3314	125.80	560	135.70	220	141.00	10595
117.85	1502	126.20	206	135.95	238	141.75	657
118.10	1540	127.05	256	136.80	382	142.10	357
119.05	4104	128.00	2836	137.05	1052	143.05	8317
119.90	200	128.85	2033	137.70	597	144.05	503
121.40	75	130.05	2907	138.55	153	144.80	234
123.00	313	130.90	1607	138.90	409	145.00	349
123.90	239	131.85	644	139.15	688	145.75	1321
124.15	380	133.90	83	139.60	327	146.90	828
124.60	96	134.75	642	139.90	306	147.80	398

Average of 14.401 to 14.407 min.: VL038811.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.05	1708	155.90	92	166.30	97	171.10	319
148.85	1063	156.30	770	166.80	125	172.00	799
149.70	94	157.10	2013	167.30	71	173.10	4184
150.05	813	158.10	100	167.55	403	174.10	715669
151.00	116	158.70	182	168.30	174	175.10	52448
151.95	594	159.15	843	168.75	599	176.10	693269
152.80	739	160.30	153	169.00	199	177.10	45267
153.80	467	160.95	744	169.30	258	177.95	1285
154.10	82	162.30	106	169.85	526	178.20	153
154.80	708	163.00	284	170.30	66	191.20	117
155.10	2435	163.65	198	170.70	314	192.30	106

Average of 14.401 to 14.407 min.: VL038811.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
193.20	56	257.10	111				
194.90	60	263.70	51				
206.00	78	268.20	103				
207.90	77	269.20	82				
211.50	83	276.00	127				
222.90	126	289.10	53				
223.70	59	290.70	185				

224.30	60
241.10	72
252.00	65
253.90	75

Instrument :
MSVOA_L
ClientSampleId :
BFB